
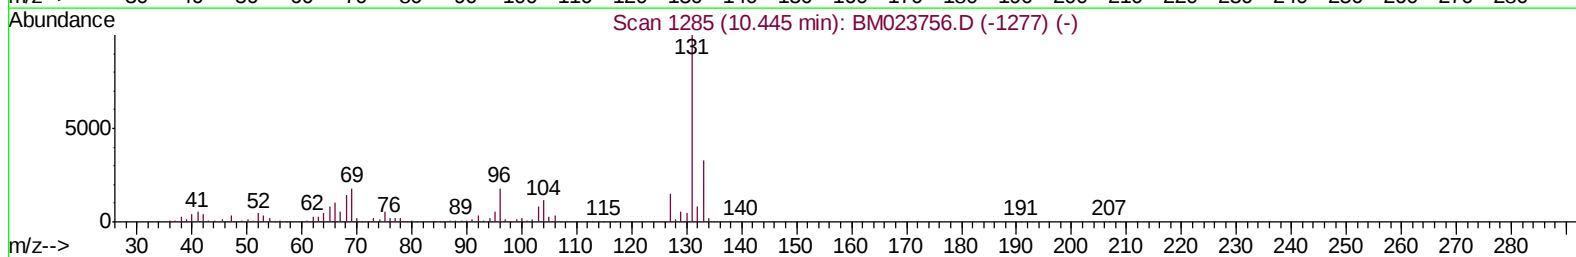
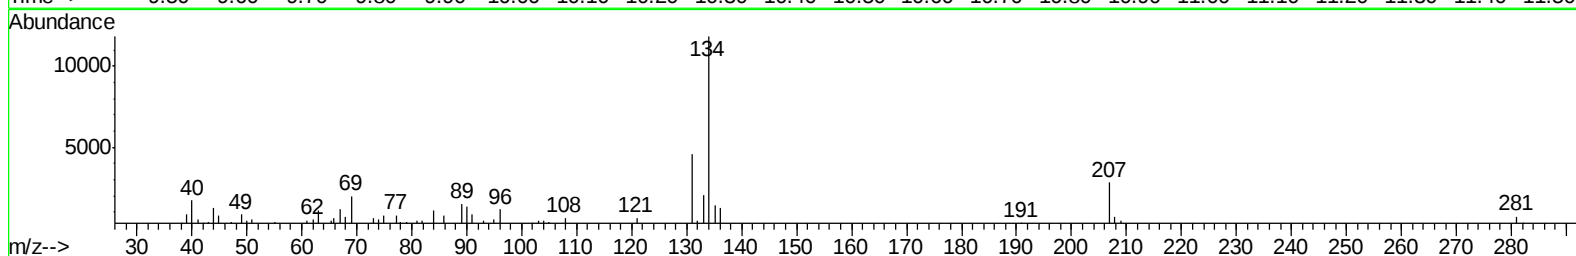


Data File : BM023763.D
Acq On : 15 Nov 2019 21:13
Operator : JU
Sample : K5699-02MS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Nov 16 03:21:12 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 16 03:18:12 2019
Response via : Initial Calibration

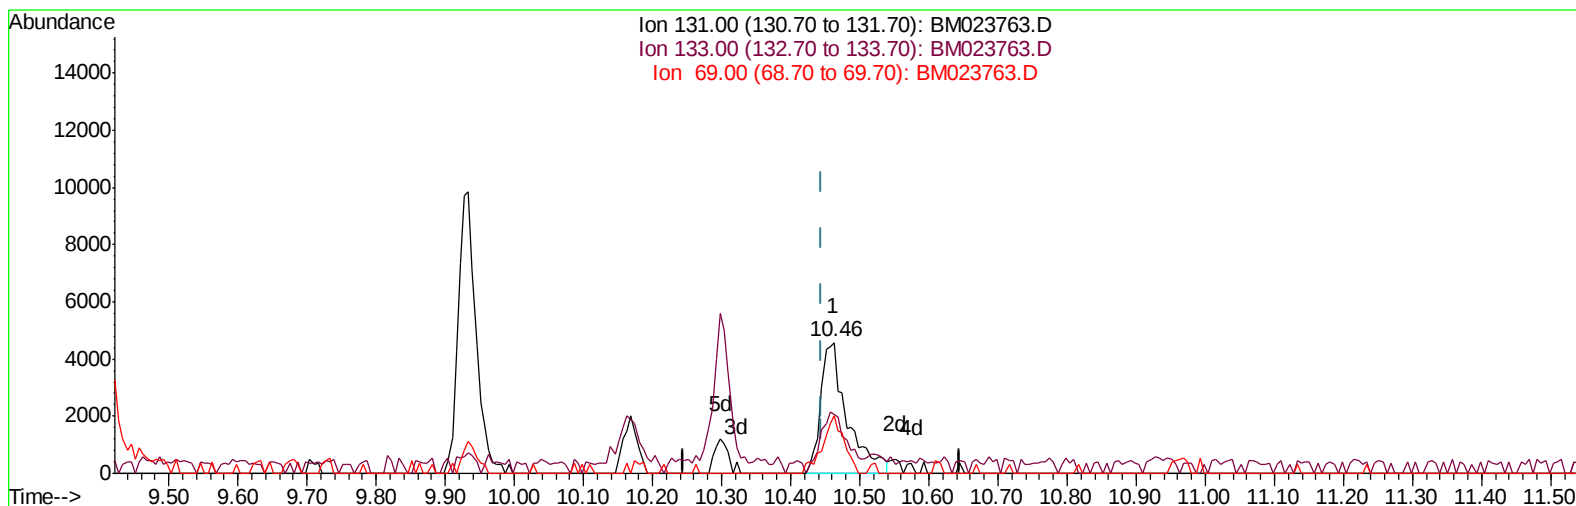

TIC: BM023763.D

(29) 4-Chloroaniline-d4 (S)

10.463min (+0.018) 0.56ng/ul m

response 12141

Ion	Exp%	Act%
131.00	100	100
133.00	32.50	45.24#
69.00	19.60	43.45#
0.00	0.00	0.00