

Data File : BM023720.D
Acq On : 14 Nov 2019 17:16
Operator : JU
Sample : K5678-08
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLM81

Quant Time: Nov 15 06:33:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 15 06:30:14 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	381923	20.00	ng/ul	0.00
18) Naphthalene-d8	10.30	136	1582973	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.19	164	983374	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.94	188	1992371	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	1920161	20.00	ng/ul	0.00
86) Perylene-d12	23.31	264	2296157	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.07	96	20738	2.24	ng/uL	0.00
5) Phenol-d5	6.72	99	521305	14.97	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.87	67	342498	17.12	ng/ul	0.00
9) 2-Chlorophenol-d4	7.07	132	458724	18.19	ng/ul	0.00
13) 4-Methylphenol-d8	8.25	113	473483	17.05	ng/ul	0.00
19) Nitrobenzene-d5	8.68	128	240766	21.25	ng/ul	0.00
22) 2-Nitrophenol-d4	9.40	143	276395	23.21	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.94	165	514221	18.94	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	12851	0.43	ng/ul	0.01
44) Dimethylphthalate-d6	13.61	166	1592746	20.77	ng/ul	0.00
47) Acenaphthylene-d8	13.87	160	1874199	21.42	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	98002	7.49	ng/ul	0.00
58) Fluorene-d10	15.19	176	1393333	20.58	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.32	200	187901	16.30	ng/ul	0.00
71) Anthracene-d10	17.04	188	1973141	20.88	ng/ul	0.00
79) Pyrene-d10	19.34	212	2168228	21.66	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	2537708	21.00	ng/ul	0.00

Target Compounds


					Qvalue	
4) Benzaldehyde	6.69	77	67965	3.328	ng/ul	93
6) Phenol	6.75	94	44637	1.245	ng/ul	98
14) Acetophenone	8.36	105	68178	1.574	ng/ul	99
45) Dimethylphthalate	13.66	163	277000	3.686	ng/ul	100
49) 3-Nitroaniline	14.06	138	19838	1.525	ng/ul#	7
76) Di-n-butylphthalate	17.93	149	445868	4.396	ng/ul	97
77) Fluoranthene	19.01	202	194988	1.658	ng/ul	97
80) Pyrene	19.37	202	206914	1.667	ng/ul	97
81) Butylbenzylphthalate	20.30	149	57179	1.455	ng/ul#	82
84) Bis(2-ethylhexyl)phthalate	21.09	149	779580	13.135	ng/ul	99
85) Chrysene	21.18	228	157292	1.319	ng/ul#	92
87) Di-n-octyl phthalate	21.96	149	160331	1.429	ng/ul	100
88) Benzo(b)fluoranthene	22.67	252	256981	1.756	ng/ul#	60
91) Benzo(a)pyrene	23.21	252	151072	1.127	ng/ul#	55
94) Benzo(g,h,i)perylene	26.11	276	127846	1.101	ng/ul#	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM023720.D
Acq On : 14 Nov 2019 17:16
Operator : JU
Sample : K5678-08
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLM81

Quant Time: Nov 15 06:33:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 15 06:30:14 2019
Response via : Initial Calibration

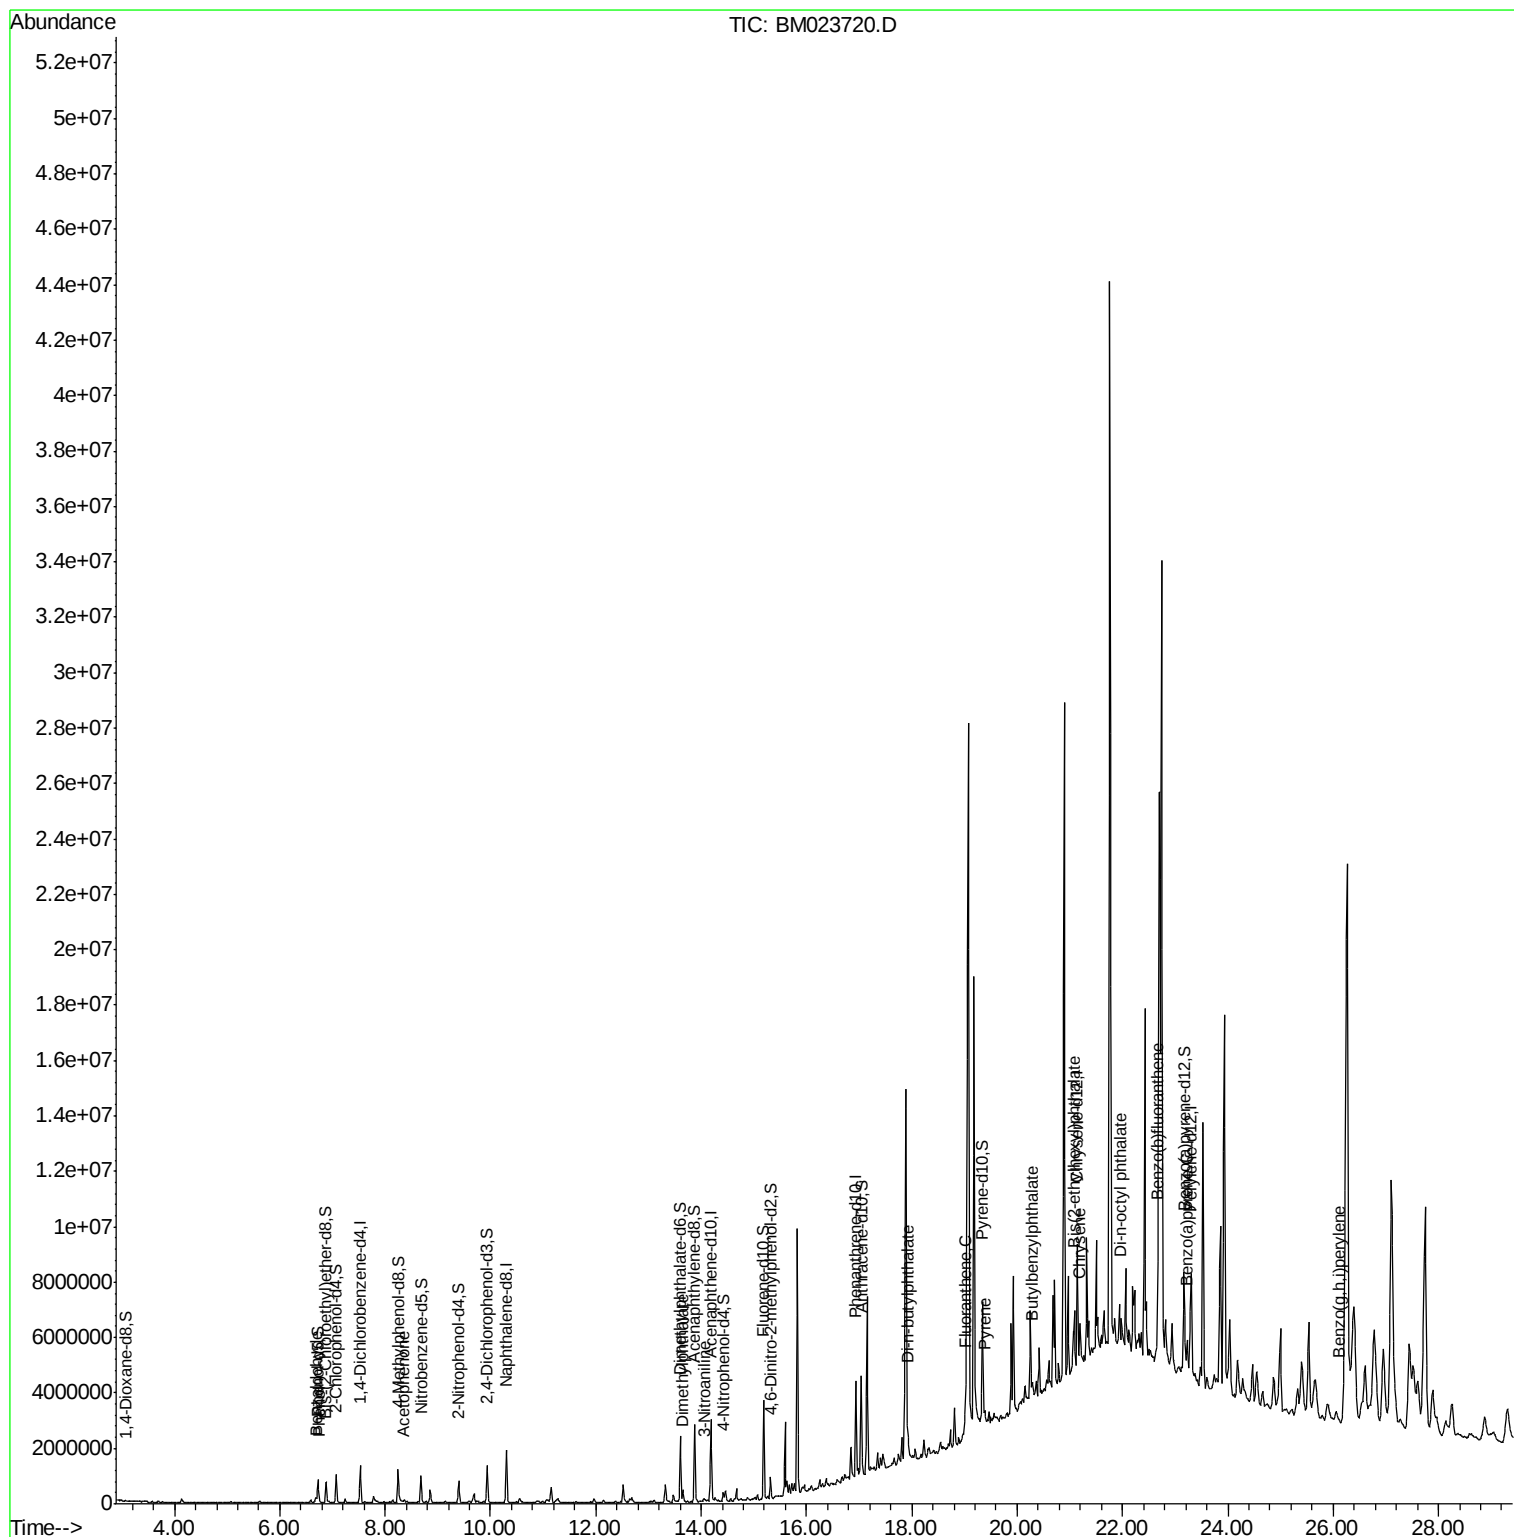

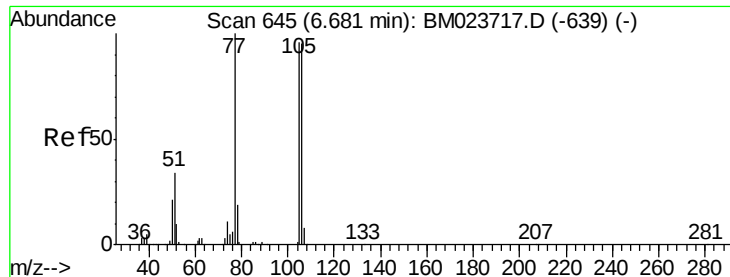

#4

Benzaldehyde

Concen: 3.328 ng/ul

RT: 6.69 min Scan# 646

Delta R.T. 0.01 min

Lab File: BM023720.D

Acq: 14 Nov 2019 17:16

Instrument :

BNA_M

ClientSampleId :

JLM81


Tgt Ion: 77 Resp: 67965

Ion Ratio Lower Upper

77 100

105 102.0 75.9 113.9




106 94.5 70.2 105.4

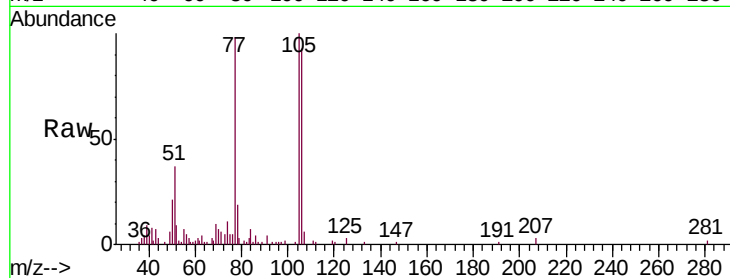

Abundance Ion 77.00 (76.70 to 77.70): BM023717.D (-639) (-)

Ion 105.00 (104.70 to 105.70): BM023717.D (-639) (-)

Ion 106.00 (105.70 to 106.70): BM023717.D (-639) (-)

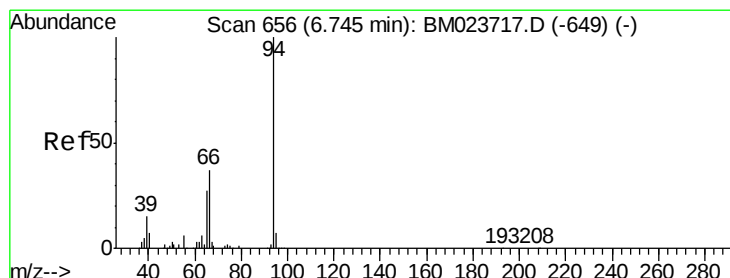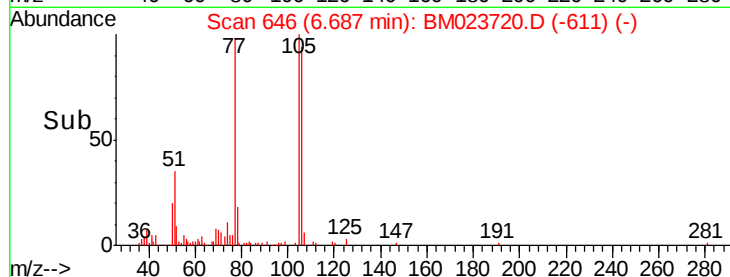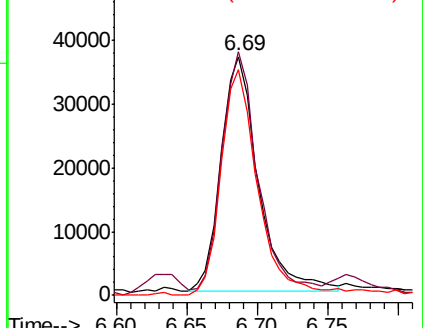

#6

Phenol

Concen: 1.245 ng/ul

RT: 6.75 min Scan# 657

Delta R.T. 0.01 min

Lab File: BM023720.D

Acq: 14 Nov 2019 17:16


Tgt Ion: 94 Resp: 44637

Ion Ratio Lower Upper

94 100

65 29.1 21.4 32.2



66 38.1 30.7 46.1

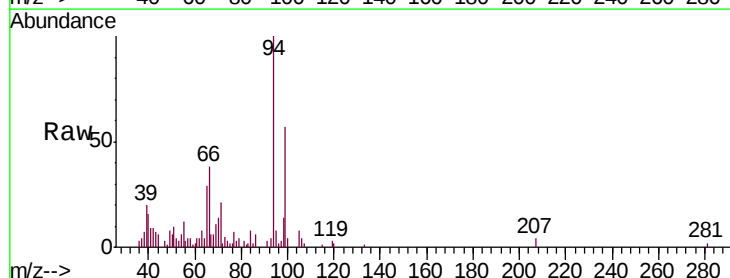


Abundance Ion 94.00 (93.70 to 94.70): BM023717.D (-649) (-)

Ion 65.00 (64.70 to 65.70): BM023717.D (-649) (-)

Ion 66.00 (65.70 to 66.70): BM023717.D (-649) (-)

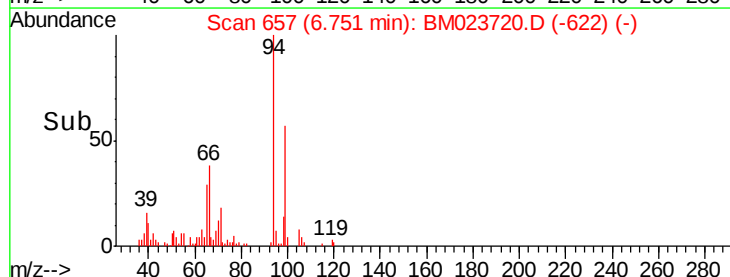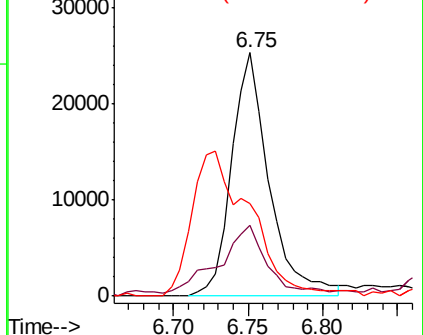

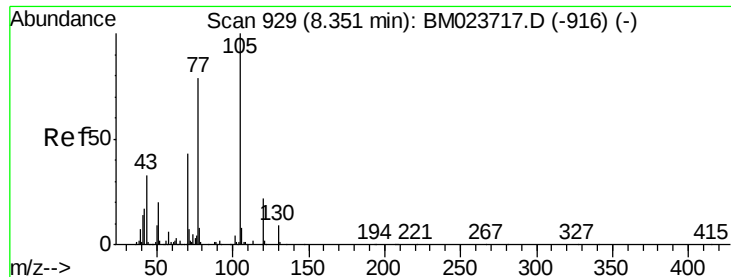

#14

Acetophenone

Concen: 1.574 ng/ul

RT: 8.36 min Scan# 930

Delta R.T. 0.01 min

Lab File: BM023720.D

Acq: 14 Nov 2019 17:16

Instrument :

BNA_M

ClientSampleId :

JLM81


Tgt Ion:105 Resp: 68178

Ion Ratio Lower Upper

105 100

77 79.6 63.8 95.6




51 22.7 16.3 24.5

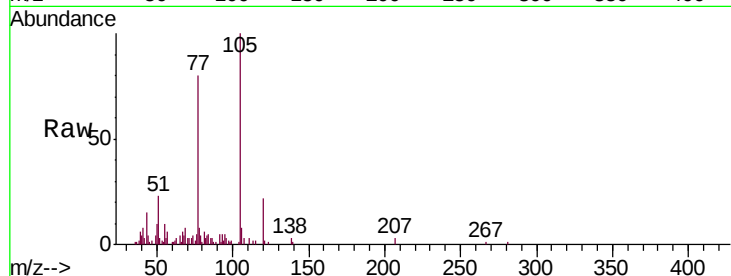

Abundance Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BM0

Ion 51.00 (50.70 to 51.70): BM0

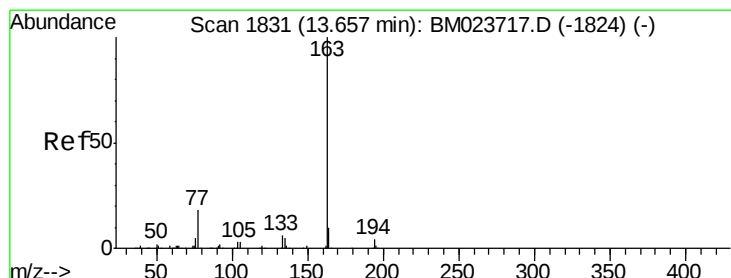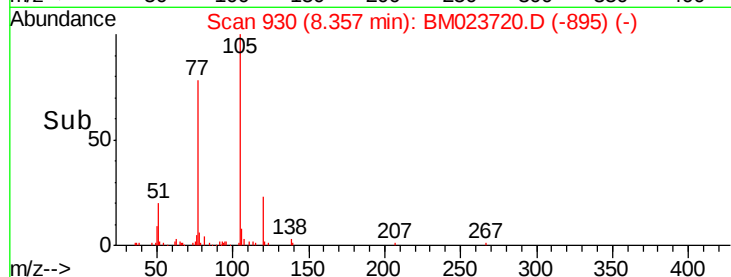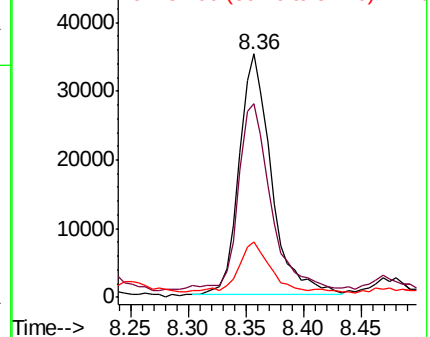

#45

Dimethylphthalate

Concen: 3.686 ng/ul

RT: 13.66 min Scan# 1831

Delta R.T. 0.00 min

Lab File: BM023720.D

Acq: 14 Nov 2019 17:16


Tgt Ion:163 Resp: 277000

Ion Ratio Lower Upper

163 100

194 4.5 3.4 5.2



164 9.9 8.0 12.0

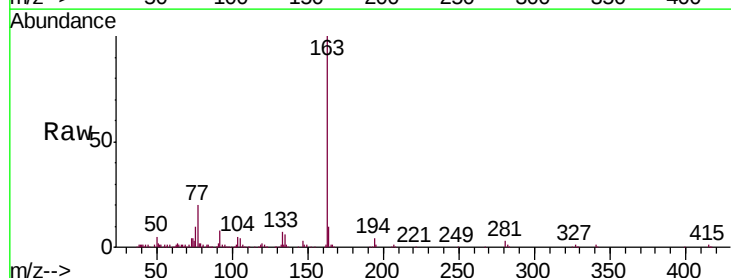


Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E



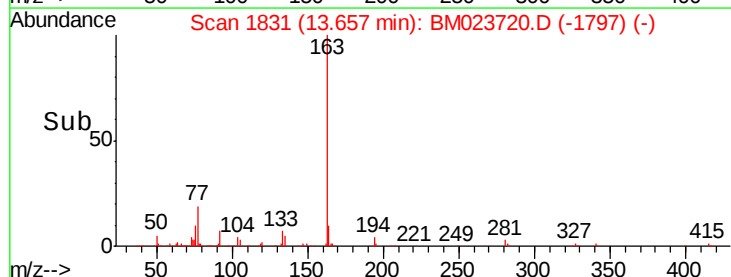
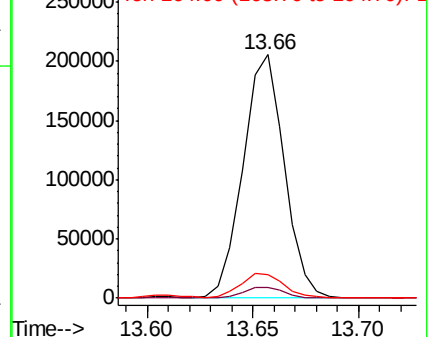


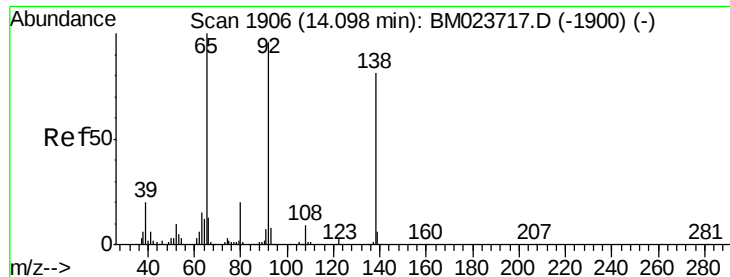

#49
3-Nitroaniline
Concen: 1.525 ng/ul
RT: 14.06 min Scan# 1900
Delta R.T. -0.04 min
Lab File: BM023720.D
Acq: 14 Nov 2019 17:16




Instrument :
BNA_M
ClientSampleId :
JLM81


Tgt Ion:138 Resp: 19838
Ion Ratio Lower Upper
138 100
108 10.7 10.2 15.2
92 12.8 105.4 158.0#

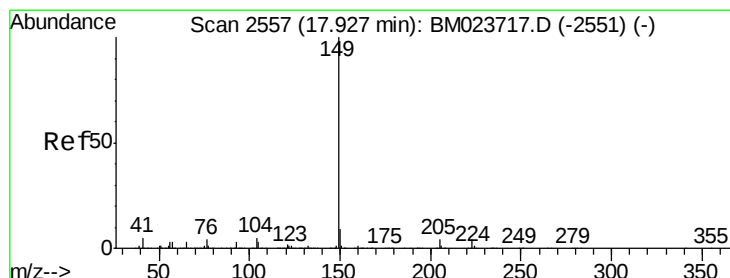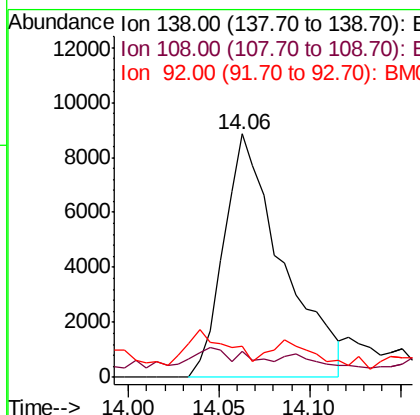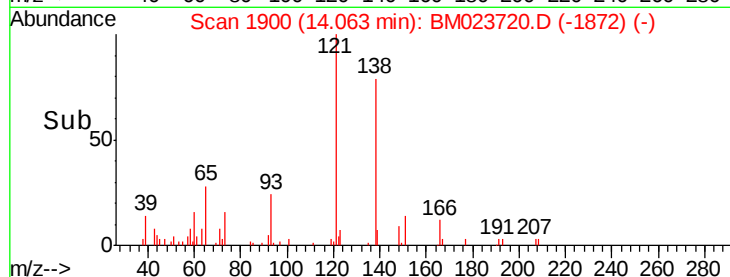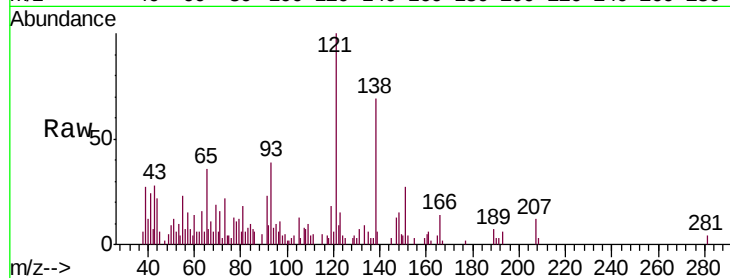

#76
Di-n-butylphthalate
Concen: 4.396 ng/ul
RT: 17.93 min Scan# 2557
Delta R.T. 0.00 min
Lab File: BM023720.D
Acq: 14 Nov 2019 17:16

Tgt Ion:149 Resp: 445868
Ion Ratio Lower Upper
149 100
150 10.4 7.1 10.7
104 5.1 4.2 6.2

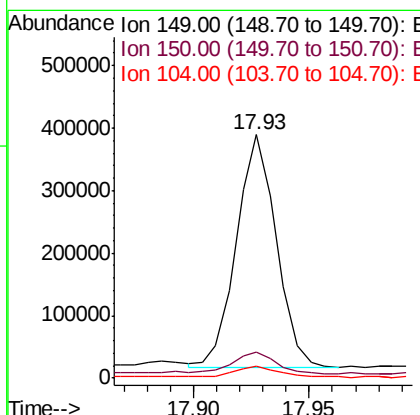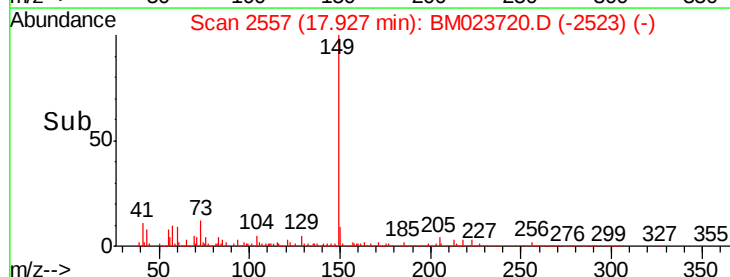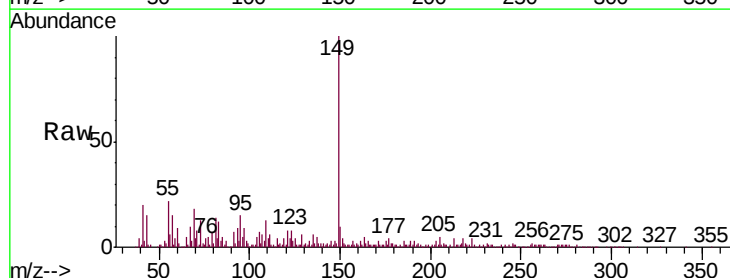

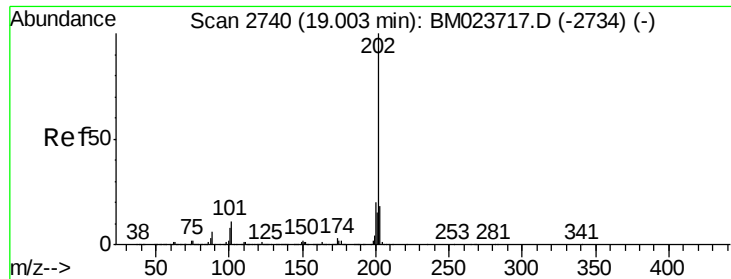

#77

Fluoranthene

Concen: 1.658 ng/ul

RT: 19.01 min Scan# 2741

Delta R.T. 0.01 min

Lab File: BM023720.D

Acq: 14 Nov 2019 17:16

Instrument :

BNA_M

ClientSampleId :

JLM81


Tgt Ion:202 Resp: 194988

Ion Ratio Lower Upper

202 100

101 11.4 7.7 11.5




100 8.1 6.0 9.0

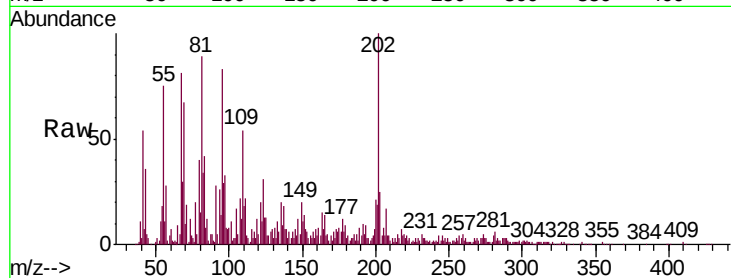

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

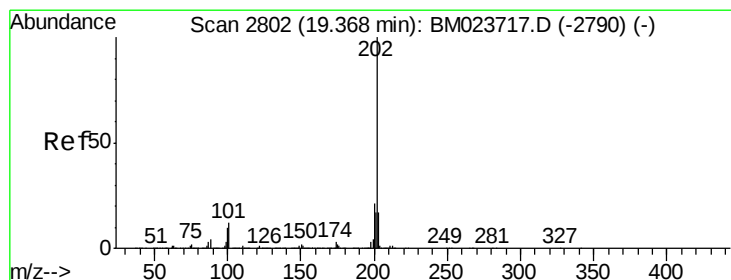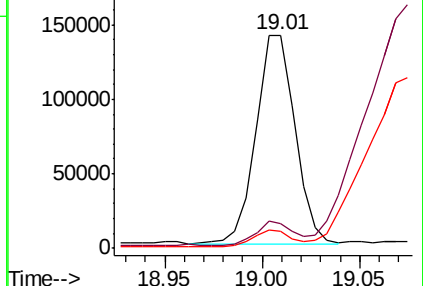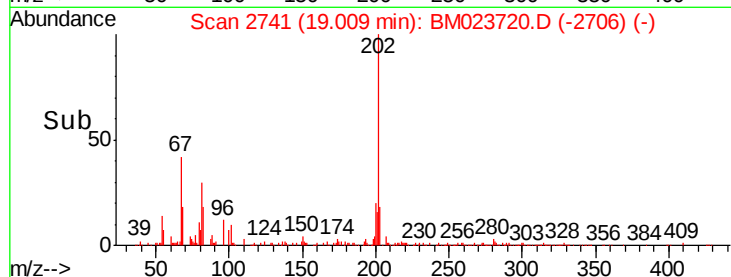

#80

Pyrene

Concen: 1.667 ng/ul

RT: 19.37 min Scan# 2803

Delta R.T. 0.01 min

Lab File: BM023720.D

Acq: 14 Nov 2019 17:16


Tgt Ion:202 Resp: 206914

Ion Ratio Lower Upper

202 100

101 14.2 9.8 14.6



100 10.4 8.1 12.1

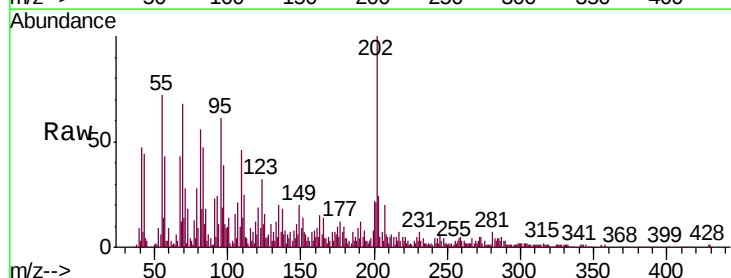


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

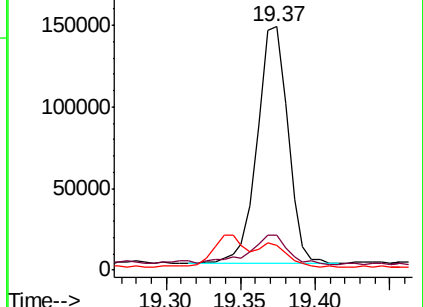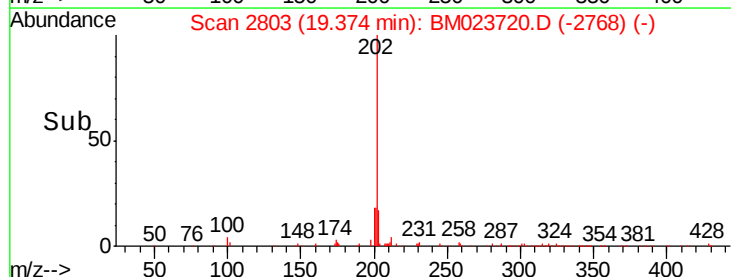

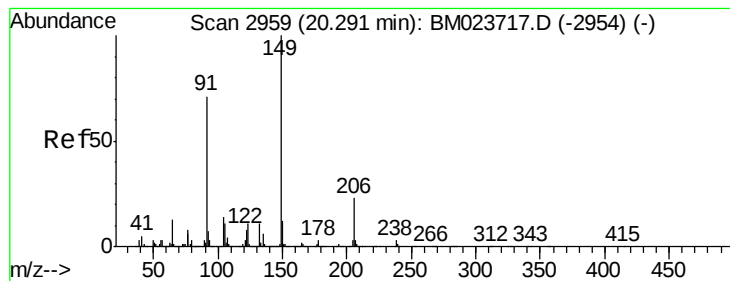

#81

Butylbenzylphthalate

Concen: 1.455 ng/ul

RT: 20.30 min Scan# 2960

Delta R.T. 0.01 min

Lab File: BM023720.D

Acq: 14 Nov 2019 17:16

Instrument :

BNA_M

ClientSampleId :

JLM81


Tgt Ion:149 Resp: 57179

Ion Ratio Lower Upper

149 100

91 87.5 54.9 82.3#

206 25.2 19.3 28.9



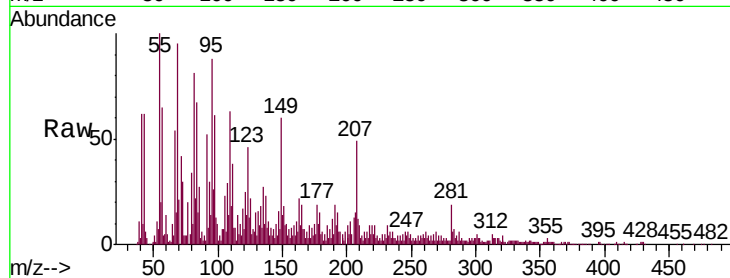


Abundance

Ion 149.00 (148.70 to 149.70): E

Ion 91.00 (90.70 to 91.70): BM

Ion 206.00 (205.70 to 206.70): E

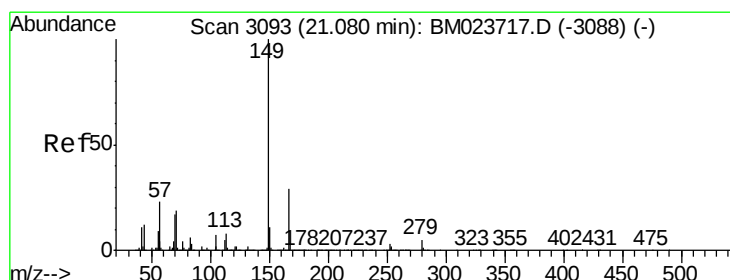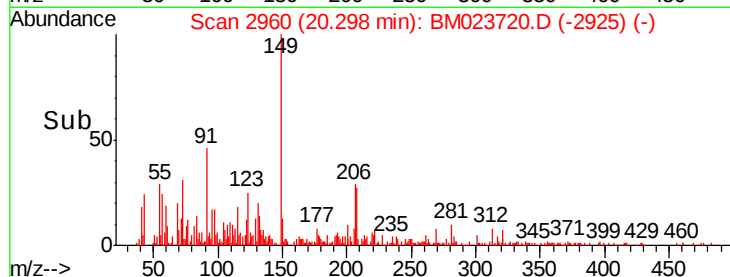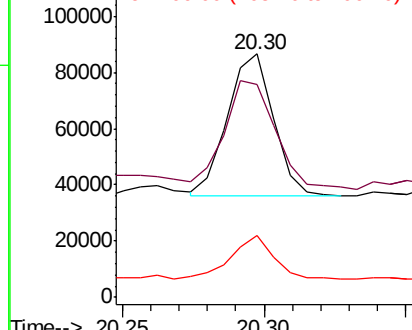

#84

Bis(2-ethylhexyl)phthalate

Concen: 13.135 ng/ul

RT: 21.09 min Scan# 3094

Delta R.T. 0.01 min

Lab File: BM023720.D

Acq: 14 Nov 2019 17:16


Tgt Ion:149 Resp: 779580

Ion Ratio Lower Upper

149 100

167 28.9 23.4 35.2

279 6.1 5.0 7.4


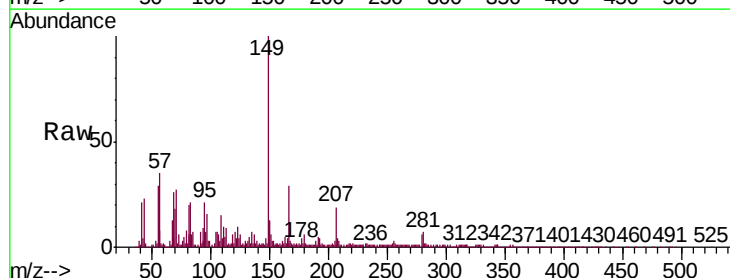



Abundance

Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

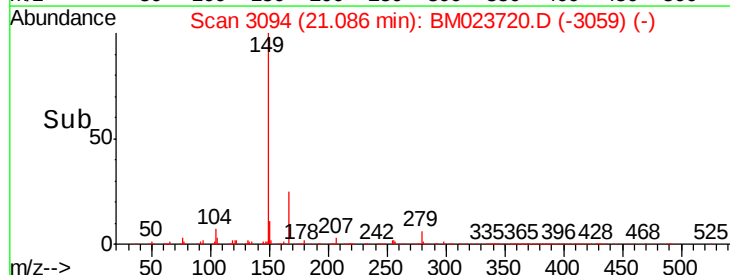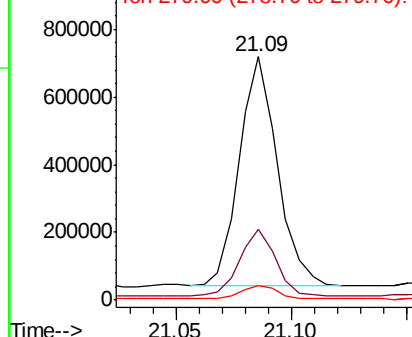

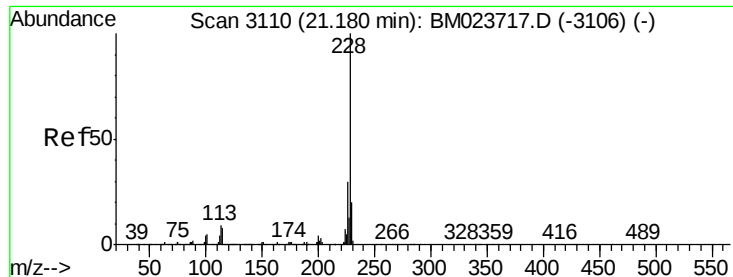

#85

Chrysene

Concen: 1.319 ng/ul

RT: 21.18 min Scan# 3110

Delta R.T. 0.00 min

Lab File: BM023720.D

Acq: 14 Nov 2019 17:16

Instrument :

BNA_M

ClientSampleId :

JLM81





Tgt Ion: 228 Resp: 157292

Ion Ratio Lower Upper

228 100

226 30.6 23.8 35.8

229 28.1 15.8 23.6#

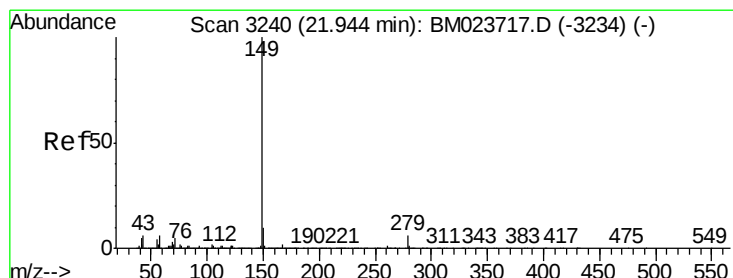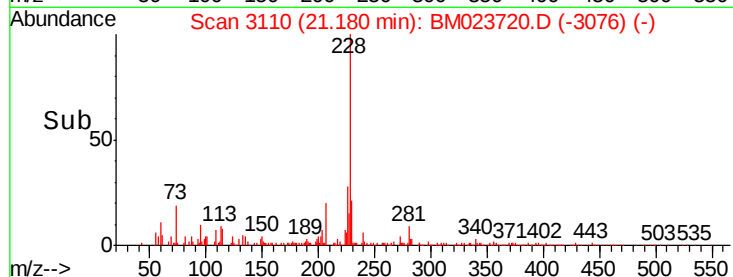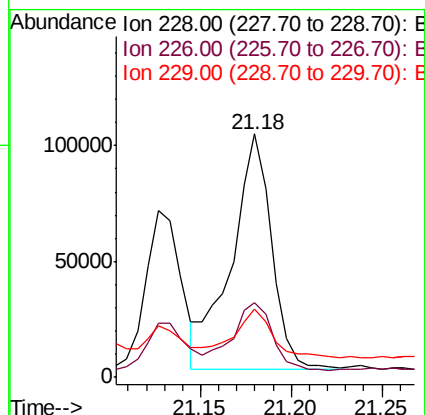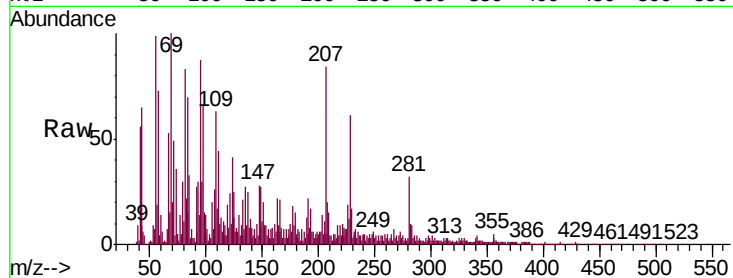

#87

Di-n-octyl phthalate

Concen: 1.429 ng/ul




RT: 21.96 min Scan# 3242


Delta R.T. 0.01 min

Lab File: BM023720.D

Acq: 14 Nov 2019 17:16

Tgt Ion: 149 Resp: 160331

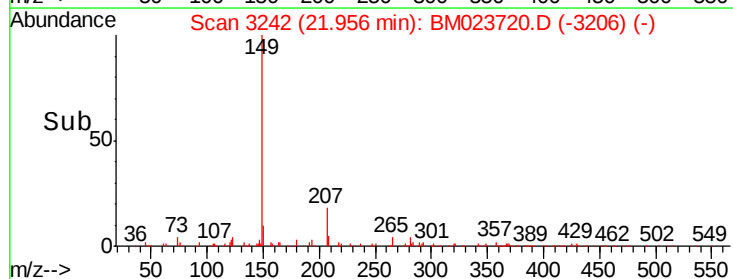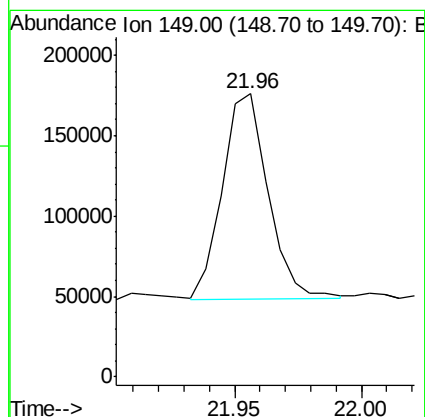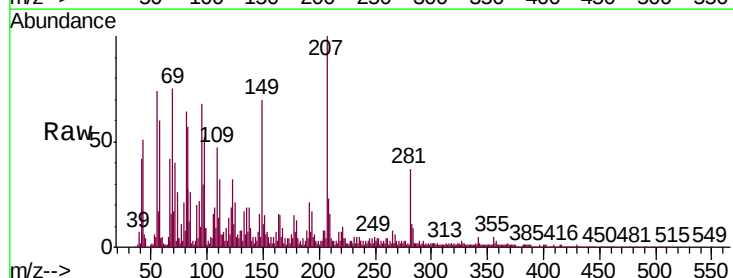

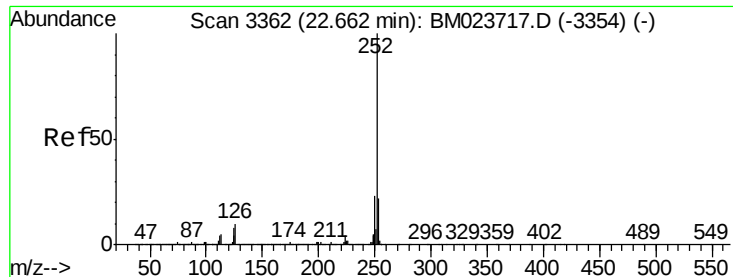

#88

Benzo(b)fluoranthene

Concen: 1.756 ng/ul

RT: 22.67 min Scan# 3363

Delta R.T. 0.01 min

Lab File: BM023720.D

Acq: 14 Nov 2019 17:16

Instrument :

BNA_M

ClientSampleId :

JLM81





Tgt Ion:252 Resp: 256981

Ion Ratio Lower Upper

252 100

253 30.2 17.8 26.8#

125 45.1 6.5 9.7#

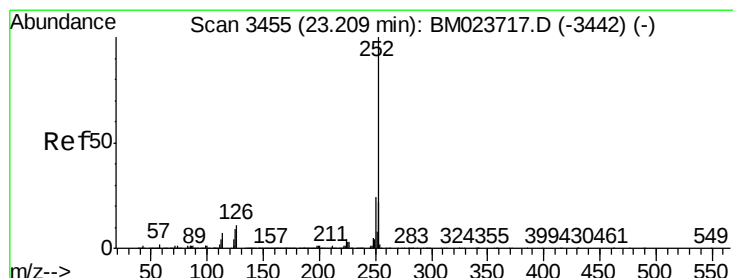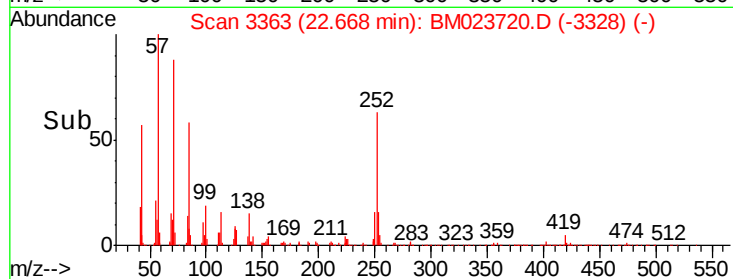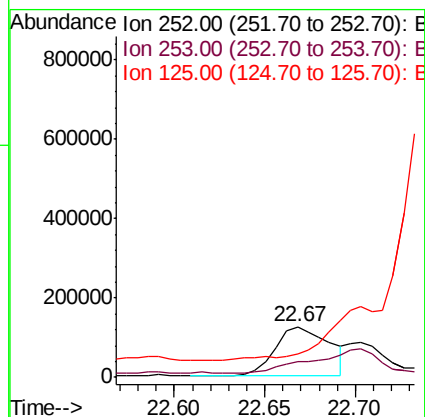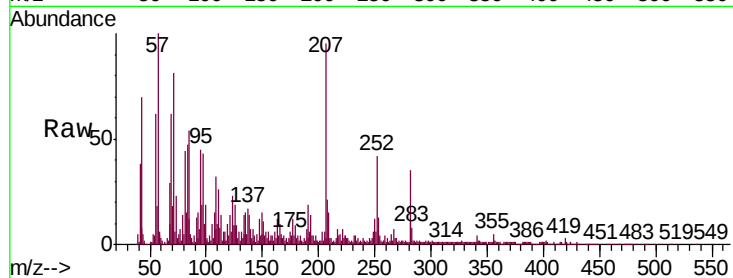

#91

Benzo(a)pyrene

Concen: 1.127 ng/ul

RT: 23.21 min Scan# 3456

Delta R.T. 0.01 min

Lab File: BM023720.D

Acq: 14 Nov 2019 17:16




Tgt Ion:252 Resp: 151072


Ion Ratio Lower Upper

252 100

253 30.7 17.3 25.9#

125 48.1 6.9 10.3#

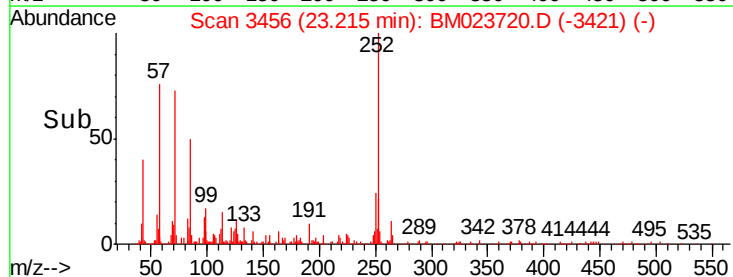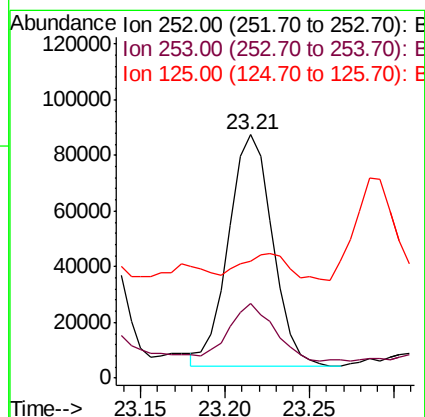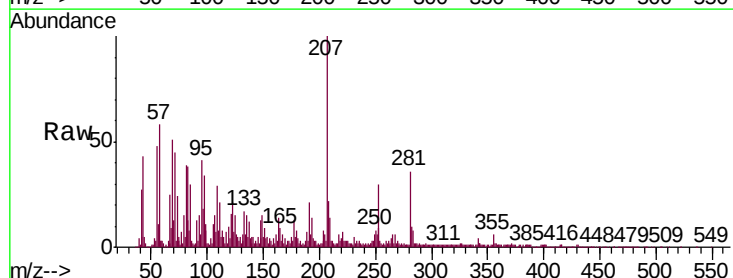

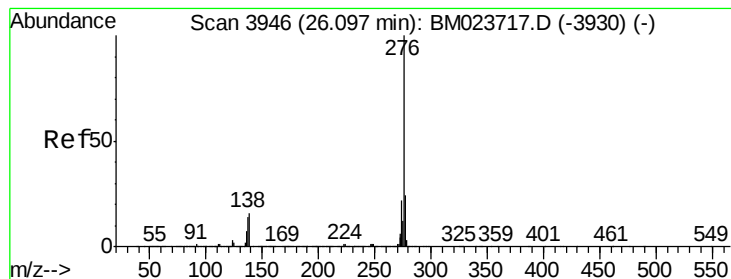

#94

Benzo(g,h,i)perylene

Concen: 1.101 ng/ul

RT: 26.11 min Scan# 3949

Delta R.T. 0.02 min

Lab File: BM023720.D

Acq: 14 Nov 2019 17:16

Instrument :

BNA_M

ClientSampleId :

JLM81

Tgt Ion:276 Resp: 127846

Ion Ratio Lower Upper

276 100

138 23.4 13.2 19.8#

277 29.7 18.6 28.0#

