

Data File : BM023764.D
Acq On : 15 Nov 2019 21:49
Operator : JU
Sample : K5699-03MSD
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F2J00MSD

Quant Time: Nov 16 03:21:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 16 03:18:12 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	313582	20.00	ng/ul	0.00
18) Naphthalene-d8	10.30	136	1261380	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.18	164	785294	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.93	188	1675196	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	1672406	20.00	ng/ul	0.00
86) Perylene-d12	23.29	264	2007252	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.06	96	53778	7.07	ng/uL	0.00
5) Phenol-d5	6.72	99	150946	5.28	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.87	67	395579	24.08	ng/ul	0.00
9) 2-Chlorophenol-d4	7.06	132	436109	21.06	ng/ul	0.00
13) 4-Methylphenol-d8	8.25	113	276904	12.14	ng/ul	0.00
19) Nitrobenzene-d5	8.67	128	259082	28.69	ng/ul	0.00
22) 2-Nitrophenol-d4	9.39	143	282460	29.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.93	165	546690	25.27	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	12186	0.51	ng/ul	0.01
44) Dimethylphthalate-d6	13.60	166	1838542	30.02	ng/ul	0.00
47) Acenaphthylene-d8	13.87	160	1990195	28.48	ng/ul	0.00
52) 4-Nitrophenol-d4	14.45	143	57664	5.52	ng/ul	0.04
58) Fluorene-d10	15.18	176	1555359	28.76	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.32	200	277748	28.66	ng/ul	0.00
71) Anthracene-d10	17.03	188	2531671	31.86	ng/ul	0.00
79) Pyrene-d10	19.33	212	2974274	34.11	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.16	264	3547827	33.59	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
6) Phenol	6.74	94	227052	7.711	ng/ul	97
10) 2-Chlorophenol	7.09	128	423411	19.828	ng/ul	98
15) N-Nitroso-di-n-propylamine	8.33	70	411308	22.015	ng/ul	98
28) Naphthalene	10.35	128	178357	2.690	ng/ul	99
33) 4-Chloro-3-methylphenol	11.62	107	524917	22.721	ng/ul	98
45) Dimethylphthalate	13.65	163	236317	3.938	ng/ul	99
50) Acenaphthene	14.24	153	1343912	26.916	ng/ul	99
53) 4-Nitrophenol	14.47	109	48580	5.759	ng/ul	95
55) 2,4-Dinitrotoluene	14.56	165	493878	29.561	ng/ul	99
69) Pentachlorophenol	16.59	266	402904	28.174	ng/ul	99
77) Fluoranthene	19.00	202	110756	1.120	ng/ul#	94
80) Pyrene	19.36	202	3690572	34.140	ng/ul	99
88) Benzo(b)fluoranthene	22.65	252	212149	1.658	ng/ul#	95
89) Benzo(k)fluoranthene	22.65	252	212149	1.721	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM023764.D
Acq On : 15 Nov 2019 21:49
Operator : JU
Sample : K5699-03MSD
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F2J00MSD

Quant Time: Nov 16 03:21:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 16 03:18:12 2019
Response via : Initial Calibration

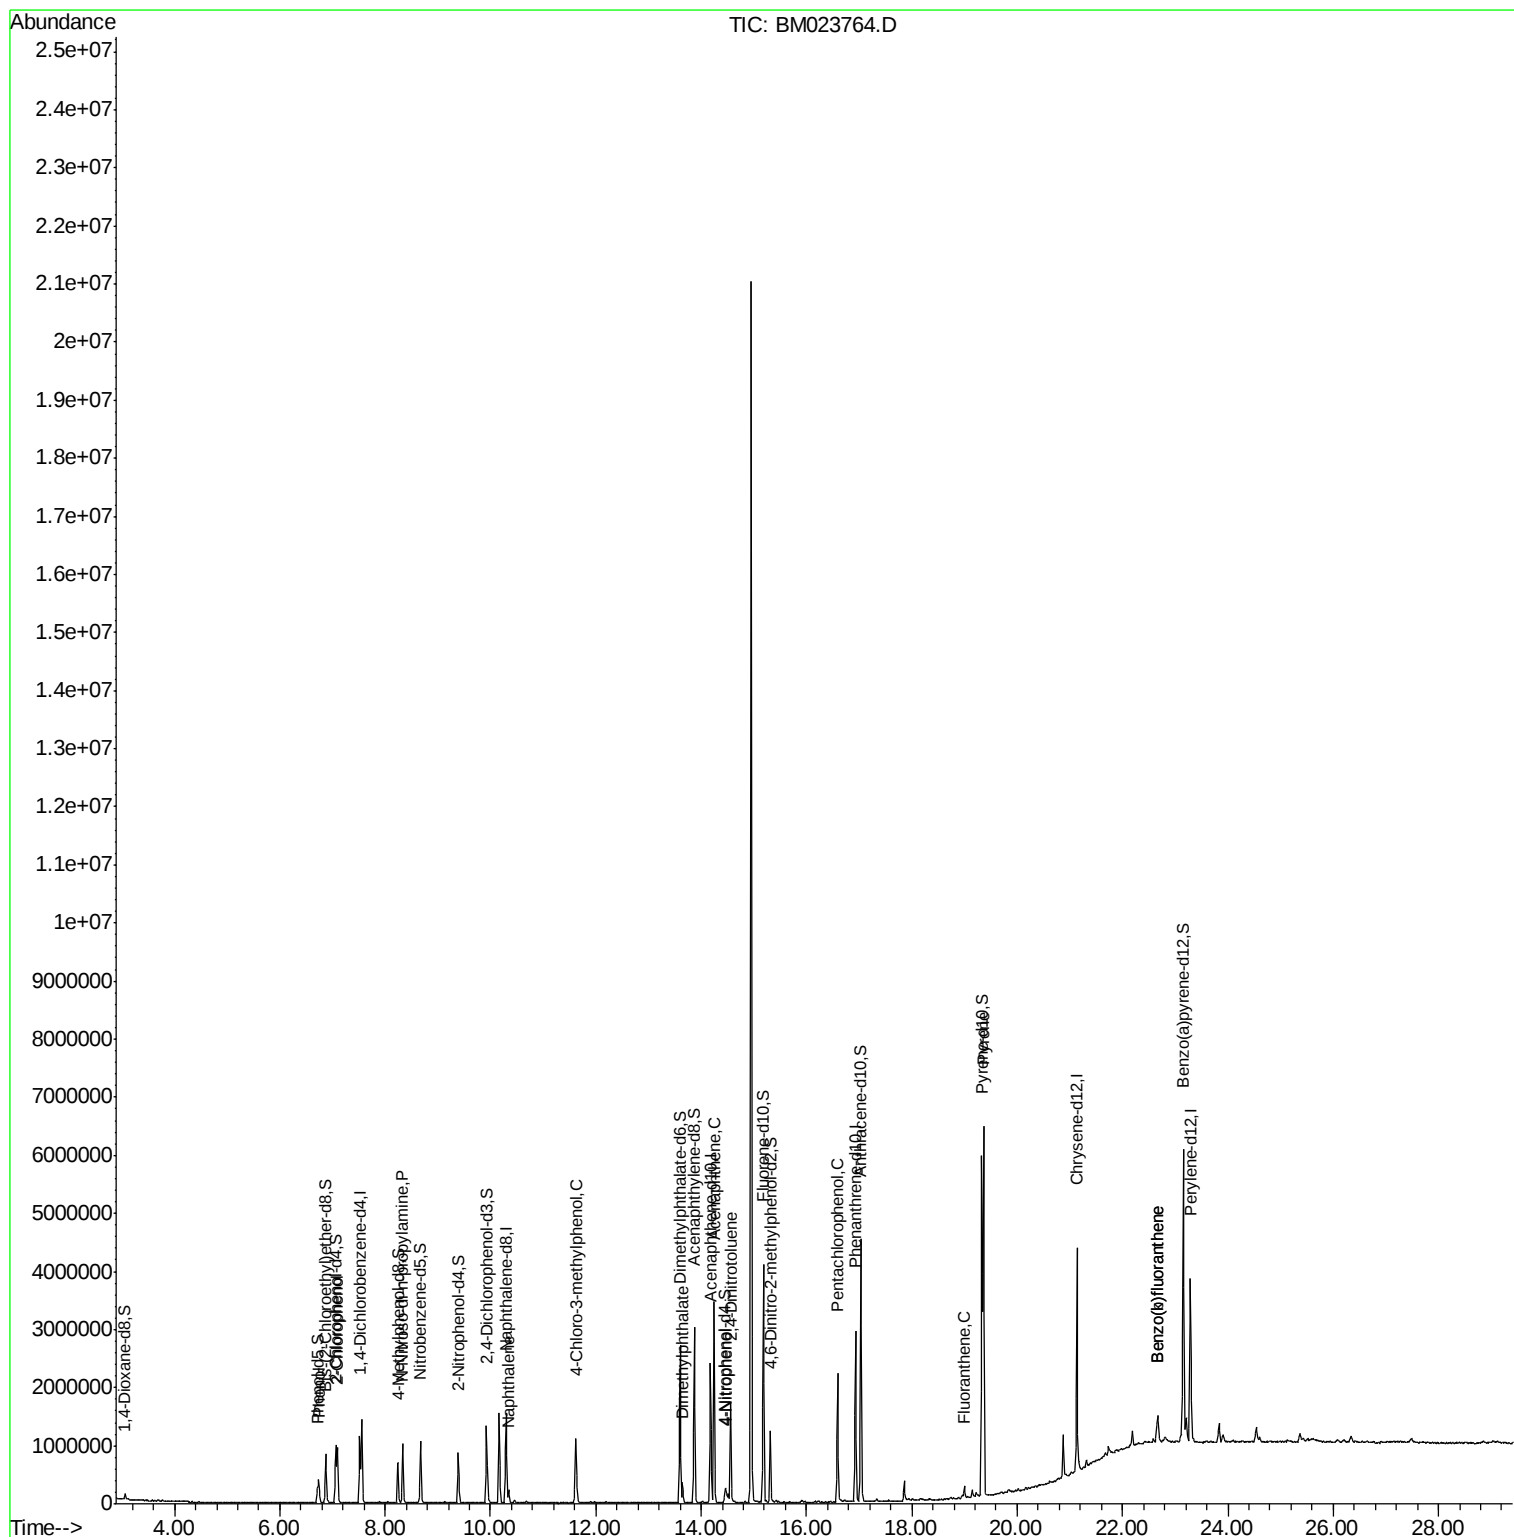



#6

Phenol

Concen: 7.711 ng/ul

RT: 6.74 min Scan# 655

Delta R.T. -0.00 min

Lab File: BM023764.D

Acq: 15 Nov 2019 21:49

Instrument :

BNA_M

ClientSampleId :

F2J00MSD


Tgt Ion: 94 Resp: 227052

Ion Ratio Lower Upper

94 100

65 27.4 21.4 32.2

66 35.4 30.7 46.1

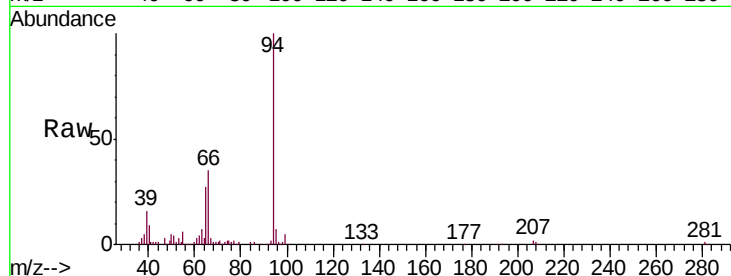

Abundance Ion 94.00 (93.70 to 94.70): BM023756.D (-648) (-)

Ion 65.00 (64.70 to 65.70): BM023756.D (-648) (-)

Ion 66.00 (65.70 to 66.70): BM023756.D (-648) (-)

6.74

150000



100000

50000

0

6.70 6.75 6.80

Time-->

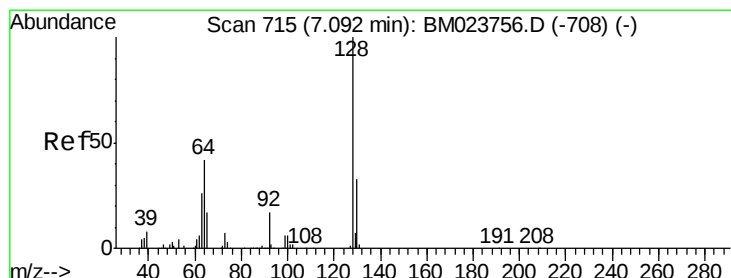

#10

2-Chlorophenol

Concen: 19.828 ng/ul

RT: 7.09 min Scan# 715

Delta R.T. -0.00 min

Lab File: BM023764.D

Acq: 15 Nov 2019 21:49


Tgt Ion: 128 Resp: 423411

Ion Ratio Lower Upper

128 100

64 45.9 38.1 57.1

130 32.0 26.4 39.6

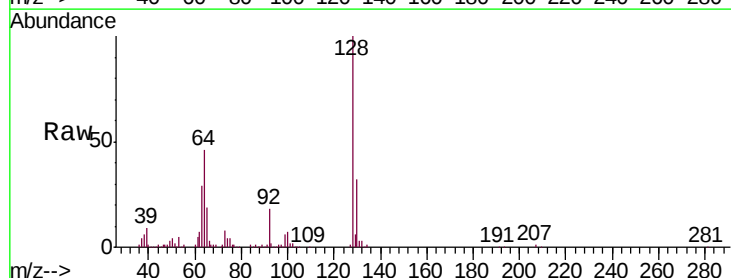

Abundance Ion 128.00 (127.70 to 128.70): BM023756.D (-708) (-)

Ion 64.00 (63.70 to 64.70): BM023756.D (-708) (-)

Ion 130.00 (129.70 to 130.70): BM023756.D (-708) (-)

7.09

300000


200000


100000

0

7.00 7.05 7.10 7.15 7.20

Time-->






#15
N-Nitroso-di-n-propylamine
Concen: 22.015 ng/ul
RT: 8.33 min Scan# 926
Delta R.T. -0.01 min
Lab File: BM023764.D
Acq: 15 Nov 2019 21:49

Instrument :
BNA_M
ClientSampleId :
F2J00MSD

Tgt Ion	Ratio	Lower	Upper
70	100		
42	41.8	32.1	48.1
101	10.0	7.4	11.2
130	20.0	15.8	23.6

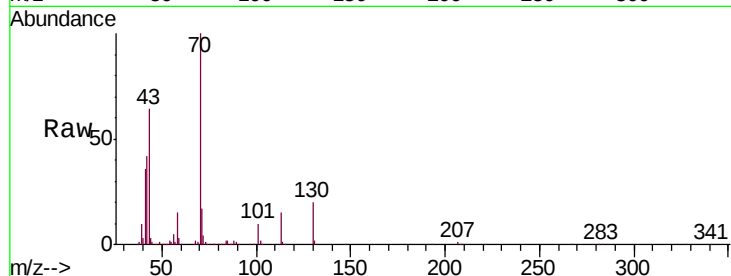




Abundance

Ion 70.00 (69.70 to 70.70): BM023756.D (-920) (-)

Ion 42.00 (41.70 to 42.70): BM023756.D (-920) (-)


Ion 101.00 (100.70 to 101.70): BM023756.D (-920) (-)

Ion 130.00 (129.70 to 130.70): BM023756.D (-920) (-)

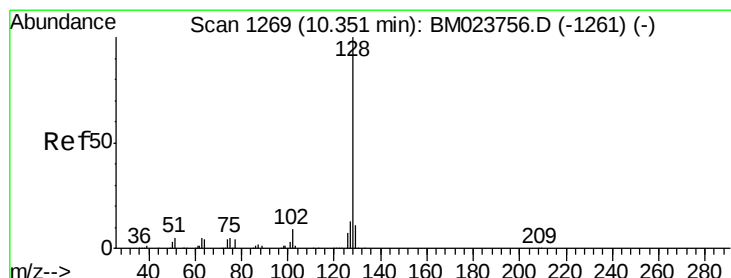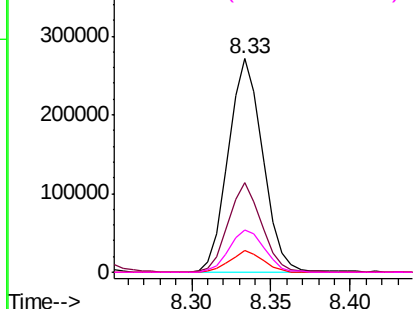

#28
Naphthalene
Concen: 2.690 ng/ul
RT: 10.35 min Scan# 1268
Delta R.T. -0.01 min
Lab File: BM023764.D
Acq: 15 Nov 2019 21:49

Tgt Ion	Ratio	Lower	Upper
128	100		
129	11.4	8.7	13.1
127	13.0	10.6	16.0


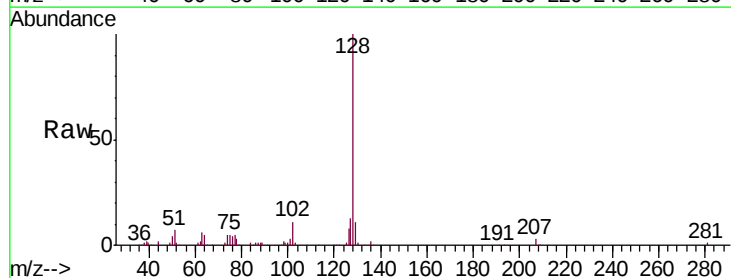



Abundance

Ion 128.00 (127.70 to 128.70): BM023756.D (-1261) (-)

Ion 129.00 (128.70 to 129.70): BM023756.D (-1261) (-)

Ion 127.00 (126.70 to 127.70): BM023756.D (-1261) (-)



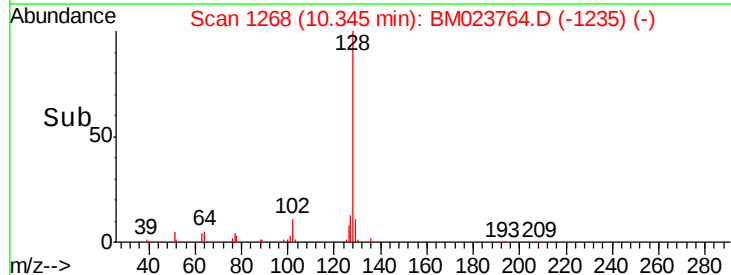
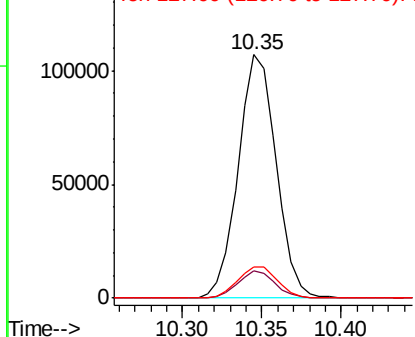




#33
 4-Chloro-3-methylphenol
 Concen: 22.721 ng/ul
 RT: 11.62 min Scan# 1485
 Delta R.T. 0.01 min
 Lab File: BM023764.D
 Acq: 15 Nov 2019 21:49




Instrument :
 BNA_M
 ClientSampleId :
 F2J00MSD


Tgt Ion:107 Resp: 524917
 Ion Ratio Lower Upper
 107 100
 144 26.3 20.6 30.8
 142 80.2 62.9 94.3

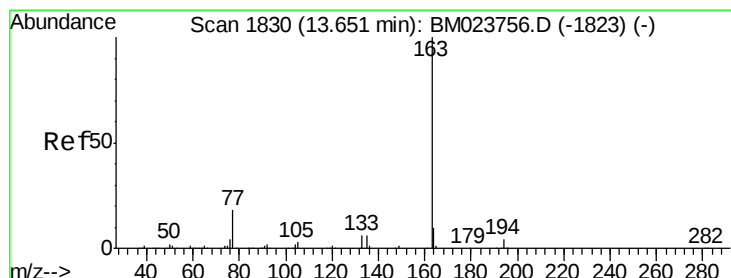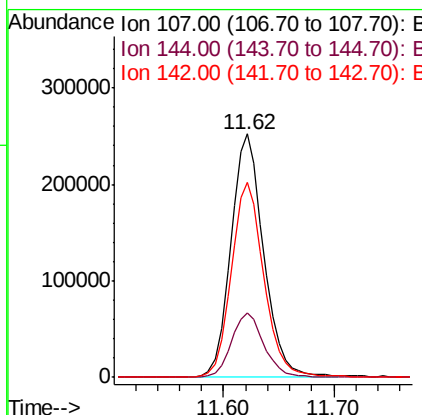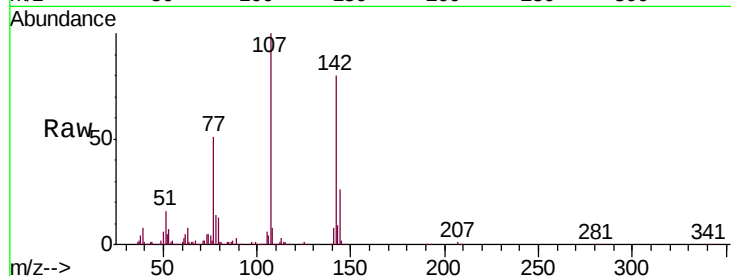

#45
 Dimethylphthalate
 Concen: 3.938 ng/ul
 RT: 13.65 min Scan# 1830
 Delta R.T. -0.00 min
 Lab File: BM023764.D
 Acq: 15 Nov 2019 21:49

Tgt Ion:163 Resp: 236317
 Ion Ratio Lower Upper
 163 100
 194 4.2 3.4 5.2
 164 10.3 8.0 12.0

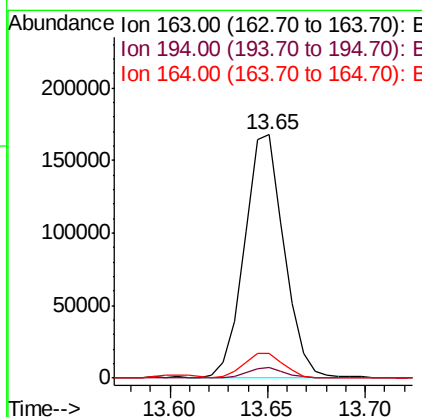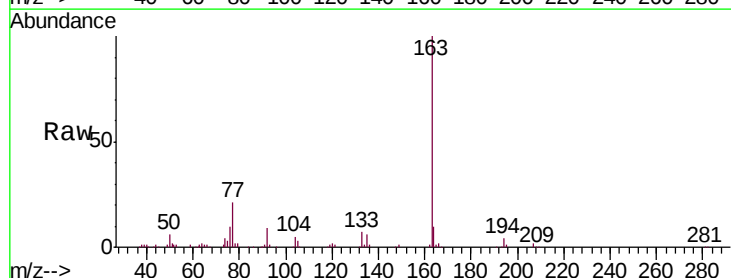

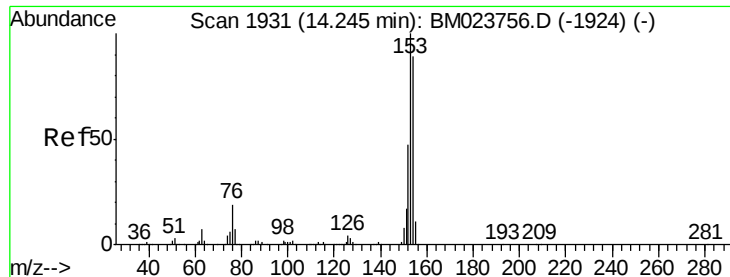

#50

Acenaphthene

Concen: 26.916 ng/ul

RT: 14.24 min Scan# 1931

Delta R.T. -0.00 min

Lab File: BM023764.D

Acq: 15 Nov 2019 21:49

Instrument :

BNA_M

ClientSampleId :

F2J00MSD


Tgt Ion:153 Resp: 1343912

Ion Ratio Lower Upper

153 100

152 47.1 37.7 56.5




154 89.6 70.6 106.0

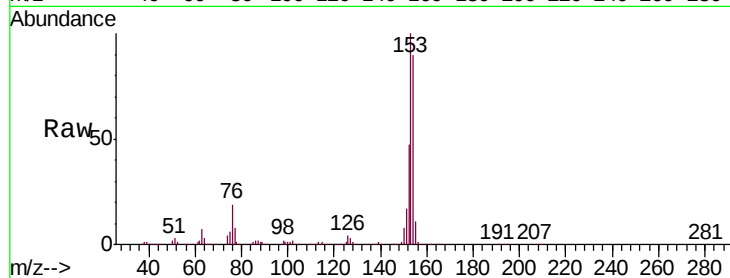

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

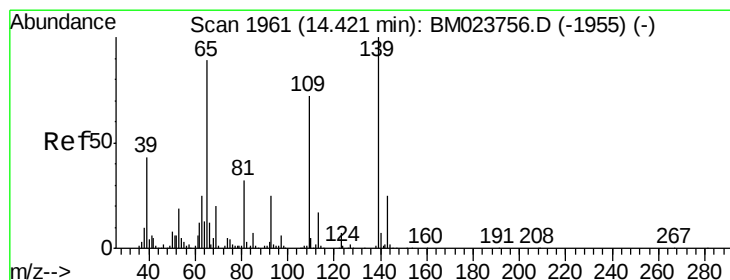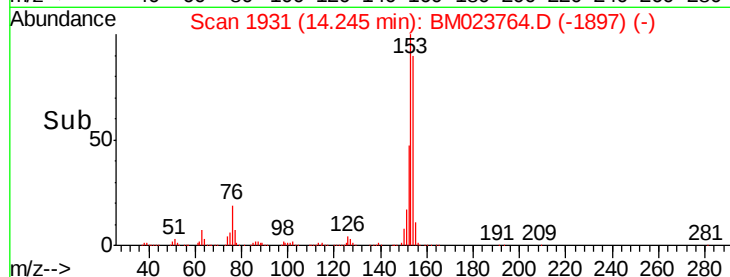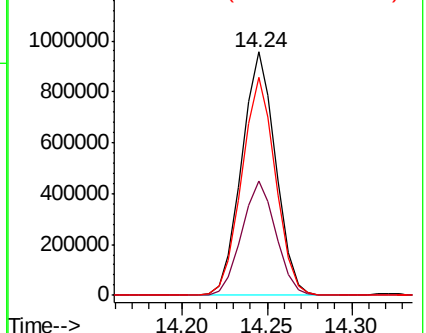

#53

4-Nitrophenol

Concen: 5.759 ng/ul

RT: 14.47 min Scan# 1969

Delta R.T. 0.05 min

Lab File: BM023764.D

Acq: 15 Nov 2019 21:49


Tgt Ion:109 Resp: 48580

Ion Ratio Lower Upper

109 100

139 118.5 103.4 155.0



65 125.6 101.3 151.9

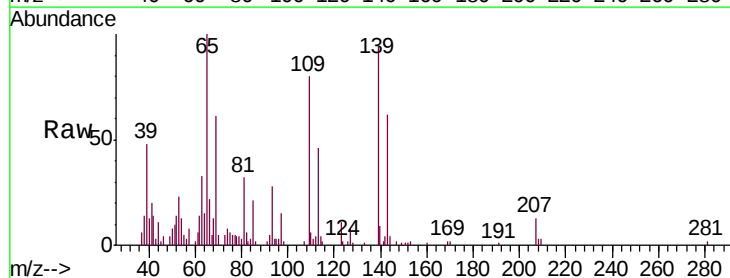


Abundance Ion 109.00 (108.70 to 109.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 65.00 (64.70 to 65.70): BM

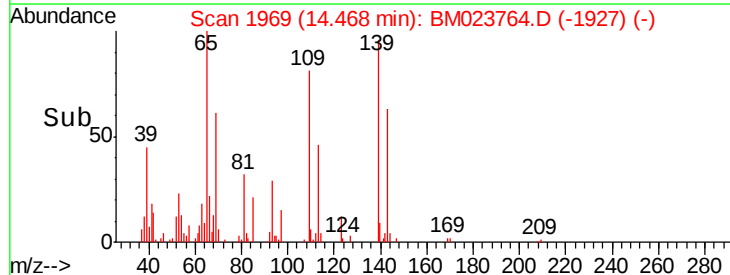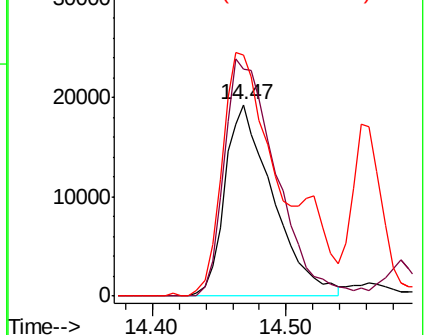


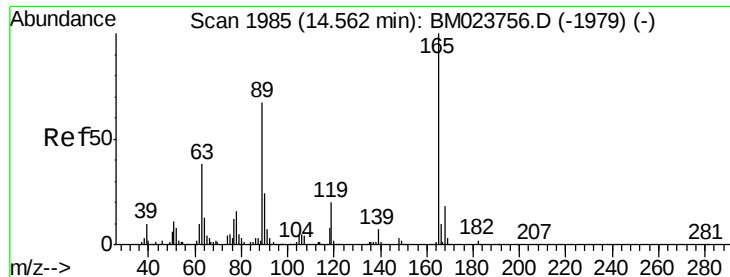




#55
2,4-Dinitrotoluene
Concen: 29.561 ng/ul
RT: 14.56 min Scan# 1985
Delta R.T. -0.00 min
Lab File: BM023764.D
Acq: 15 Nov 2019 21:49

Instrument :
BNA_M
ClientSampleId :
F2J00MSD

Tgt Ion	Ratio	Lower	Upper
165	100		
63	38.1	31.0	46.6
182	3.0	2.4	3.6

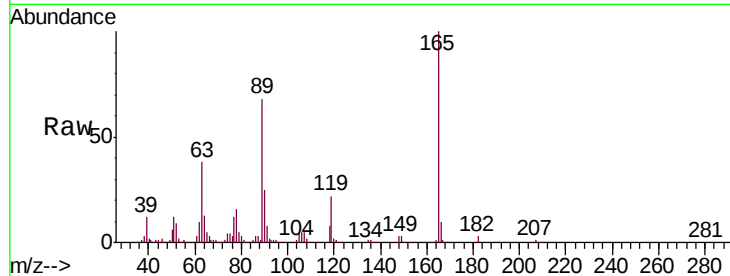


Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BM
Ion 182.00 (181.70 to 182.70): E

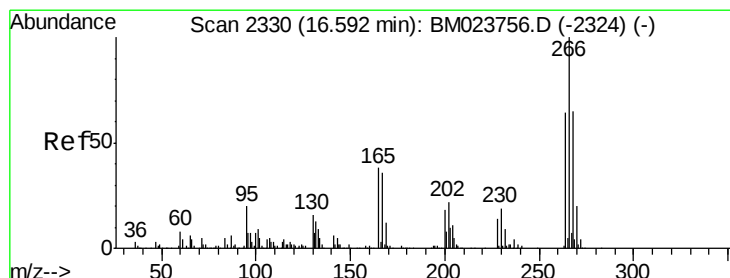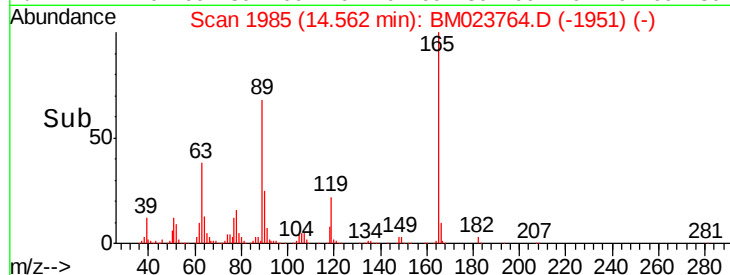
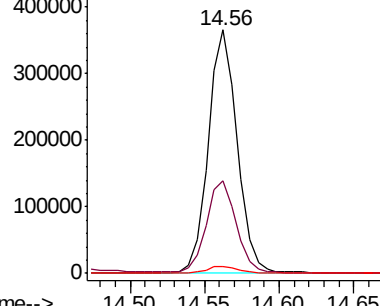



#69
Pentachlorophenol
Concen: 28.174 ng/ul
RT: 16.59 min Scan# 2330
Delta R.T. -0.00 min
Lab File: BM023764.D
Acq: 15 Nov 2019 21:49

Tgt Ion	Ratio	Lower	Upper
266	100		
264	61.5	50.6	75.8
268	63.7	50.9	76.3

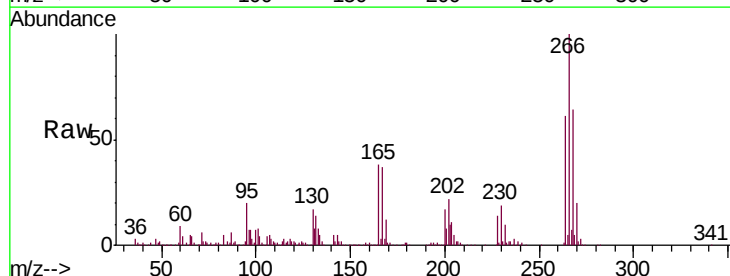

Abundance Ion 265.70 (265.40 to 266.40): E
Ion 264.00 (263.70 to 264.70): E
Ion 268.00 (267.70 to 268.70): E



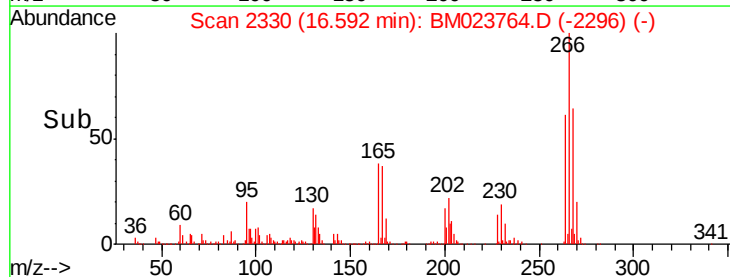
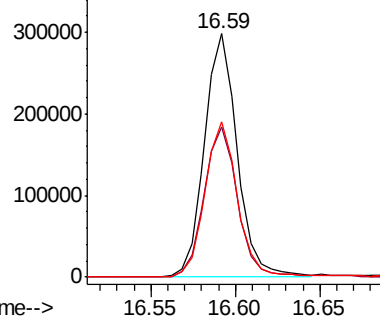




#77
Fluoranthene
 Concen: 1.120 ng/ul
 RT: 19.00 min Scan# 2739
 Delta R.T. -0.01 min
 Lab File: BM023764.D
 Acq: 15 Nov 2019 21:49




Instrument :
 BNA_M
 ClientSampleId :
 F2J00MSD


Tgt Ion	Ratio	Lower	Upper
202	100		
101	11.8	7.7	11.5#
100	9.3	6.0	9.0#

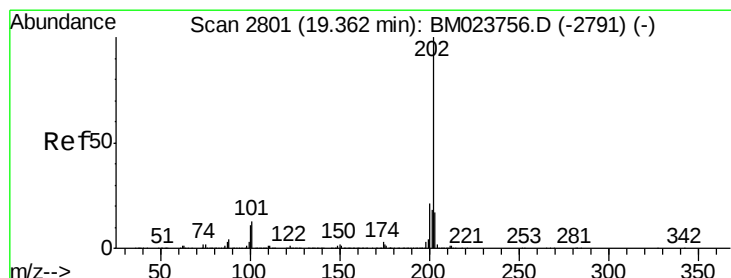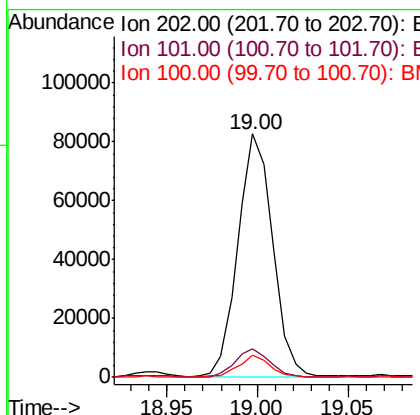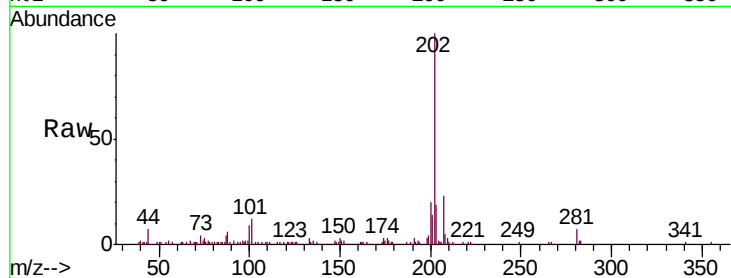

#80
Pyrene
 Concen: 34.140 ng/ul
 RT: 19.36 min Scan# 2801
 Delta R.T. -0.00 min
 Lab File: BM023764.D
 Acq: 15 Nov 2019 21:49

Tgt Ion	Ratio	Lower	Upper
202	100		
101	12.8	9.8	14.6
100	10.3	8.1	12.1

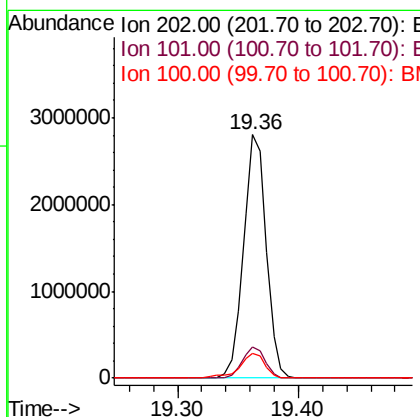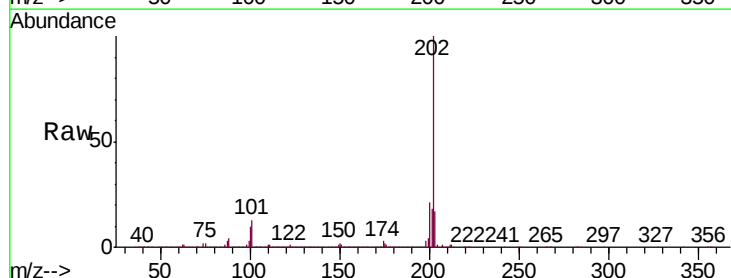

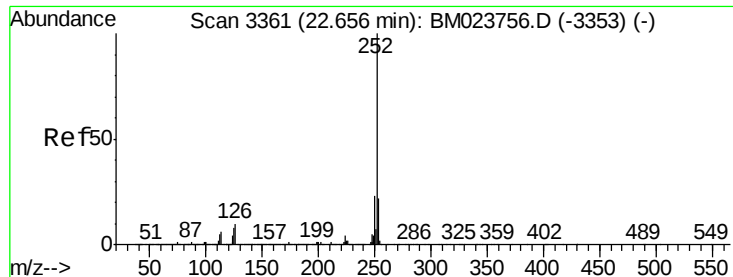

#88

Benzo(b)fluoranthene

Concen: 1.658 ng/ul

RT: 22.65 min Scan# 3360

Delta R.T. -0.01 min

Lab File: BM023764.D

Acq: 15 Nov 2019 21:49





Instrument :

BNA_M

ClientSampleId :

F2J00MSD

Tgt Ion:	252	Resp:	212149
Ion Ratio	Lower	Upper	
252	100		
253	24.1	17.8	26.8
125	10.8	6.5	9.7#

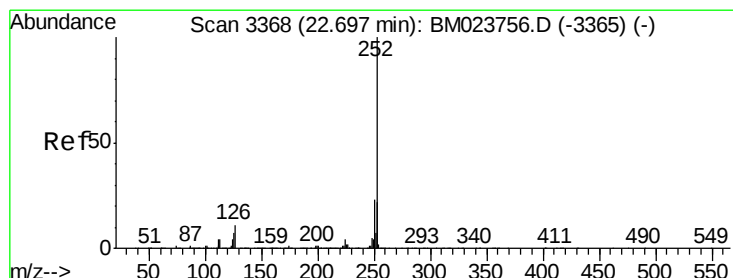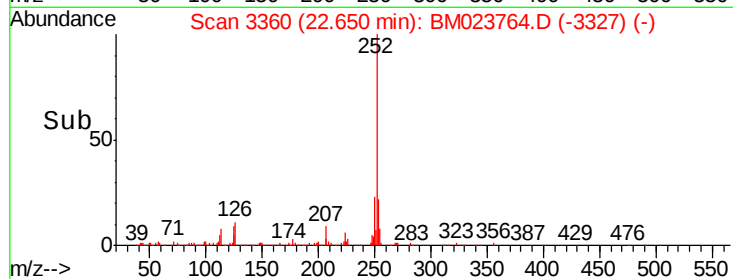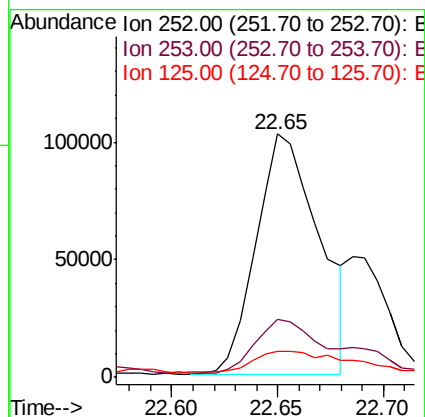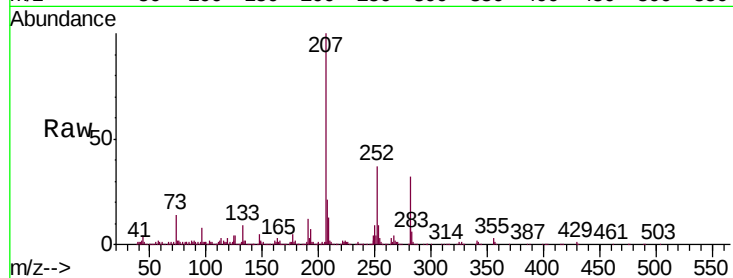

#89

Benzo(k)fluoranthene

Concen: 1.721 ng/ul

RT: 22.65 min Scan# 3360

Delta R.T. -0.05 min

Lab File: BM023764.D

Acq: 15 Nov 2019 21:49

Tgt Ion:	252	Resp:	212149
Ion Ratio	Lower	Upper	
252	100		
253	24.1	17.2	25.8
125	10.8	5.9	8.9#

