

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111419\
 Data File : BM023725.D
 Acq On : 14 Nov 2019 20:17
 Operator : JU
 Sample : K5700-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEGY0

Quant Time: Nov 15 06:33:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 15 06:30:14 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	266356	20.00	ng/ul	0.00
18) Naphthalene-d8	10.30	136	1090359	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.19	164	713932	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.94	188	1550936	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	1510218	20.00	ng/ul	0.00
86) Perylene-d12	23.30	264	1778371	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.06	96	35695	5.52	ng/uL	0.00
5) Phenol-d5	6.72	99	119231	4.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.87	67	302081	21.65	ng/ul	0.00
9) 2-Chlorophenol-d4	7.07	132	343634	19.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.25	113	220205	11.37	ng/ul	0.00
19) Nitrobenzene-d5	8.68	128	203163	26.03	ng/ul	0.00
22) 2-Nitrophenol-d4	9.40	143	230469	28.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.94	165	411697	22.01	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	37353	1.82	ng/ul	0.00
44) Dimethylphthalate-d6	13.61	166	1506227	27.05	ng/ul	0.00
47) Acenaphthylene-d8	13.87	160	1647749	25.93	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	42244	4.45	ng/ul	0.00
58) Fluorene-d10	15.19	176	1337040	27.20	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.32	200	231861	25.84	ng/ul	0.00
71) Anthracene-d10	17.04	188	2304189	31.32	ng/ul	0.00
79) Pyrene-d10	19.34	212	2564963	32.57	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.16	264	2962836	31.66	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.66	163	95413	1.749	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111419\
Data File : BM023725.D
Acq On : 14 Nov 2019 20:17
Operator : JU
Sample : K5700-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEGY0

Quant Time: Nov 15 06:33:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 15 06:30:14 2019
Response via : Initial Calibration

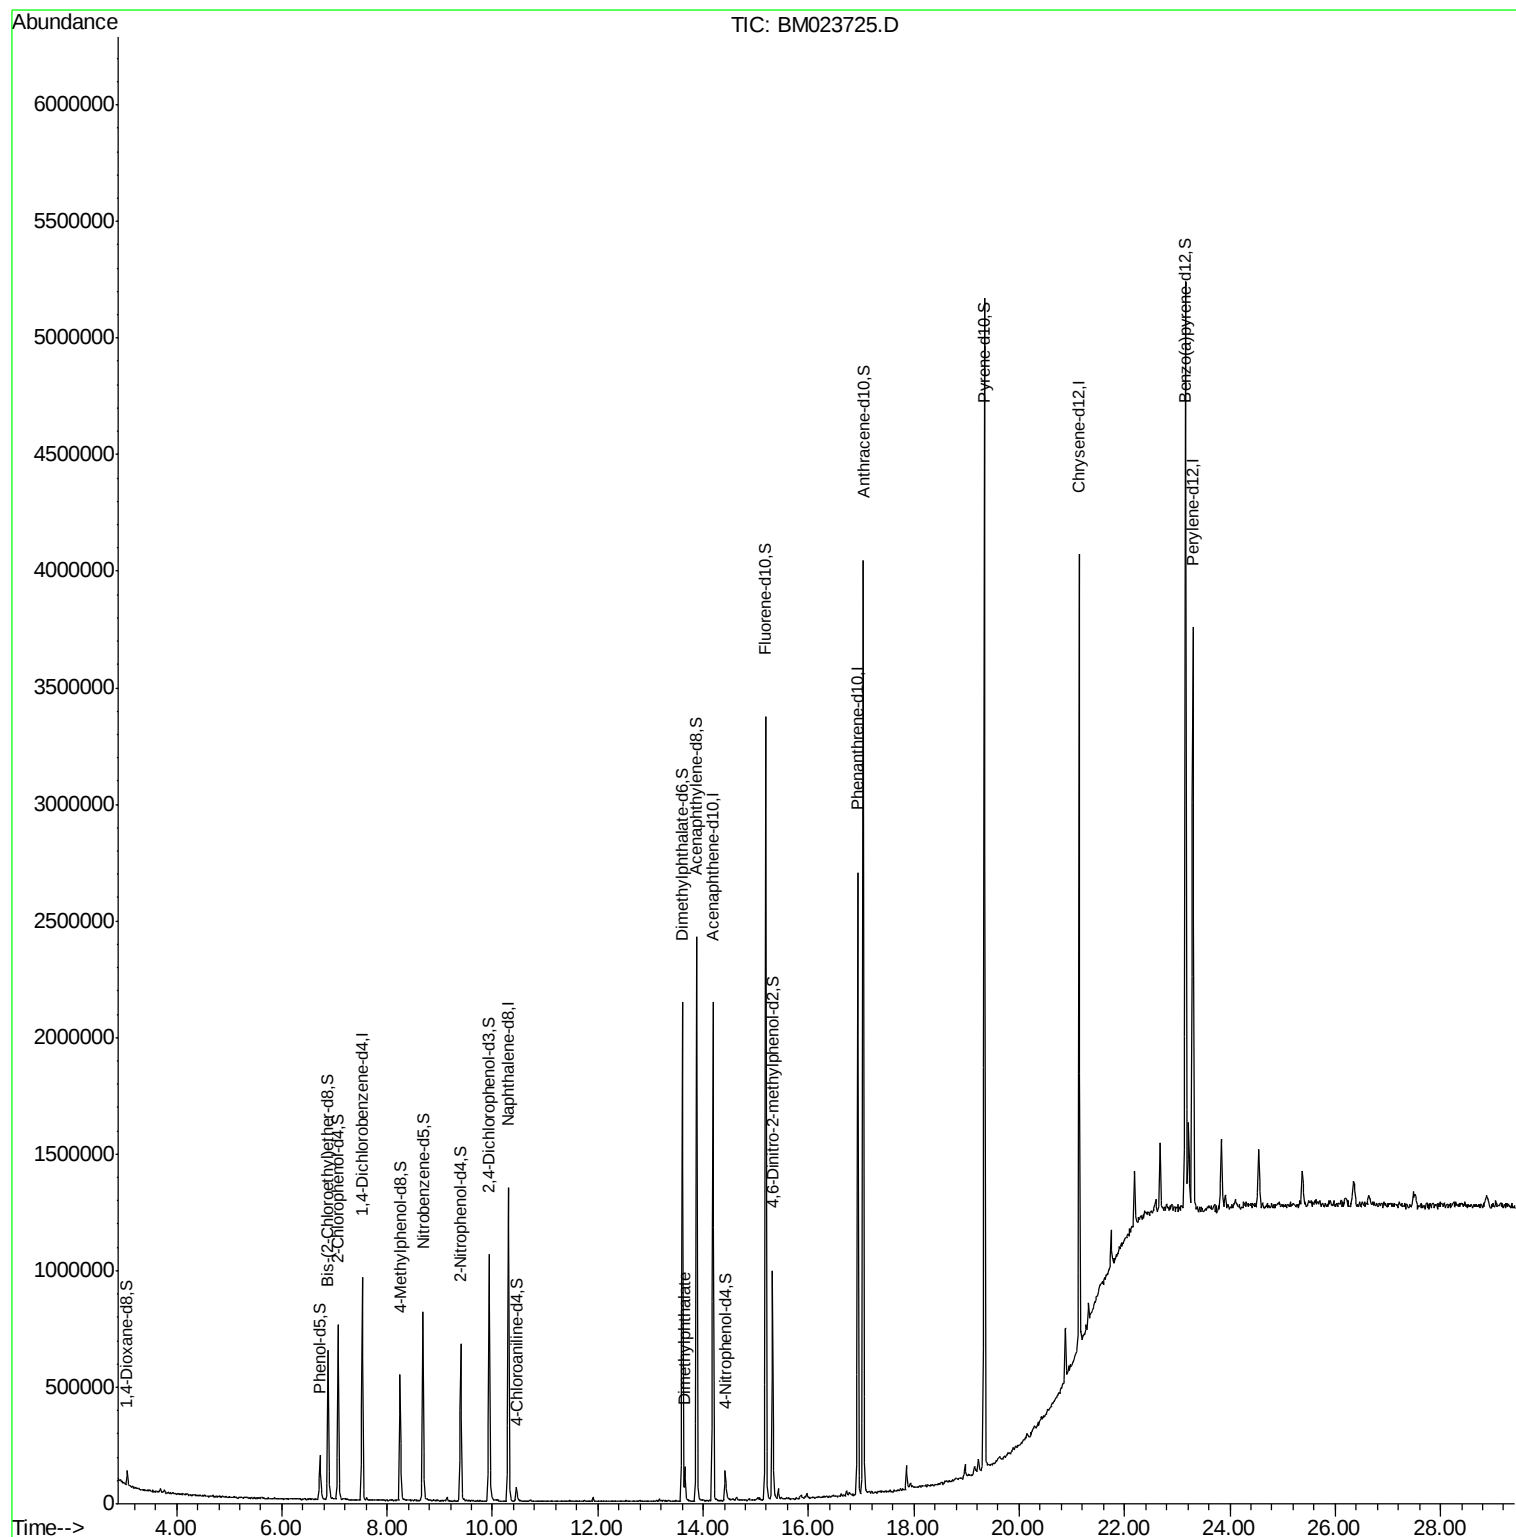

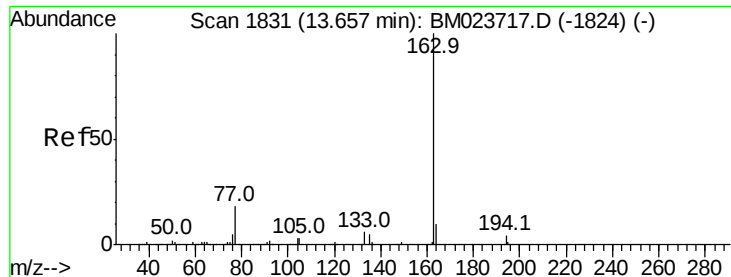

#45

Dimethylphthalate

Concen: 1.749 ng/ul

RT: 13.66 min Scan# 1831

Delta R.T. 0.00 min

Lab File: BM023725.D

Acq: 14 Nov 2019 20:17

Instrument :

BNA_M

ClientSampleId :

BEGY0

Tot Ion:163 Resp: 95413

Ion Ratio Lower Upper

163 100

194 5.0 3.4 5.2

164 9.9 8.0 12.0

