

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111419\
 Data File : BM023754.D
 Acq On : 15 Nov 2019 15:29
 Operator : JU
 Sample : K5700-16DL2 100X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEGY8DL2

Quant Time: Nov 15 17:11:21 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 15 07:53:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	393708	20.00	ng/ul	0.00
18) Naphthalene-d8	10.30	136	1603064	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.18	164	967210	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.93	188	2001882	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	2014039	20.00	ng/ul	0.00
86) Perylene-d12	23.29	264	2444252	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL	
5) Phenol-d5	0.00	99	0d	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	6.88	67	4642	0.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.07	132	4222	0.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	2268	0.08	ng/ul	0.01
19) Nitrobenzene-d5	8.69	128	2941	0.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.40	143	1791	0.15	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	3247	0.12	ng/ul	0.01
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
44) Dimethylphthalate-d6	13.60	166	17933	0.24	ng/ul	0.00
47) Acenaphthylene-d8	13.87	160	17335	0.20	ng/ul	0.00
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	15.18	176	17236	0.26	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	0.00	200	0d	0.00	ng/ul	
71) Anthracene-d10	0.00	188	0d	0.00	ng/ul	
79) Pyrene-d10	19.33	212	26880	0.26	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.16	264	31281	0.24	ng/ul	0.00

Target Compounds


					Ovalue	
28) Naphthalene	10.35	128	3933023	46.679	ng/ul	100
34) 2-Methylnaphthalene	11.97	142	65841	1.022	ng/ul	94
41) 1,1'-Biphenyl	13.01	154	78213	1.048	ng/ul	99
50) Acenaphthene	14.25	153	203744	3.313	ng/ul	99
54) Dibenzofuran	14.59	168	207543	2.280	ng/ul	100
59) Fluorene	15.24	166	113609	1.538	ng/ul	95
70) Phenanthrene	16.97	178	165683	1.503	ng/ul	100
75) Carbazole	17.34	167	197371	2.135	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111419\
Data File : BM023754.D
Acq On : 15 Nov 2019 15:29
Operator : JU
Sample : K5700-16DL2 100X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEGY8DL2

Quant Time: Nov 15 17:11:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 15 07:53:56 2019
Response via : Initial Calibration

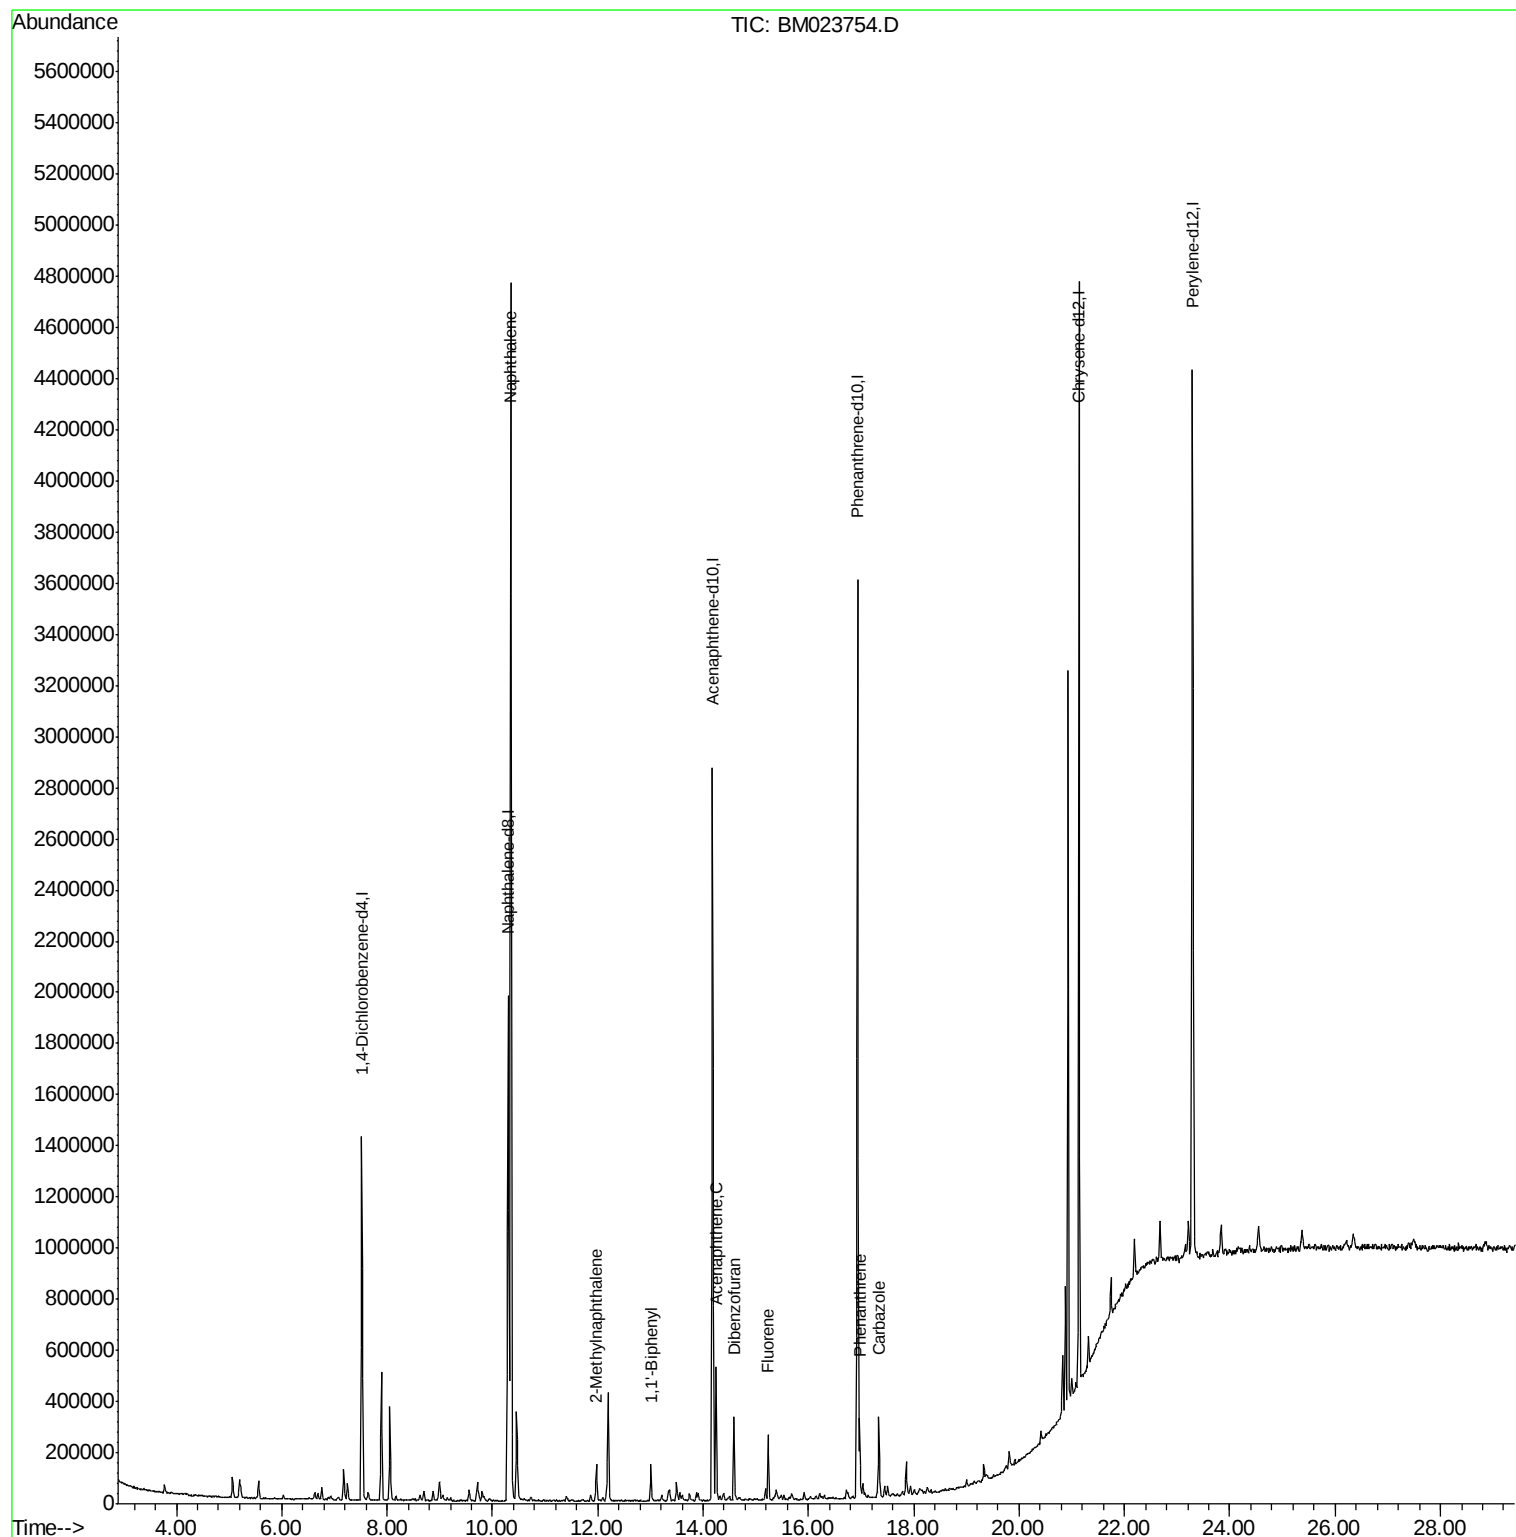

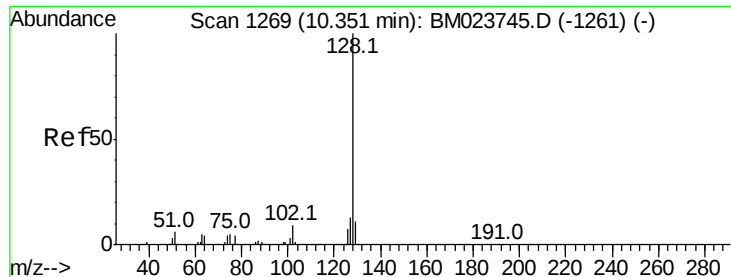

#28

Naphthalene

Concen: 46.679 ng/ul

RT: 10.35 min Scan# 1269

Delta R.T. 0.00 min

Lab File: BM023754.D

Acq: 15 Nov 2019 15:29

Instrument :

BNA_M

ClientSampleId :

BEGY8DL2


Tot Ion:128 Resp: 3933023

Ion Ratio Lower Upper

128 100

129 10.8 8.7 13.1




127 13.1 10.6 16.0

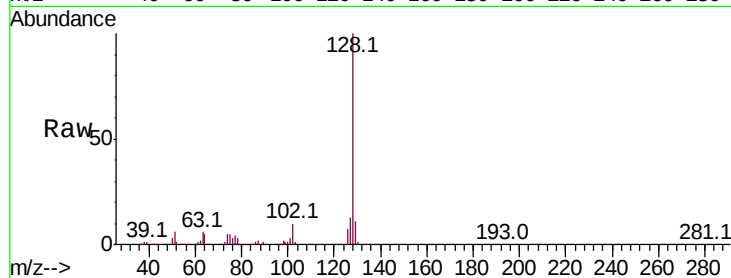

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

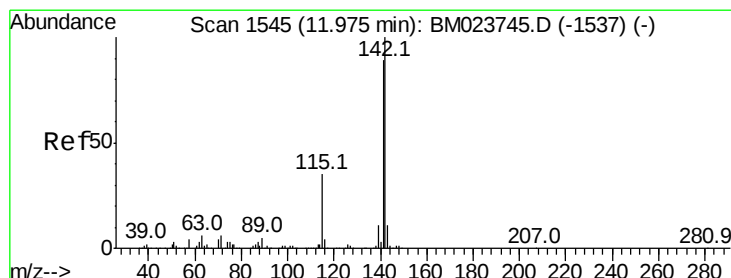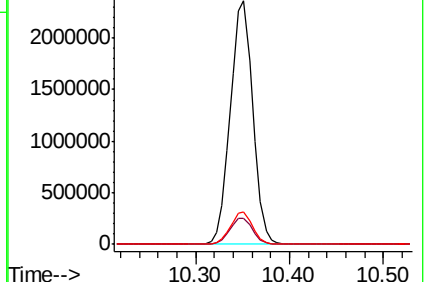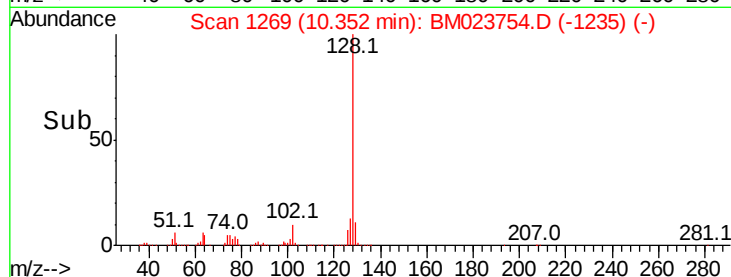

#34

2-Methylnaphthalene

Concen: 1.022 ng/ul

RT: 11.97 min Scan# 1545

Delta R.T. -0.01 min

Lab File: BM023754.D


Acq: 15 Nov 2019 15:29

Tgt Ion:142 Resp: 65841

Ion Ratio Lower Upper



142 100


141 93.2 69.8 104.8

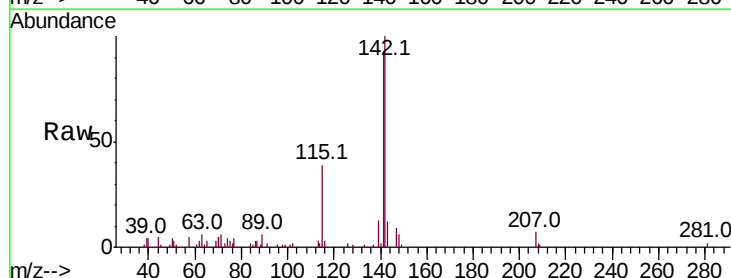

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

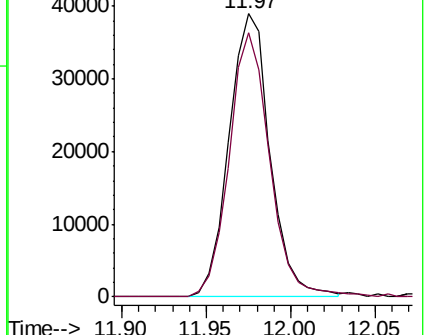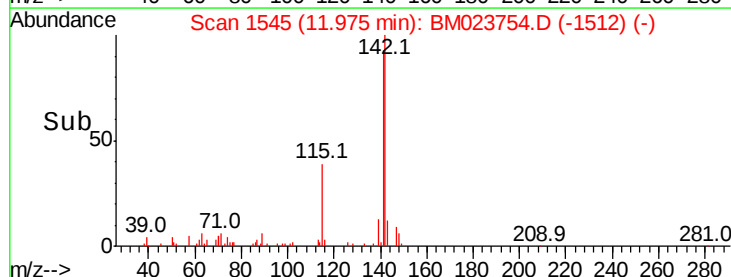

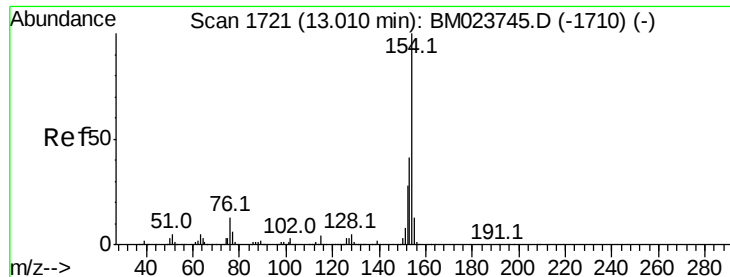

#41

1,1'-Biphenyl

Concen: 1.048 ng/ul

RT: 13.01 min Scan# 1721

Delta R.T. 0.00 min

Lab File: BM023754.D

Acq: 15 Nov 2019 15:29

Instrument :

BNA_M

ClientSampleId :

BEGY8DL2


Tot Ion:154 Resp: 78213

Ion Ratio Lower Upper

154 100

153 41.0 32.3 48.5




76 13.7 10.6 15.8

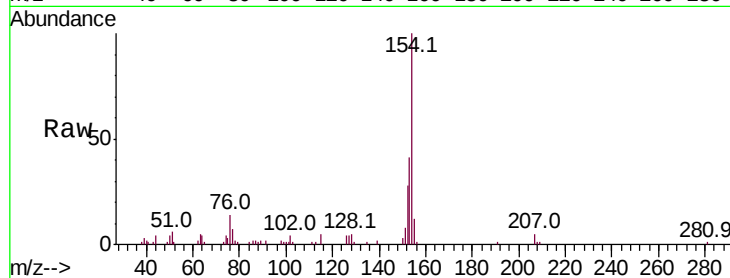

Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 76.00 (75.70 to 76.70): BM

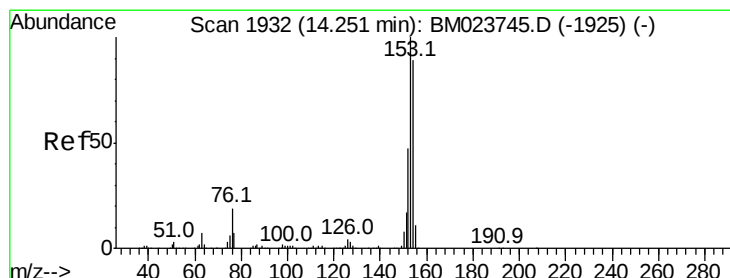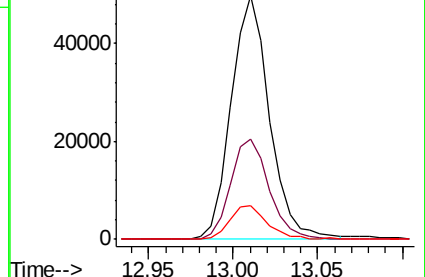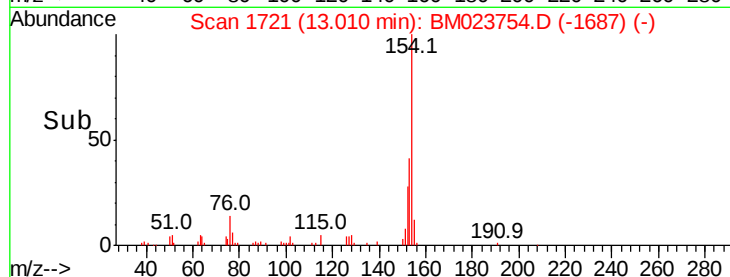

#50

Acenaphthene

Concen: 3.313 ng/ul

RT: 14.25 min Scan# 1931

Delta R.T. -0.01 min

Lab File: BM023754.D

Acq: 15 Nov 2019 15:29


Tgt Ion:153 Resp: 203744

Ion Ratio Lower Upper

153 100

152 48.2 37.7 56.5



154 88.1 70.6 106.0

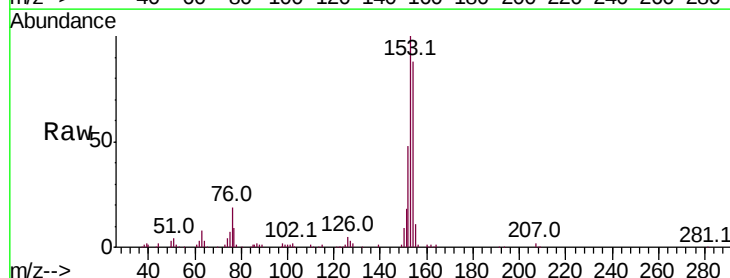


Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

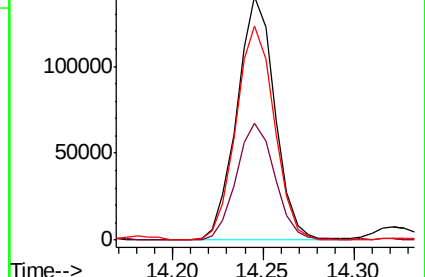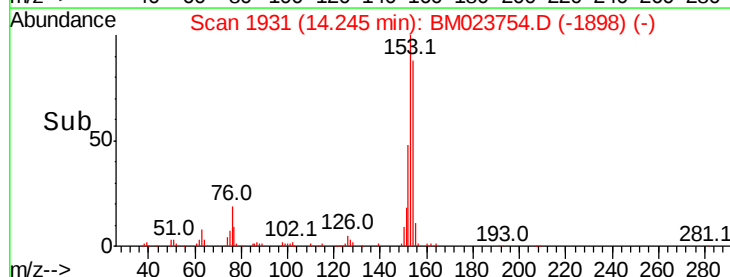

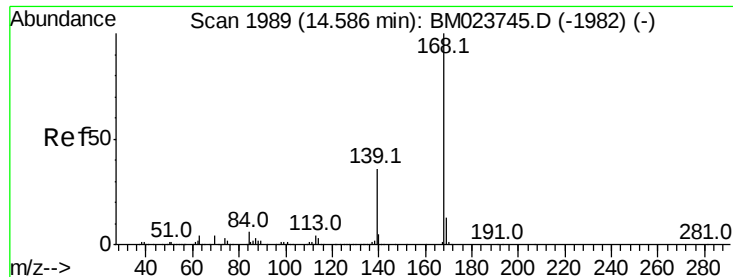

#54

Dibenzofuran

Concen: 2.280 ng/ul

RT: 14.59 min Scan# 1989

Delta R.T. 0.00 min

Lab File: BM023754.D

Acq: 15 Nov 2019 15:29

Instrument :

BNA_M

ClientSampleId :


BEGY8DL2

Tot Ion:168 Resp: 207543

Ion Ratio Lower Upper

168 100

139 36.7 29.3 43.9

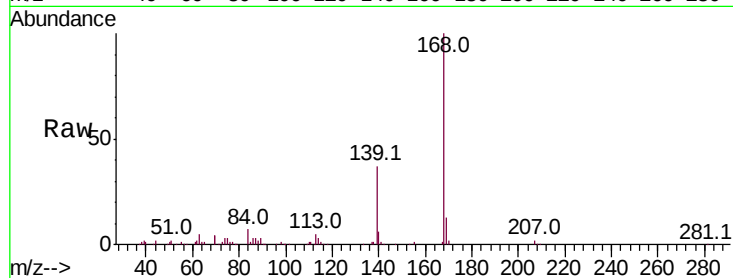

Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

150000



100000

50000

0

14.55 14.60 14.65

Time-->

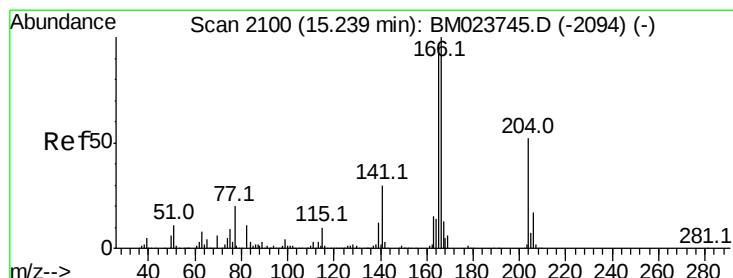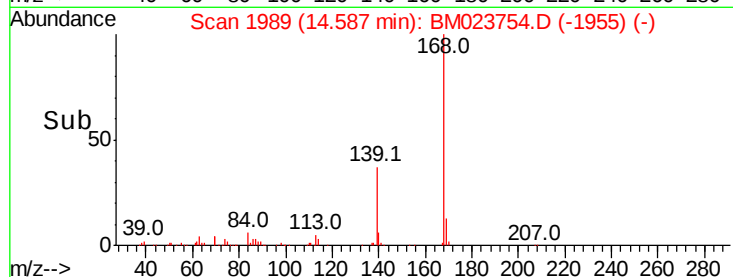

#59

Fluorene

Concen: 1.538 ng/ul

RT: 15.24 min Scan# 2100

Delta R.T. 0.00 min

Lab File: BM023754.D

Acq: 15 Nov 2019 15:29


Tgt Ion:166 Resp: 113609

Ion Ratio Lower Upper

166 100

165 101.4 77.2 115.8

167 15.1 10.9 16.3

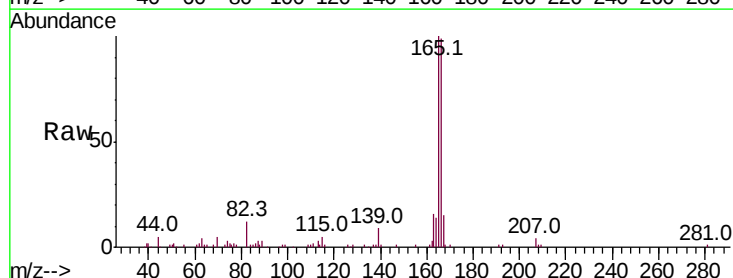

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

100000

80000

60000


40000


20000

0

15.20 15.25 15.30

Time-->

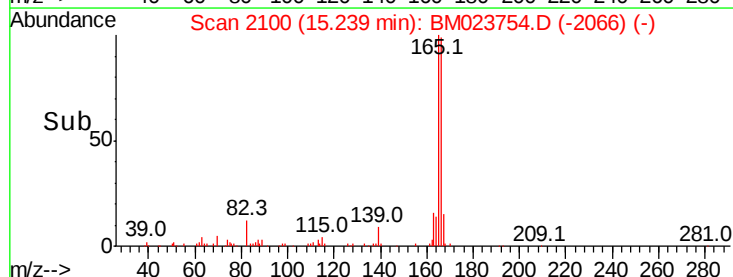

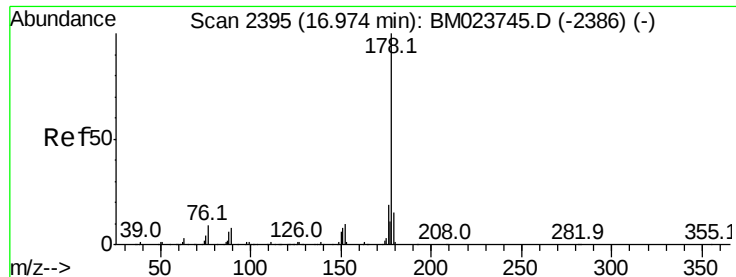

#70

Phenanthrene

Concen: 1.503 ng/ul

RT: 16.97 min Scan# 2395

Delta R.T. -0.01 min

Lab File: BM023754.D

Acq: 15 Nov 2019 15:29

Instrument :


BNA_M

ClientSampleId :

BEGY8DL2

Tot Ion:178 Resp: 165683

Ion	Ratio	Lower	Upper
178	100		
179	15.5	12.3	18.5
176	19.0	15.0	22.6



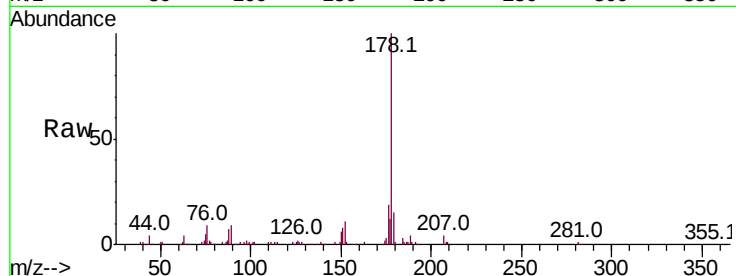


Abundance

Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

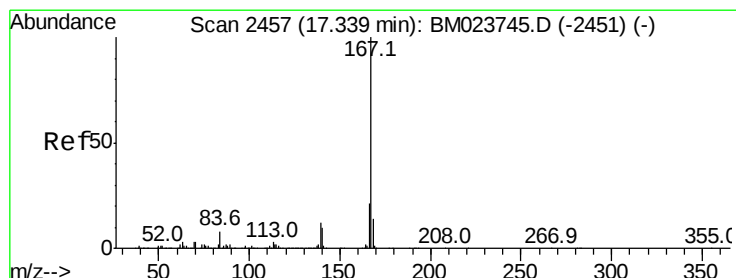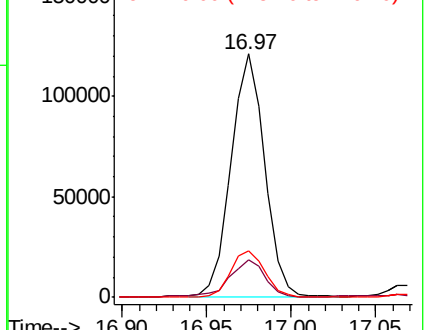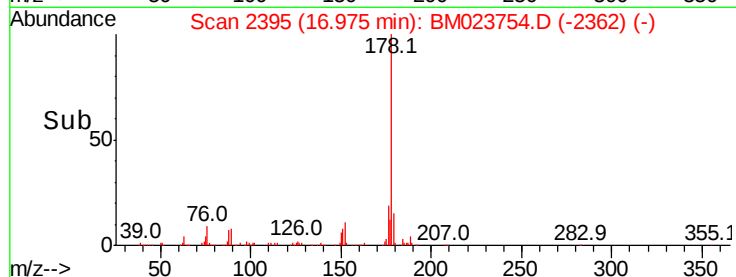

#75

Carbazole

Concen: 2.135 ng/ul

RT: 17.34 min Scan# 2457


Delta R.T. -0.01 min

Lab File: BM023754.D

Acq: 15 Nov 2019 15:29

Tgt Ion:167 Resp: 197371

Ion	Ratio	Lower	Upper
167	100		
166	21.8	17.1	25.7
139	12.8	9.8	14.6

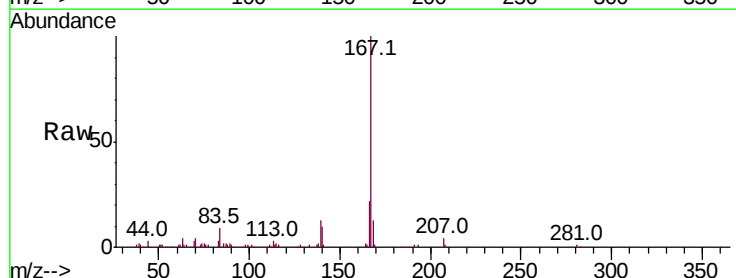

Abundance

Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

