


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM111518\
 Data File : BM017663.D
 Acq On : 15 Nov 2018 16:48
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 12 18:37:25 2018

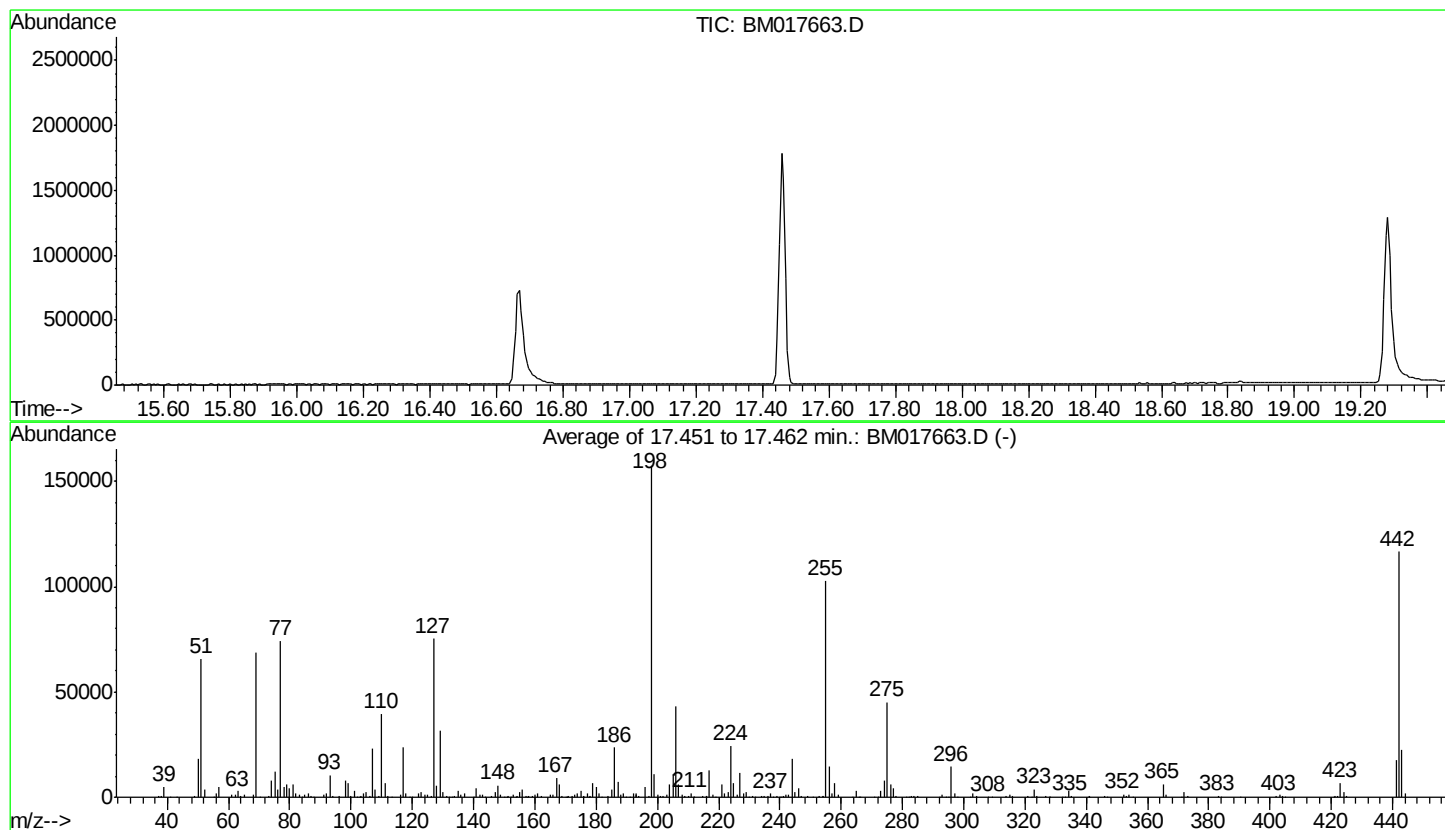

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	65666	PASS
68	69	0.00	2	2.0	1350	PASS
69	198	0.00	100	43.7	68741	PASS
70	69	0.00	2	0.4	279	PASS
127	198	10	80	47.8	75221	PASS
197	198	0.00	2	0.4	699	PASS
198	198	100	100	100.0	157450	PASS
199	198	5	9	7.0	11056	PASS
275	198	10	60	28.6	45024	PASS
365	198	1	100	4.1	6391	PASS
441	198	0.01	100	11.2	17616	PASS
442	198	50	100	74.0	116509	PASS
443	442	15	24	19.1	22221	PASS