




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111524\
Data File : BM048723.D
Acq On : 16 Nov 2024 00:25
Operator : RC/JU
Sample : P4751-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH9C8

Manual IntegrationsAPPROVED

Quant Time: Nov 16 01:05:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 15 16:55:33 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :mohammad ahmed 11/18/2024

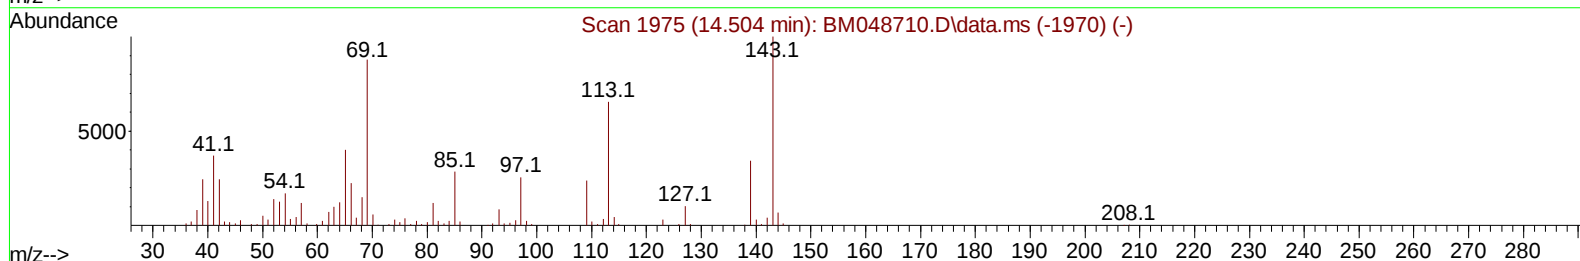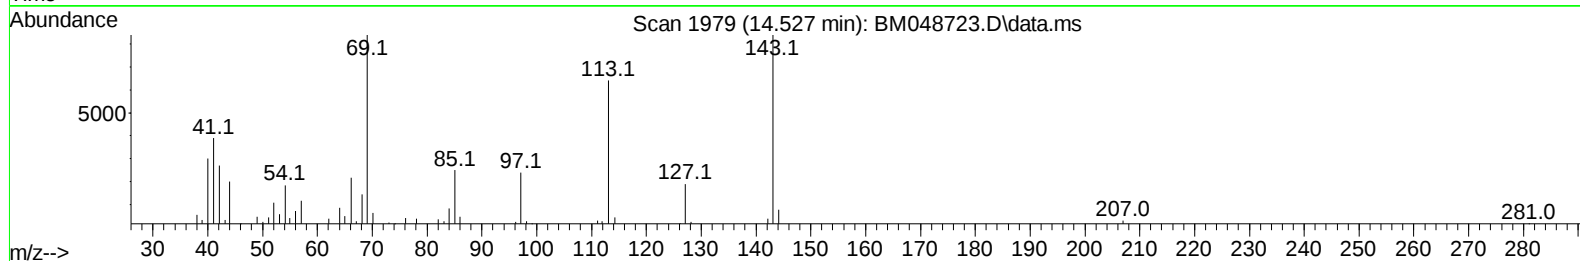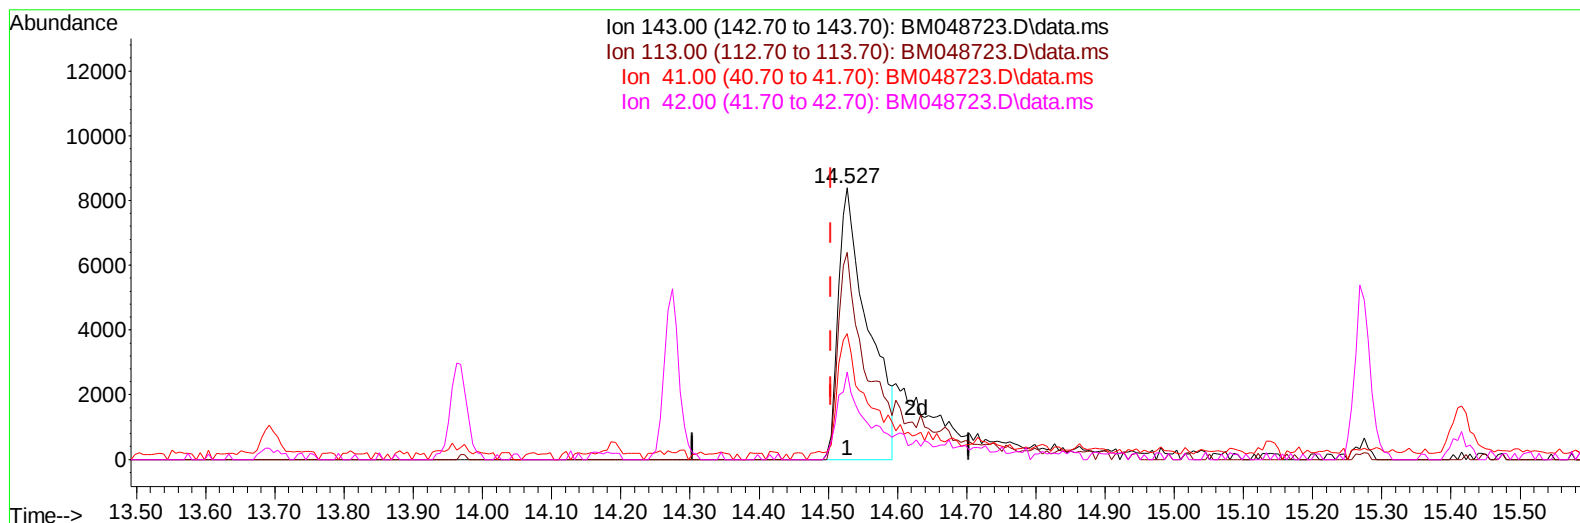

TIC: BM048723.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.527min (+ 0.023) 7.19 ng/u1

response 24846

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.50	76.37
41.00	36.20	46.36#
42.00	24.50	32.21#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111524\
Data File : BM048723.D
Acq On : 16 Nov 2024 00:25
Operator : RC/JU
Sample : P4751-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH9C8

Manual IntegrationsAPPROVED

Quant Time: Nov 16 01:05:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 15 16:55:33 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :mohammad ahmed 11/18/2024

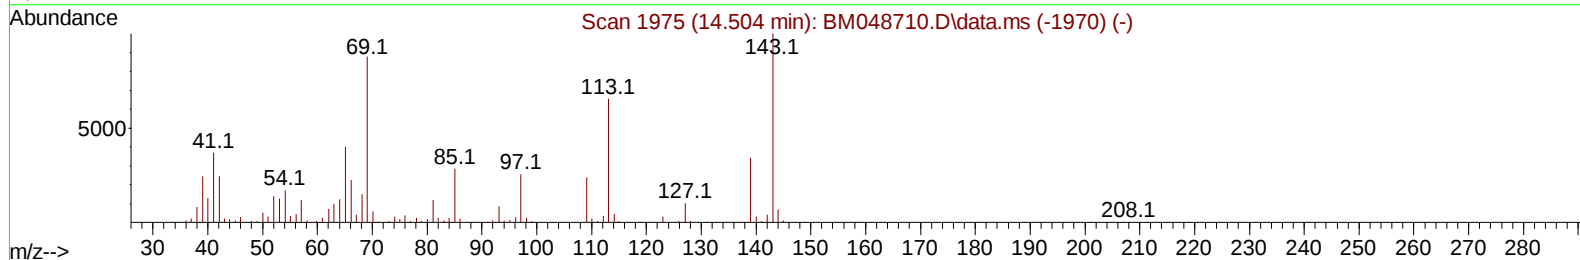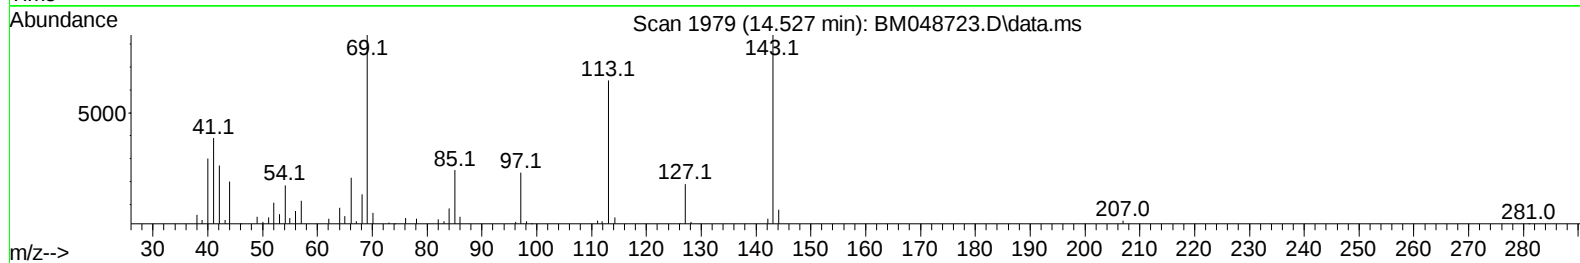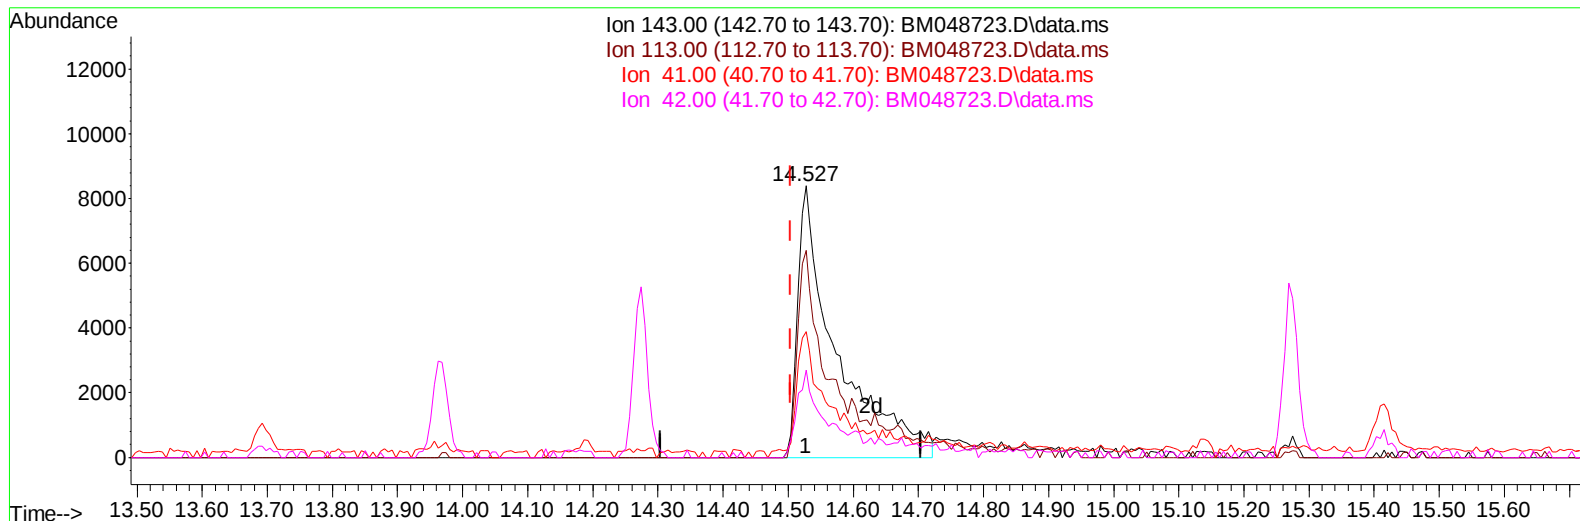

TIC: BM048723.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.527min (+ 0.023) 10.06 ng/ul m

response 34748

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.50	76.37
41.00	36.20	46.36#
42.00	24.50	32.21#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111524\
 Data File : BM048723.D
 Acq On : 16 Nov 2024 00:25
 Operator : RC/JU
 Sample : P4751-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH9C8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/18/2024
 Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 16 01:06:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 15 16:55:33 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	125456	20.000	ng/ul	0.00
20) Naphthalene-d8	10.404	136	489359	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.274	164	291460	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.021	188	590942	20.000	ng/ul	0.00
79) Chrysene-d12	21.250	240	575984	20.000	ng/ul	0.00
88) Perylene-d12	24.133	264	681917	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.087	96	9974	3.169	ng/uL	0.00
4) Pyridine-d5	3.504	84	116335	13.414	ng/ul	0.00
7) Phenol-d5	6.810	99	164704	17.246	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.963	67	99487	17.344	ng/ul	0.00
11) 2-Chlorophenol-d4	7.157	132	140837	17.803	ng/ul	0.00
15) 4-Methylphenol-d8	8.345	113	132871	17.694	ng/ul	0.00
21) Nitrobenzene-d5	8.781	128	64874	18.291	ng/ul	0.00
24) 2-Nitrophenol-d4	9.504	143	66688	17.677	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.045	165	123149	17.572	ng/ul	0.00
31) 4-Chloroaniline-d4	10.563	131	164800	16.555	ng/ul	0.00
46) Dimethylphthalate-d6	13.692	166	413852	22.244	ng/ul	0.00
49) Acenaphthylene-d8	13.969	160	457672	20.864	ng/ul	0.00
54) 4-Nitrophenol-d4	14.527	143	34748m	10.055	ng/ul	0.02
60) Fluorene-d10	15.274	176	353926	21.793	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.415	200	32735	11.012	ng/ul	0.00
73) Anthracene-d10	17.121	188	552052	22.076	ng/ul	0.00
81) Pyrene-d10	19.421	212	681554	23.578	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.938	264	719381	22.578	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111524\
Data File : BM048723.D
Acq On : 16 Nov 2024 00:25
Operator : RC/JU
Sample : P4751-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH9C8

Manual IntegrationsAPPROVED

Quant Time: Nov 16 01:06:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 15 16:55:33 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :mohammad ahmed 11/18/2024

