

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111524\
 Data File : BM048713.D
 Acq On : 15 Nov 2024 17:49
 Operator : RC/JU
 Sample : P4751-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH9E6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/18/2024
 Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 15 22:46:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 15 16:55:33 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	112577	20.000	ng/u1	0.00
20) Naphthalene-d8	10.410	136	437444	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.274	164	253130	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.021	188	505632	20.000	ng/u1	0.00
79) Chrysene-d12	21.244	240	510297	20.000	ng/u1	0.00
88) Perylene-d12	24.132	264	617739	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.087	96	3975	1.408	ng/uL	0.00
4) Pyridine-d5	3.522	84	15773m	2.027	ng/u1	0.02
7) Phenol-d5	6.816	99	47497	5.542	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	6.963	67	33466	6.502	ng/u1	0.00
11) 2-Chlorophenol-d4	7.163	132	45855	6.459	ng/u1	0.00
15) 4-Methylphenol-d8	8.357	113	26340	3.909	ng/u1	0.02
21) Nitrobenzene-d5	8.786	128	19311	6.091	ng/u1	0.00
24) 2-Nitrophenol-d4	9.510	143	19230	5.702	ng/u1	0.01
28) 2,4-Dichlorophenol-d3	10.069	165	35961m	5.740	ng/u1	0.03
31) 4-Chloroaniline-d4	10.592	131	24264m	2.727	ng/u1	0.04
46) Dimethylphthalate-d6	13.698	166	119876	7.419	ng/u1	0.00
49) Acenaphthylene-d8	13.968	160	132485	6.954	ng/u1	0.00
54) 4-Nitrophenol-d4	14.598	143	6755m	2.251	ng/u1	0.09
60) Fluorene-d10	15.274	176	104409	7.402	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.421	200	7555m	2.970	ng/u1	0.01
73) Anthracene-d10	17.127	188	130477	6.098	ng/u1	0.00
81) Pyrene-d10	19.421	212	155988	6.091	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.933	264	117948	4.087	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.463	105	38627	3.677	ng/u1	98
72) Phenanthrene	17.068	178	54070	2.156	ng/u1	98
80) Fluoranthene	19.086	202	113358	3.815	ng/u1#	96
82) Pyrene	19.450	202	76083	2.361	ng/u1	99
85) Benzo(a)anthracene	21.227	228	64211	1.996	ng/u1	99
87) Chrysene	21.291	228	64253	2.079	ng/u1	99
90) Benzo(b)fluoranthene	23.227	252	89554	2.634	ng/u1	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111524\
Data File : BM048713.D
Acq On : 15 Nov 2024 17:49
Operator : RC/JU
Sample : P4751-07
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BH9E6

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 15 22:46:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 15 16:55:33 2024
Response via : Initial Calibration

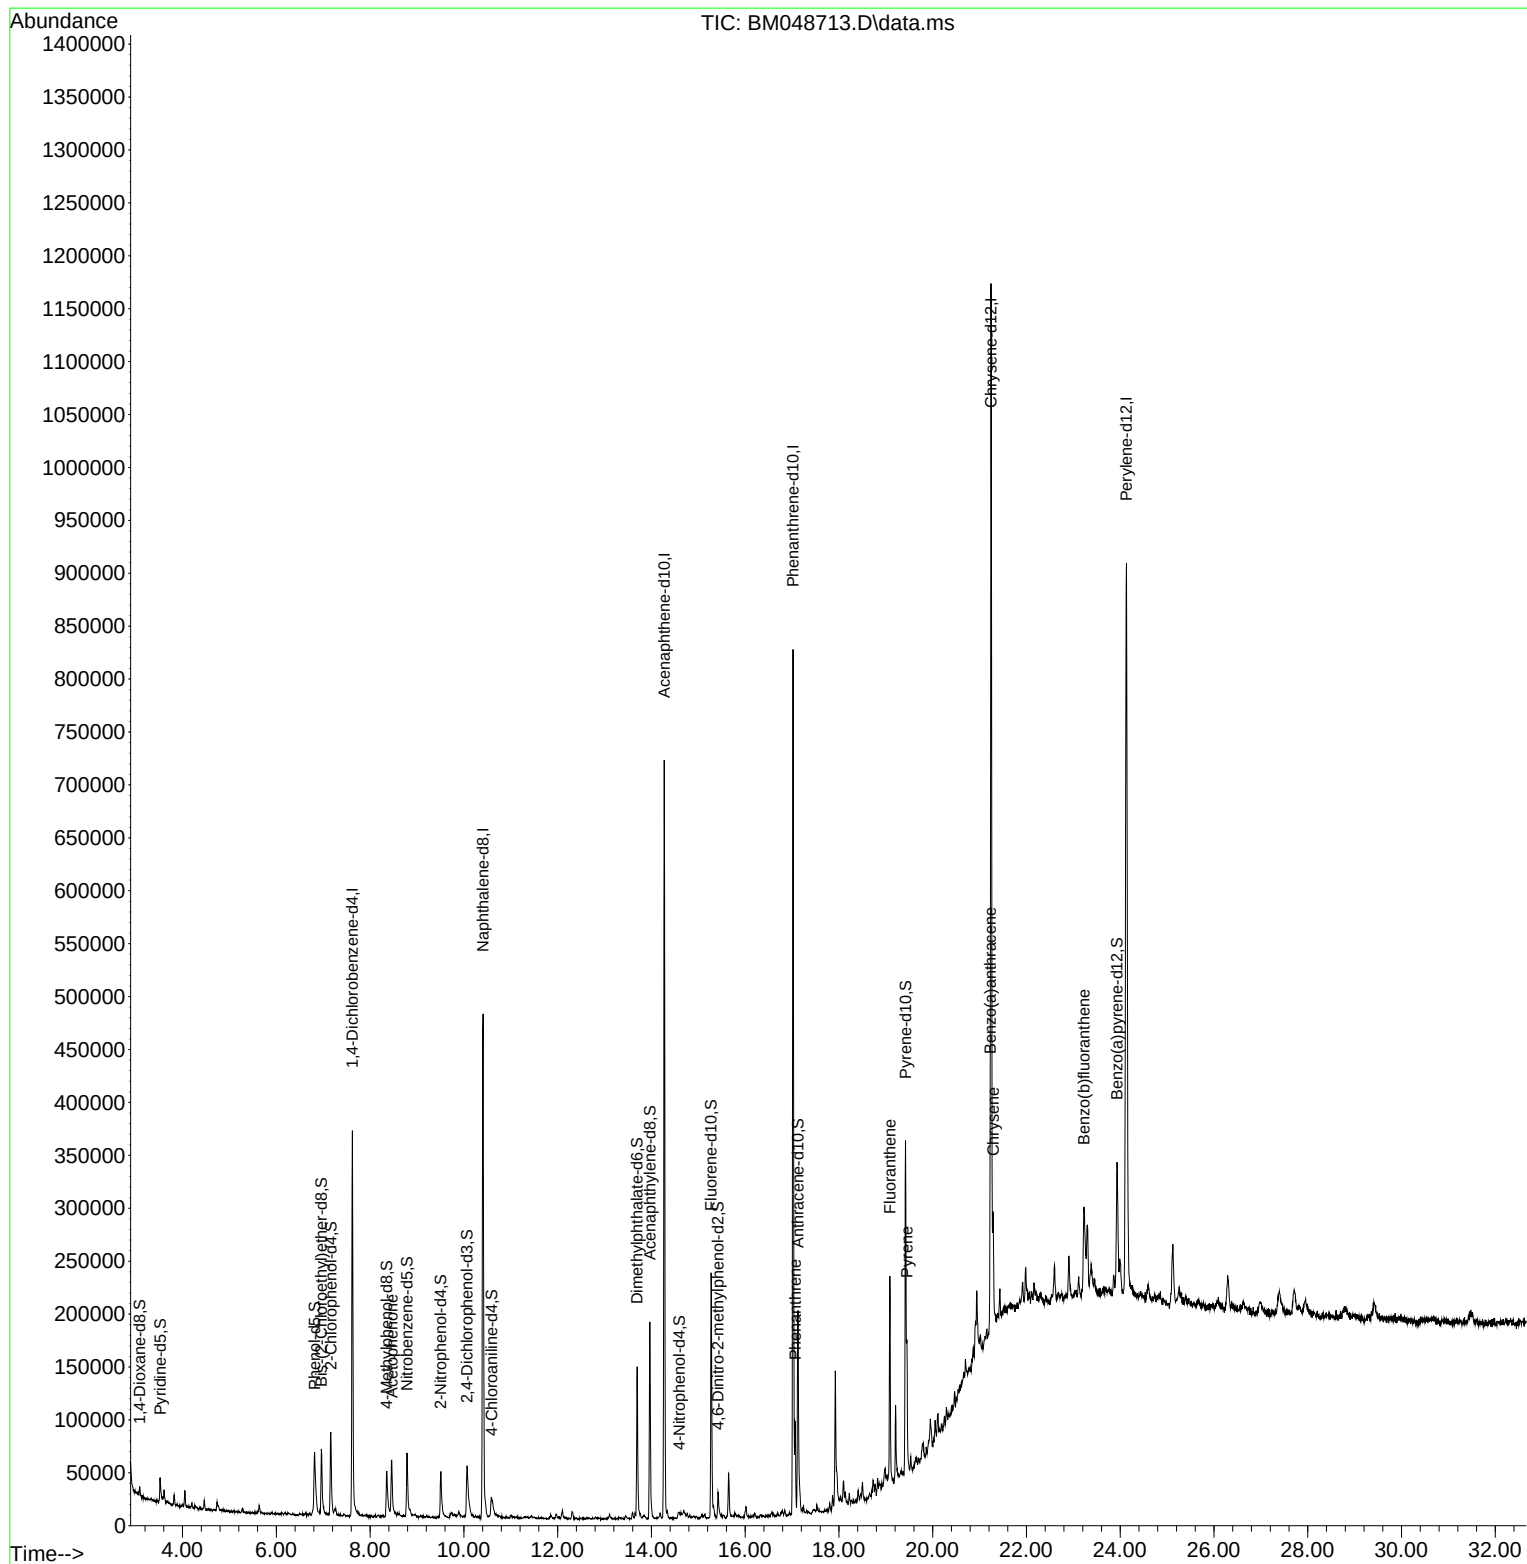

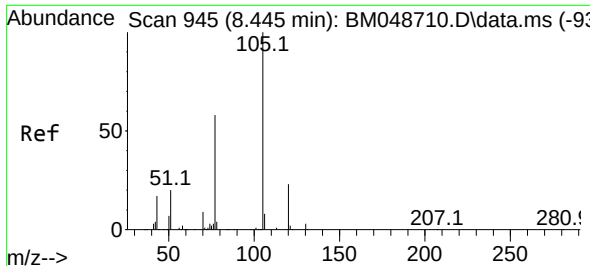





#16
Acetophenone
Concen: 3.677 ng/ul
RT: 8.463 min Scan# 945
Delta R.T. 0.018 min
Lab File: BM048713.D
Acq: 15 Nov 2024 17:49

Instrument :
BNA_M
ClientSampleId :
BH9E6

Tgt Ion:105 Resp: 3862
Ion Ratio Lower Upper
105 100
77 75.8 59.7 89.5
51 27.0 20.6 31.0




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 11/18/2024
Supervised By :mohammad ahmed 11/18/2024

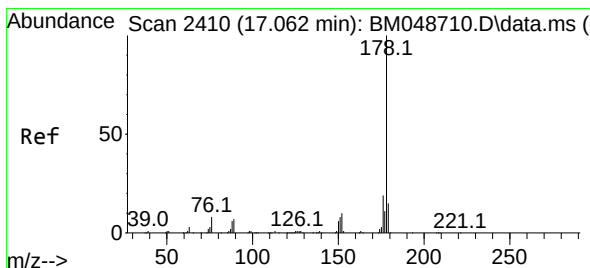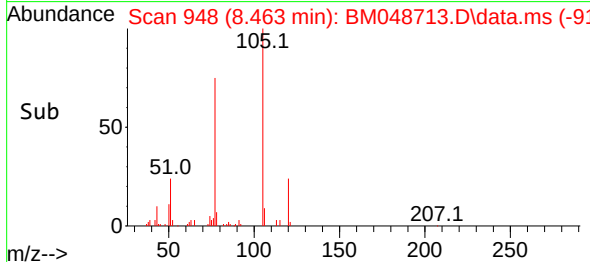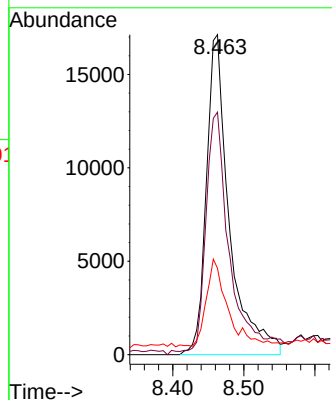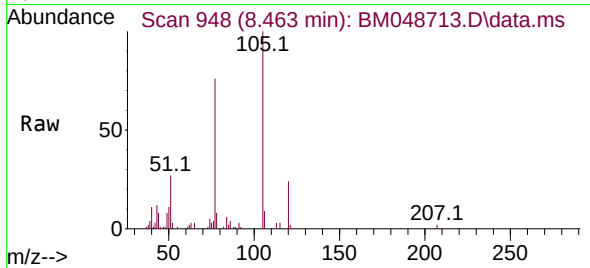

#72
Phenanthrene
Concen: 2.156 ng/ul
RT: 17.068 min Scan# 2411
Delta R.T. 0.006 min
Lab File: BM048713.D
Acq: 15 Nov 2024 17:49


Tgt Ion:178 Resp: 54070
Ion Ratio Lower Upper
178 100
179 15.7 12.0 18.0
176 19.9 15.1 22.7

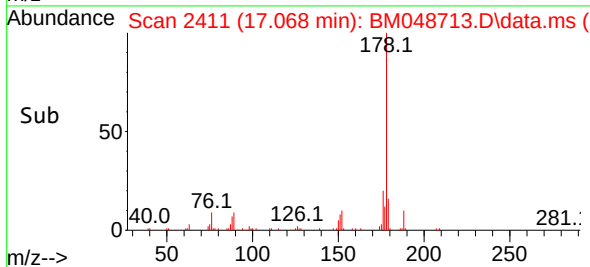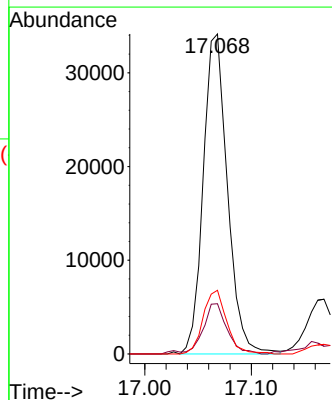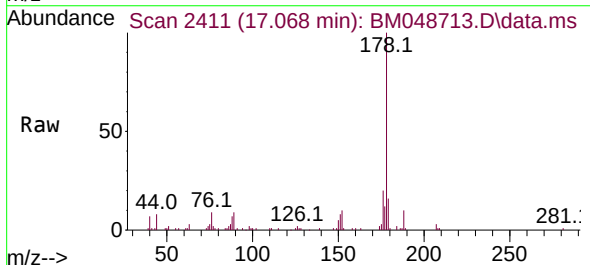

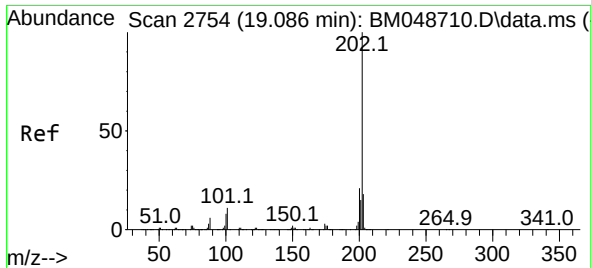

#80
Fluoranthene
Concen: 3.815 ng/ul
RT: 19.086 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM048713.D
Acq: 15 Nov 2024 17:49




Instrument :
BNA_M
ClientSampleId :
BH9E6

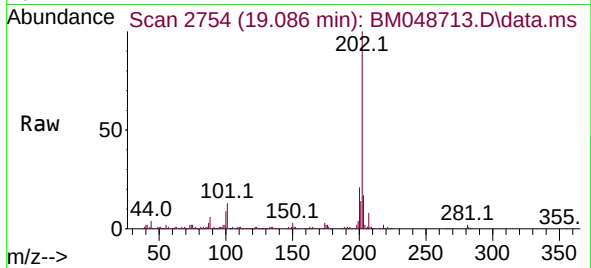

Tgt Ion:202 Resp: 113358
Ion Ratio Lower Upper
202 100
101 13.1 8.5 12.7
100 9.0 7.0 10.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 11/18/2024
Supervised By :mohammad ahmed 11/18/2024

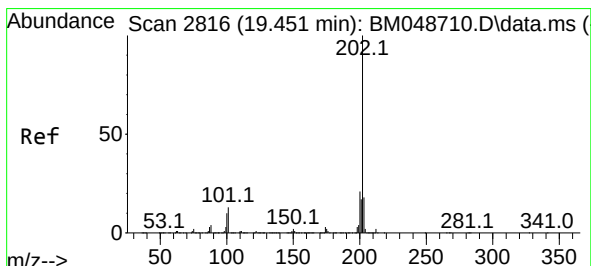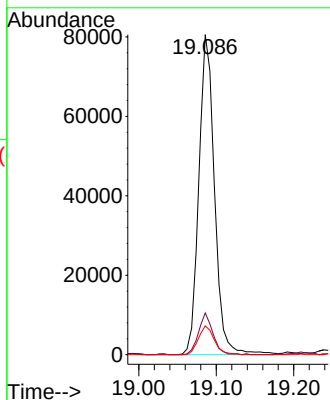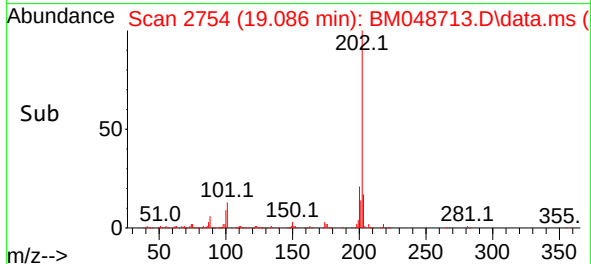

#82
Pyrene
Concen: 2.361 ng/ul
RT: 19.450 min Scan# 2816
Delta R.T. -0.000 min
Lab File: BM048713.D
Acq: 15 Nov 2024 17:49

Tgt Ion:202 Resp: 76083
Ion Ratio Lower Upper
202 100
101 13.0 10.6 15.8
100 10.8 8.9 13.3

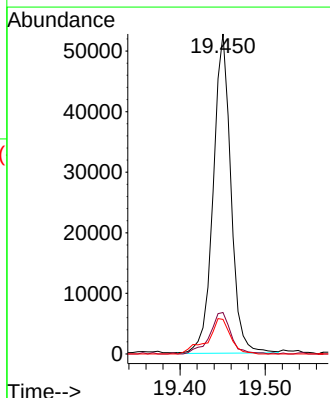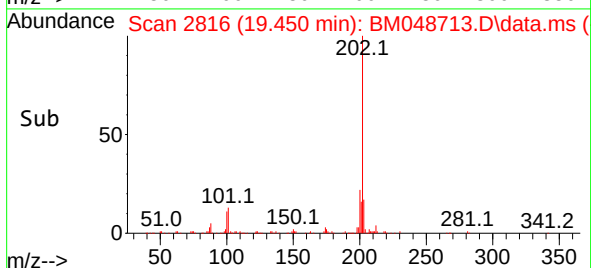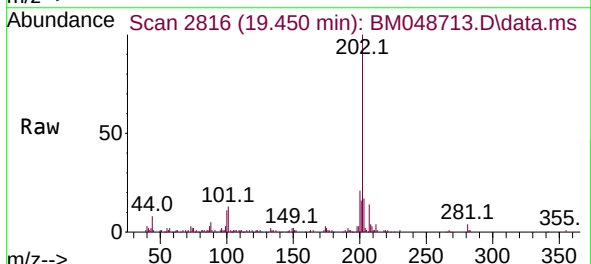

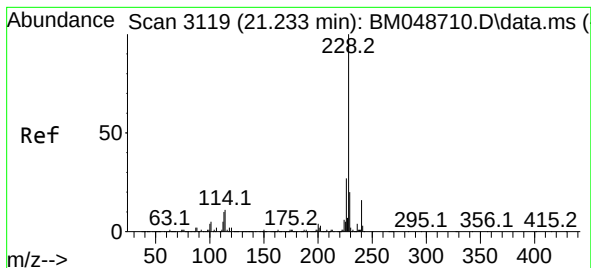

#85

Benzo(a)anthracene

Concen: 1.996 ng/ul

RT: 21.227 min Scan# 3119

Delta R.T. -0.006 min

Lab File: BM048713.D

Acq: 15 Nov 2024 17:49

Instrument :

BNA_M

ClientSampleId :

BH9E6

Tgt Ion:228 Resp: 6421





Ion	Ratio	Lower	Upper
228	100		
229	20.3	15.7	23.5
226	27.7	21.7	32.5

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 11/18/2024

Supervised By :mohammad ahmed 11/18/2024

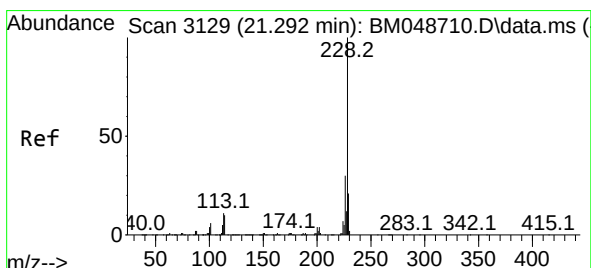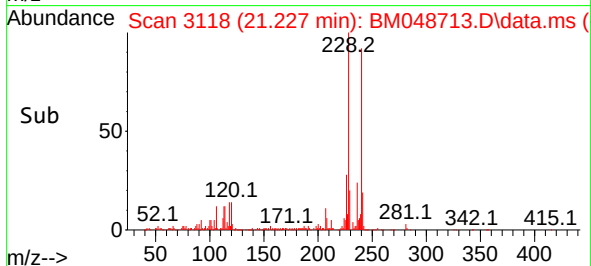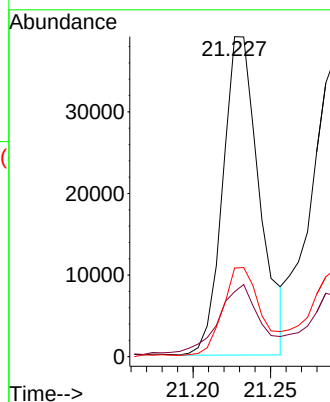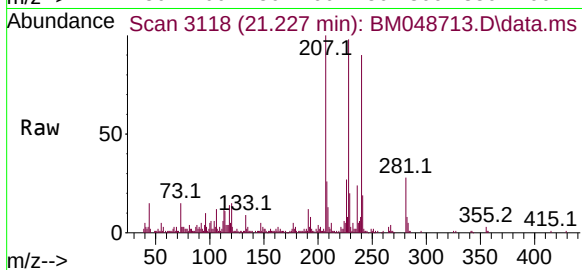

#87

Chrysene

Concen: 2.079 ng/ul

RT: 21.291 min Scan# 3129




Delta R.T. -0.000 min


Lab File: BM048713.D

Acq: 15 Nov 2024 17:49

Tgt Ion:228 Resp: 64253


Ion	Ratio	Lower	Upper
228	100		
226	29.2	23.4	35.2
229	20.4	15.6	23.4

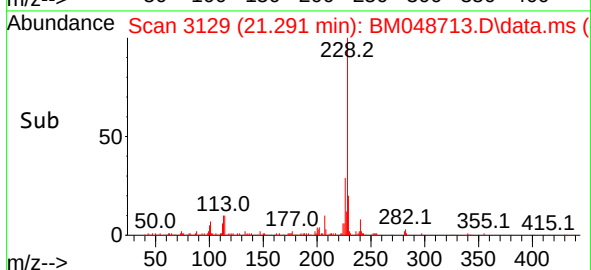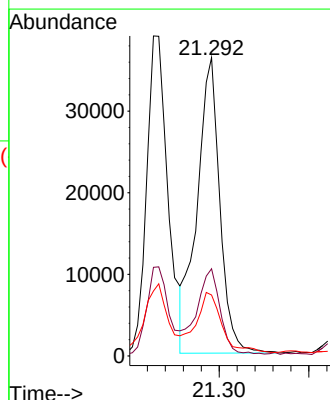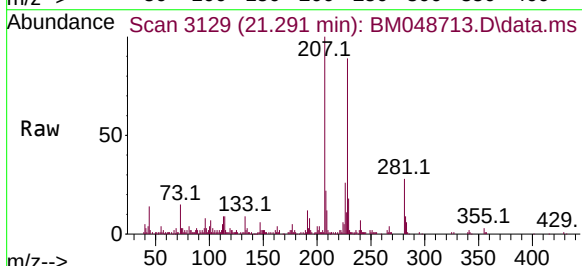

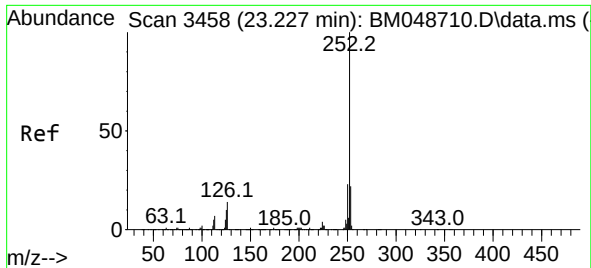

#90
Benzo(b)fluoranthene
Concen: 2.634 ng/ul
RT: 23.227 min Scan# 34
Delta R.T. -0.000 min
Lab File: BM048713.D
Acq: 15 Nov 2024 17:49

Instrument :
BNA_M
ClientSampleId :
BH9E6

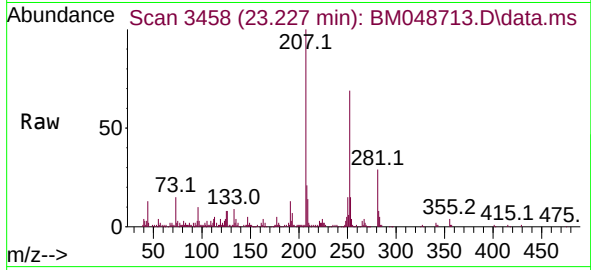

Tgt Ion:252 Resp: 89554
Ion Ratio Lower Upper
252 100
253 22.6 17.7 26.5
125 11.3 8.7 13.1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :mohammad ahmed 11/18/2024

