

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111524\
 Data File : BM048711.D
 Acq On : 15 Nov 2024 16:31
 Operator : RC/JU
 Sample : PB164821BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK821

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048711.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.087	30	34	39	rBV	30714	39193	1.76%	0.179%
2	3.499	101	104	122	rBV	327289	544247	24.44%	2.487%
3	3.822	156	159	164	rVB3	5491	5995	0.27%	0.027%
4	4.046	195	197	200	rBV3	2383	3569	0.16%	0.016%
5	4.281	234	237	238	rBV3	2533	2719	0.12%	0.012%
6	4.434	262	263	266	rBV3	1967	2387	0.11%	0.011%
7	4.681	301	305	308	rBV5	1783	2669	0.12%	0.012%
8	6.804	657	666	685	rBV	333257	611027	27.44%	2.792%
9	6.963	687	693	708	rVB	293292	503038	22.59%	2.299%
10	7.157	719	726	740	rBV	379774	659355	29.61%	3.013%
11	7.622	798	805	814	rBV	348604	578875	26.00%	2.645%
12	8.346	921	928	945	rBV	387449	734152	32.97%	3.355%
13	8.781	995	1002	1017	rBV	319552	570330	25.61%	2.606%
14	9.504	1117	1125	1142	rBV	243077	462947	20.79%	2.116%
15	10.045	1210	1217	1226	rBV	324612	628334	28.22%	2.871%
16	10.404	1271	1278	1295	rBV	446515	785711	35.29%	3.590%
17	10.563	1298	1305	1324	rBV	238828	665431	29.89%	3.041%
18	11.675	1490	1494	1498	rVB4	1394	2318	0.10%	0.011%
19	12.039	1553	1556	1559	rBV4	3433	5501	0.25%	0.025%
20	13.692	1831	1837	1853	rVB	621274	965866	43.38%	4.414%
21	13.969	1877	1884	1899	rBV	798187	1225124	55.02%	5.598%
22	14.275	1930	1936	1948	rBV	635160	956211	42.94%	4.370%
23	14.357	1948	1950	1954	rVV4	1475	2374	0.11%	0.011%
24	14.522	1971	1978	2000	rBV	99744	320407	14.39%	1.464%
25	15.274	2099	2106	2115	rBV	1024536	1479377	66.44%	6.760%
26	15.410	2123	2129	2142	rBV	219908	377131	16.94%	1.723%
27	15.516	2144	2147	2152	rVB6	6730	11228	0.50%	0.051%
28	15.851	2200	2204	2209	rVB7	1442	2765	0.12%	0.013%
29	16.821	2364	2369	2372	rVV6	1779	3257	0.15%	0.015%
30	16.980	2392	2396	2397	rBV4	2132	2320	0.10%	0.011%
31	17.021	2397	2403	2414	rVV	745315	1074201	48.24%	4.909%
32	17.121	2414	2420	2439	rVB	946772	1565266	70.30%	7.153%
33	17.316	2452	2453	2460	rBV6	1736	2555	0.11%	0.012%
34	17.580	2495	2498	2500	rBV4	2237	2339	0.11%	0.011%
35	17.886	2547	2550	2553	rBV4	2037	3057	0.14%	0.014%
36	17.933	2553	2558	2568	rBV7	16734	43525	1.95%	0.199%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111524\
Data File : BM048711.D
Acq On : 15 Nov 2024 16:31
Operator : RC/JU
Sample : PB164821BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK821

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Title : SVOA CALIBRATION

37	18.986	2733	2737	2741	rBV3	12671	18180	0.82%	0.083%
38	19.062	2746	2750	2754	rBV2	10086	15058	0.68%	0.069%
39	19.221	2773	2777	2781	rBV7	10588	19720	0.89%	0.090%
40	19.421	2805	2811	2824	rBV	1307525	1934962	86.90%	8.842%
41	21.251	3117	3122	3137	rBV2	695708	1284514	57.69%	5.870%
42	23.939	3570	3579	3596	rBV	874288	2226619	100.00%	10.175%
43	24.139	3604	3613	3631	rBV	546645	1539544	69.14%	7.035%




Sum of corrected areas: 21883398

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111524\
Data File : BM048711.D
Acq On : 15 Nov 2024 16:31
Operator : RC/JU
Sample : PB164821BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK821

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

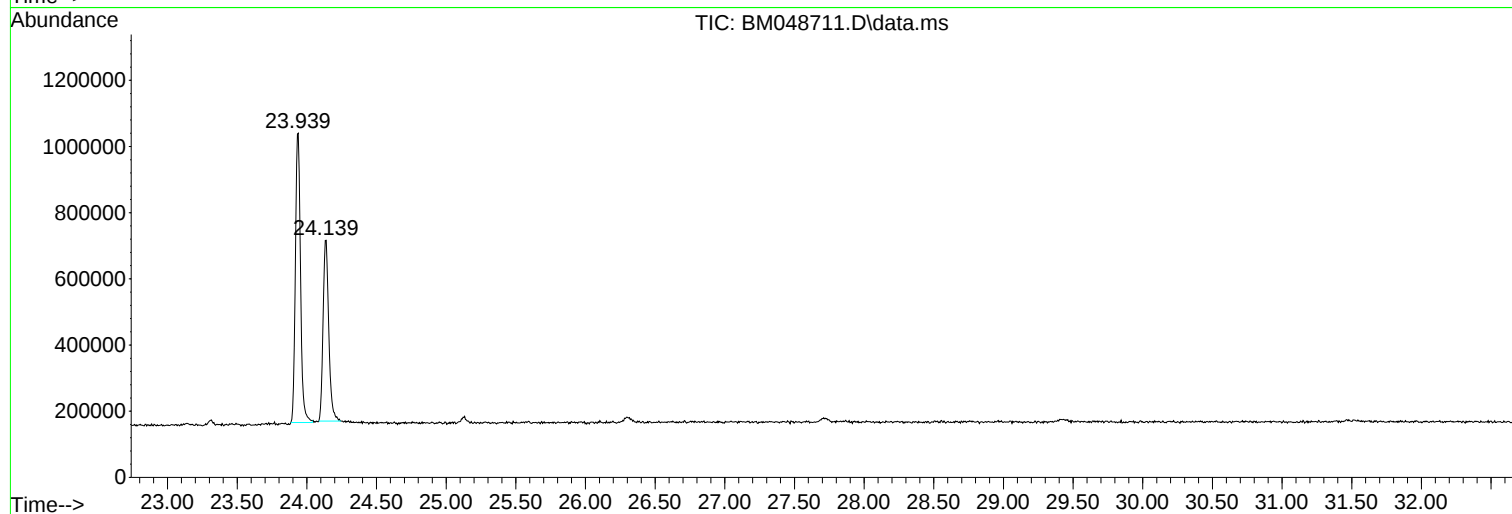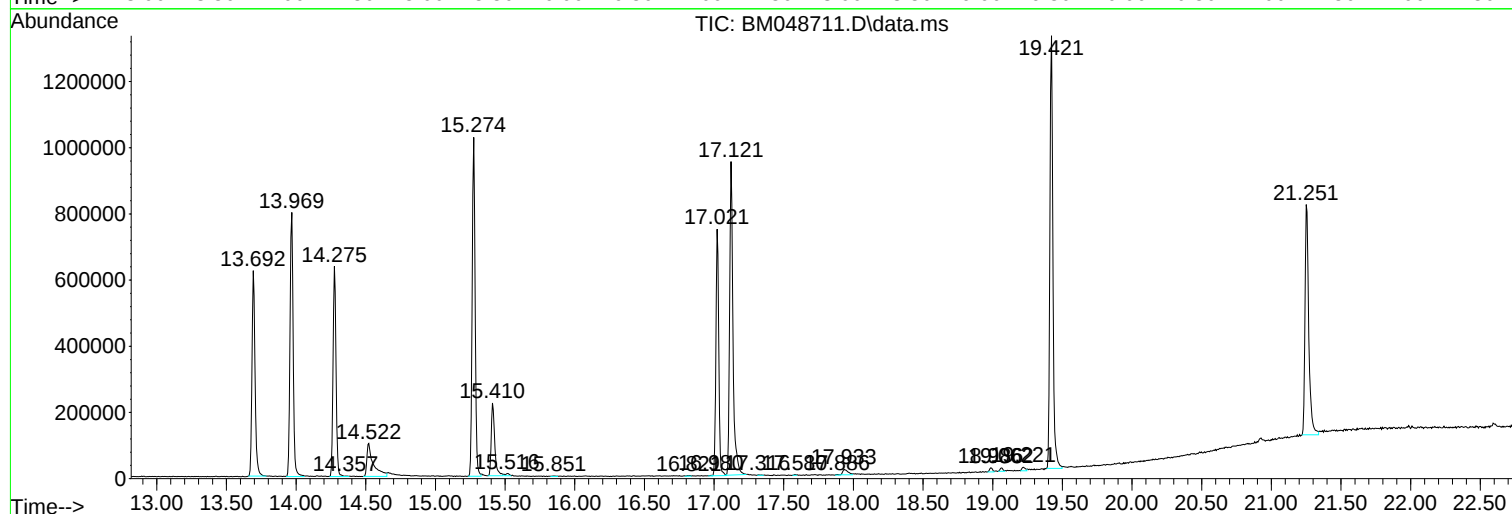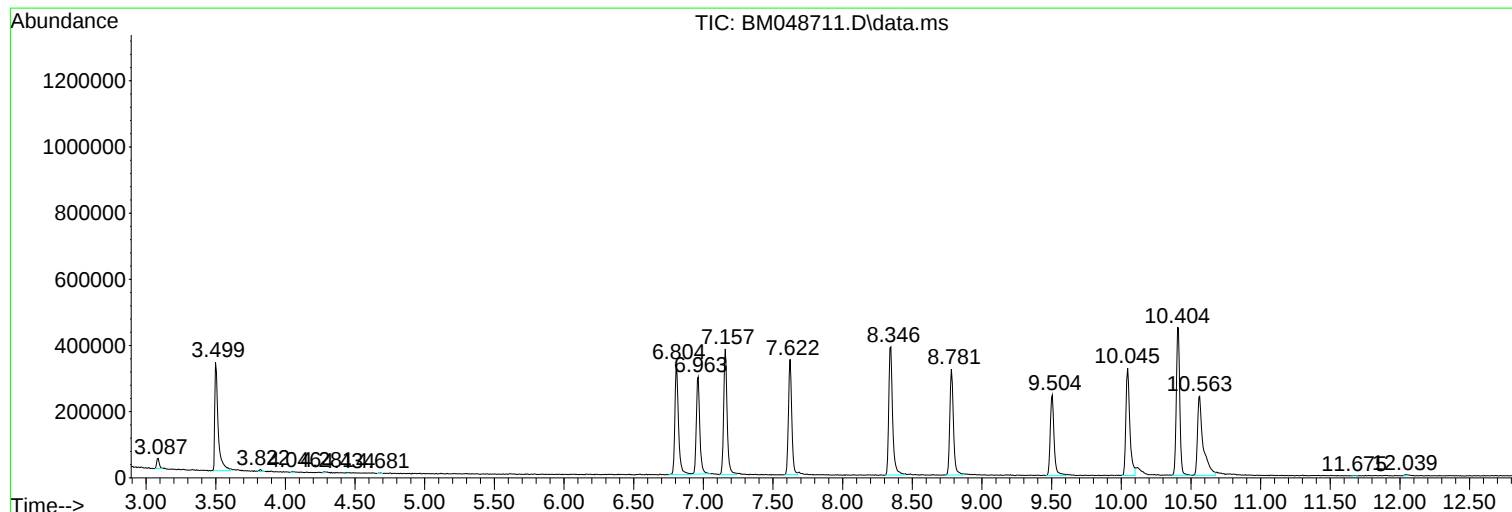

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111524\
Data File : BM048711.D
Acq On : 15 Nov 2024 16:31
Operator : RC/JU
Sample : PB164821BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK821

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111524\
Data File : BM048711.D
Acq On : 15 Nov 2024 16:31
Operator : RC/JU
Sample : PB164821BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK821

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc