

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111624\
 Data File : BM048740.D
 Acq On : 16 Nov 2024 14:03
 Operator : RC/JU
 Sample : P4803-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A0AP4

Quant Time: Nov 17 22:48:18 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Nov 17 22:31:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.629	152	4144	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.410	136	12908	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.276	164	6575	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.121	188	889683	0.400	ng/ul	0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.23
23) Perylene-d12	23.426	264	12156	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.089	96	22839	4.568	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.026	152	4718	0.283	ng/ul	-0.02
18) Fluoranthene-d10	19.059	212	9990	0.000	ng/ul	-0.01
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.123	88	1306	0.227	ng/ul#	81
26) Benzo(a)pyrene	23.277	252	2868	0.078	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111624\
Data File : BM048740.D
Acq On : 16 Nov 2024 14:03
Operator : RC/JU
Sample : P4803-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A0AP4

Quant Time: Nov 17 22:48:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 17 22:31:02 2024
Response via : Initial Calibration




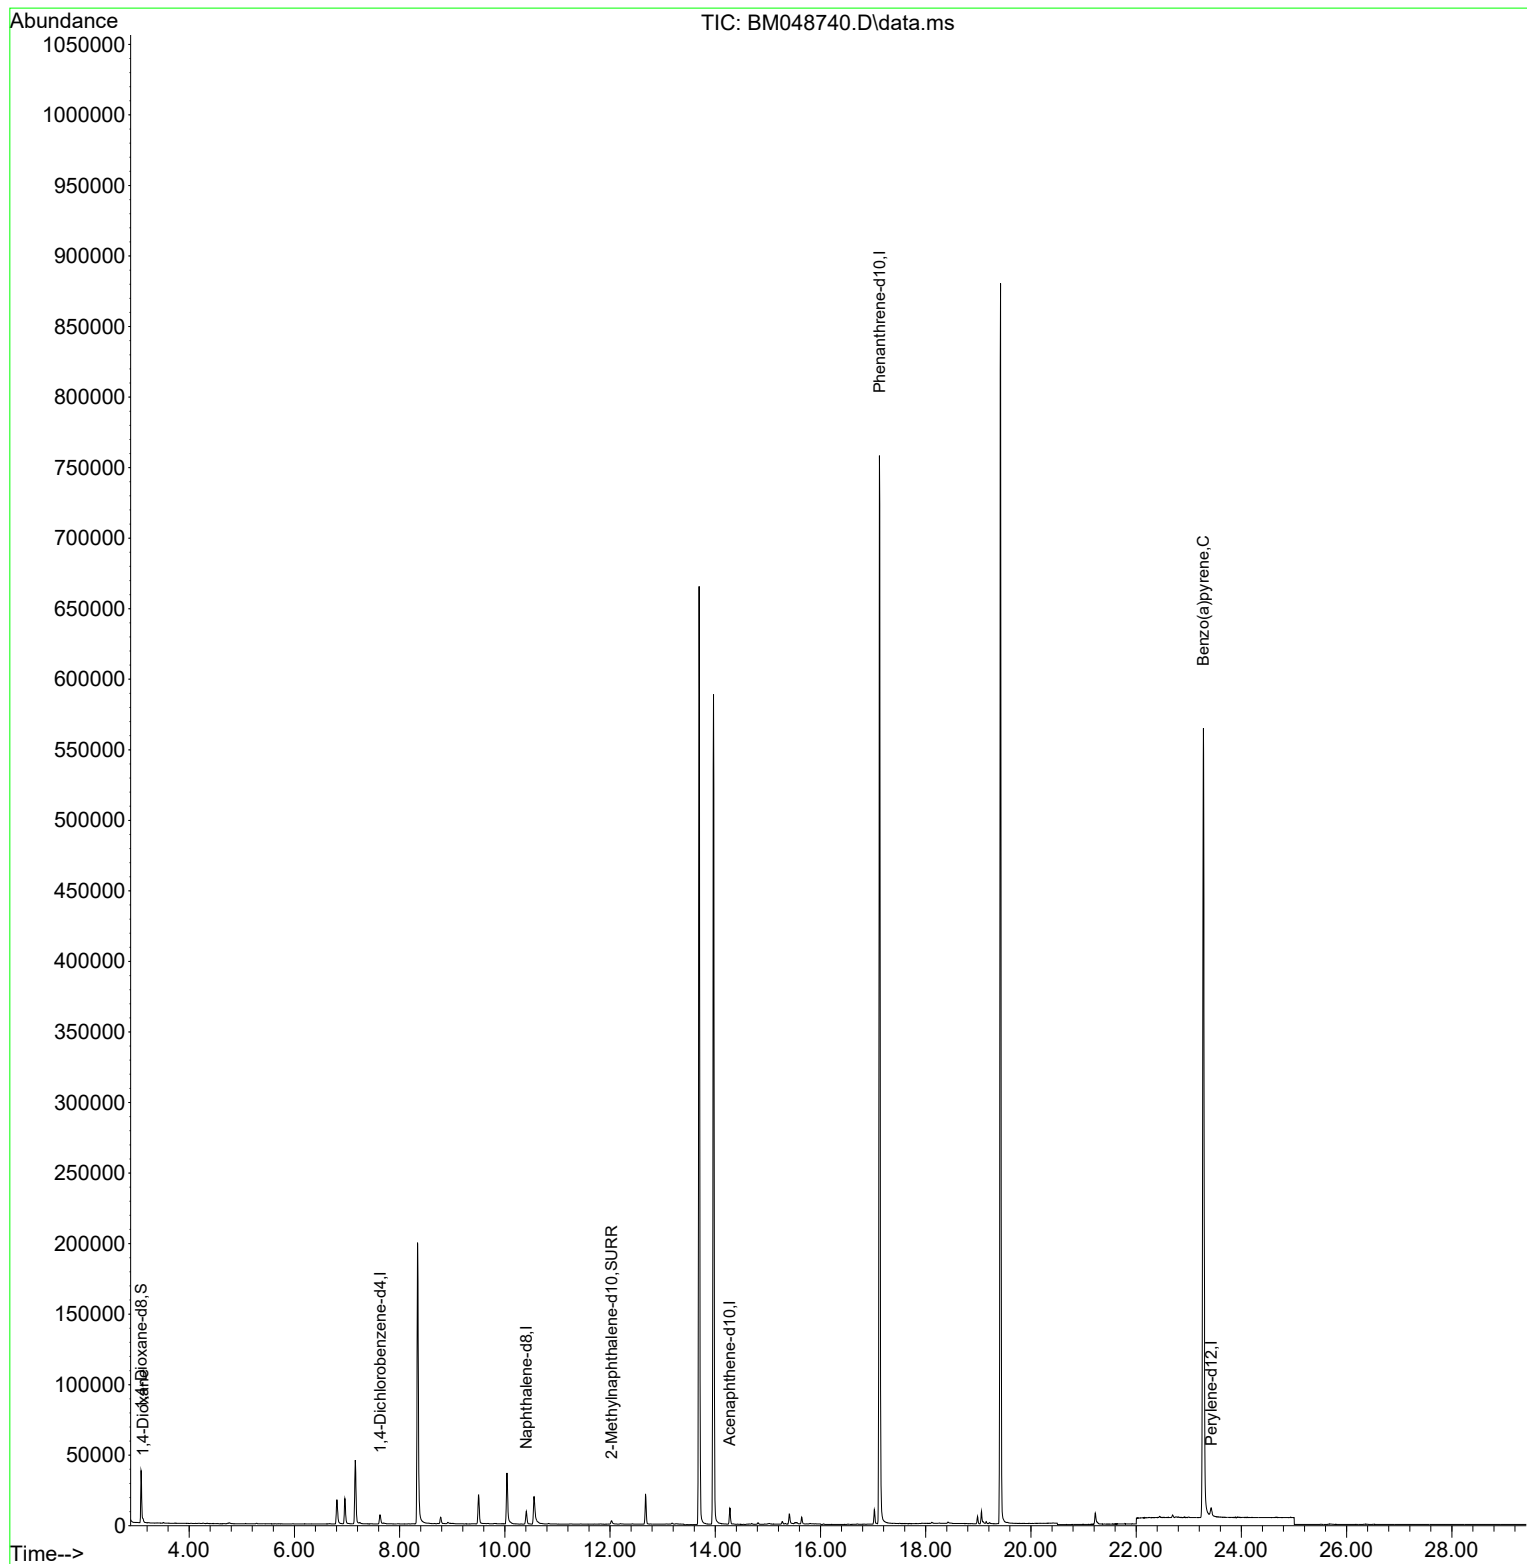


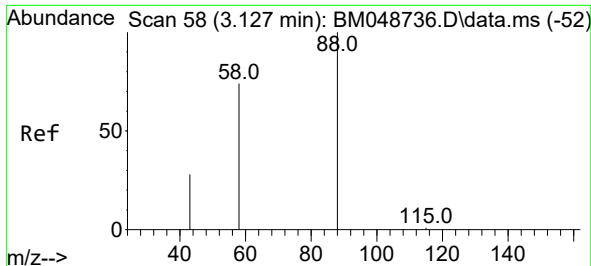

#2
1,4-Dioxane
Concen: 0.227 ng/ul
RT: 3.123 min Scan# 51
Delta R.T. -0.004 min
Lab File: BM048740.D
Acq: 16 Nov 2024 14:03

Instrument :
BNA_M
ClientSampleId :
A0AP4

Tgt Ion: 88 Resp: 1306
Ion Ratio Lower Upper
88 100
43 52.7 60.2 90.4#
58 48.9 44.2 66.2

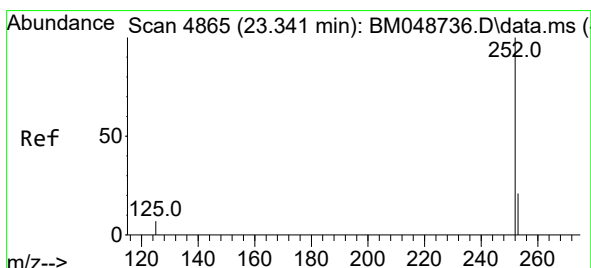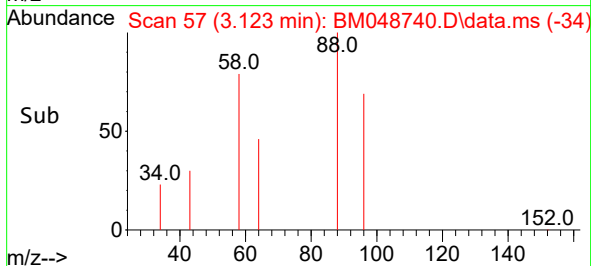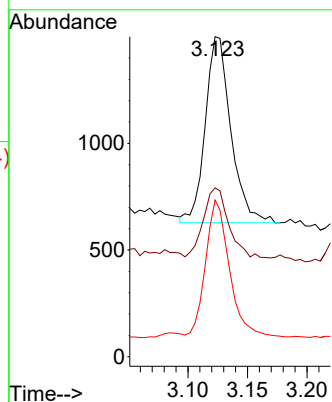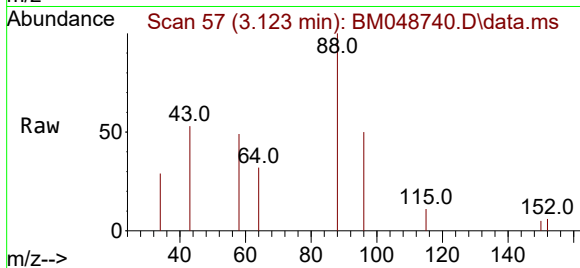

#26
Benzo(a)pyrene
Concen: 0.078 ng/ul
RT: 23.277 min Scan# 4843
Delta R.T. -0.064 min
Lab File: BM048740.D
Acq: 16 Nov 2024 14:03

Tgt Ion: 252 Resp: 2868
Ion Ratio Lower Upper
252 100
253 60.7 29.6 44.4#
125 52.5 23.9 35.9#

