

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111624\
 Data File : BM048741.D
 Acq On : 16 Nov 2024 14:39
 Operator : RC/JU
 Sample : P4803-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A0AP6

Quant Time: Nov 17 22:48:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Nov 17 22:31:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.629	152	4045	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.410	136	12312	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.276	164	6671	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.121	188	714063	0.400	ng/ul	0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.23
23) Perylene-d12	23.423	264	12750	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.089	96	22388	4.588	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.015	152	3772	0.237	ng/ul	-0.03
18) Fluoranthene-d10	19.059	212	8654	0.000	ng/ul	-0.01
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.123	88	17436	3.108	ng/ul#	62
26) Benzo(a)pyrene	23.274	252	2417	0.062	ng/ul#	45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111624\
Data File : BM048741.D
Acq On : 16 Nov 2024 14:39
Operator : RC/JU
Sample : P4803-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A0AP6

Quant Time: Nov 17 22:48:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 17 22:31:02 2024
Response via : Initial Calibration




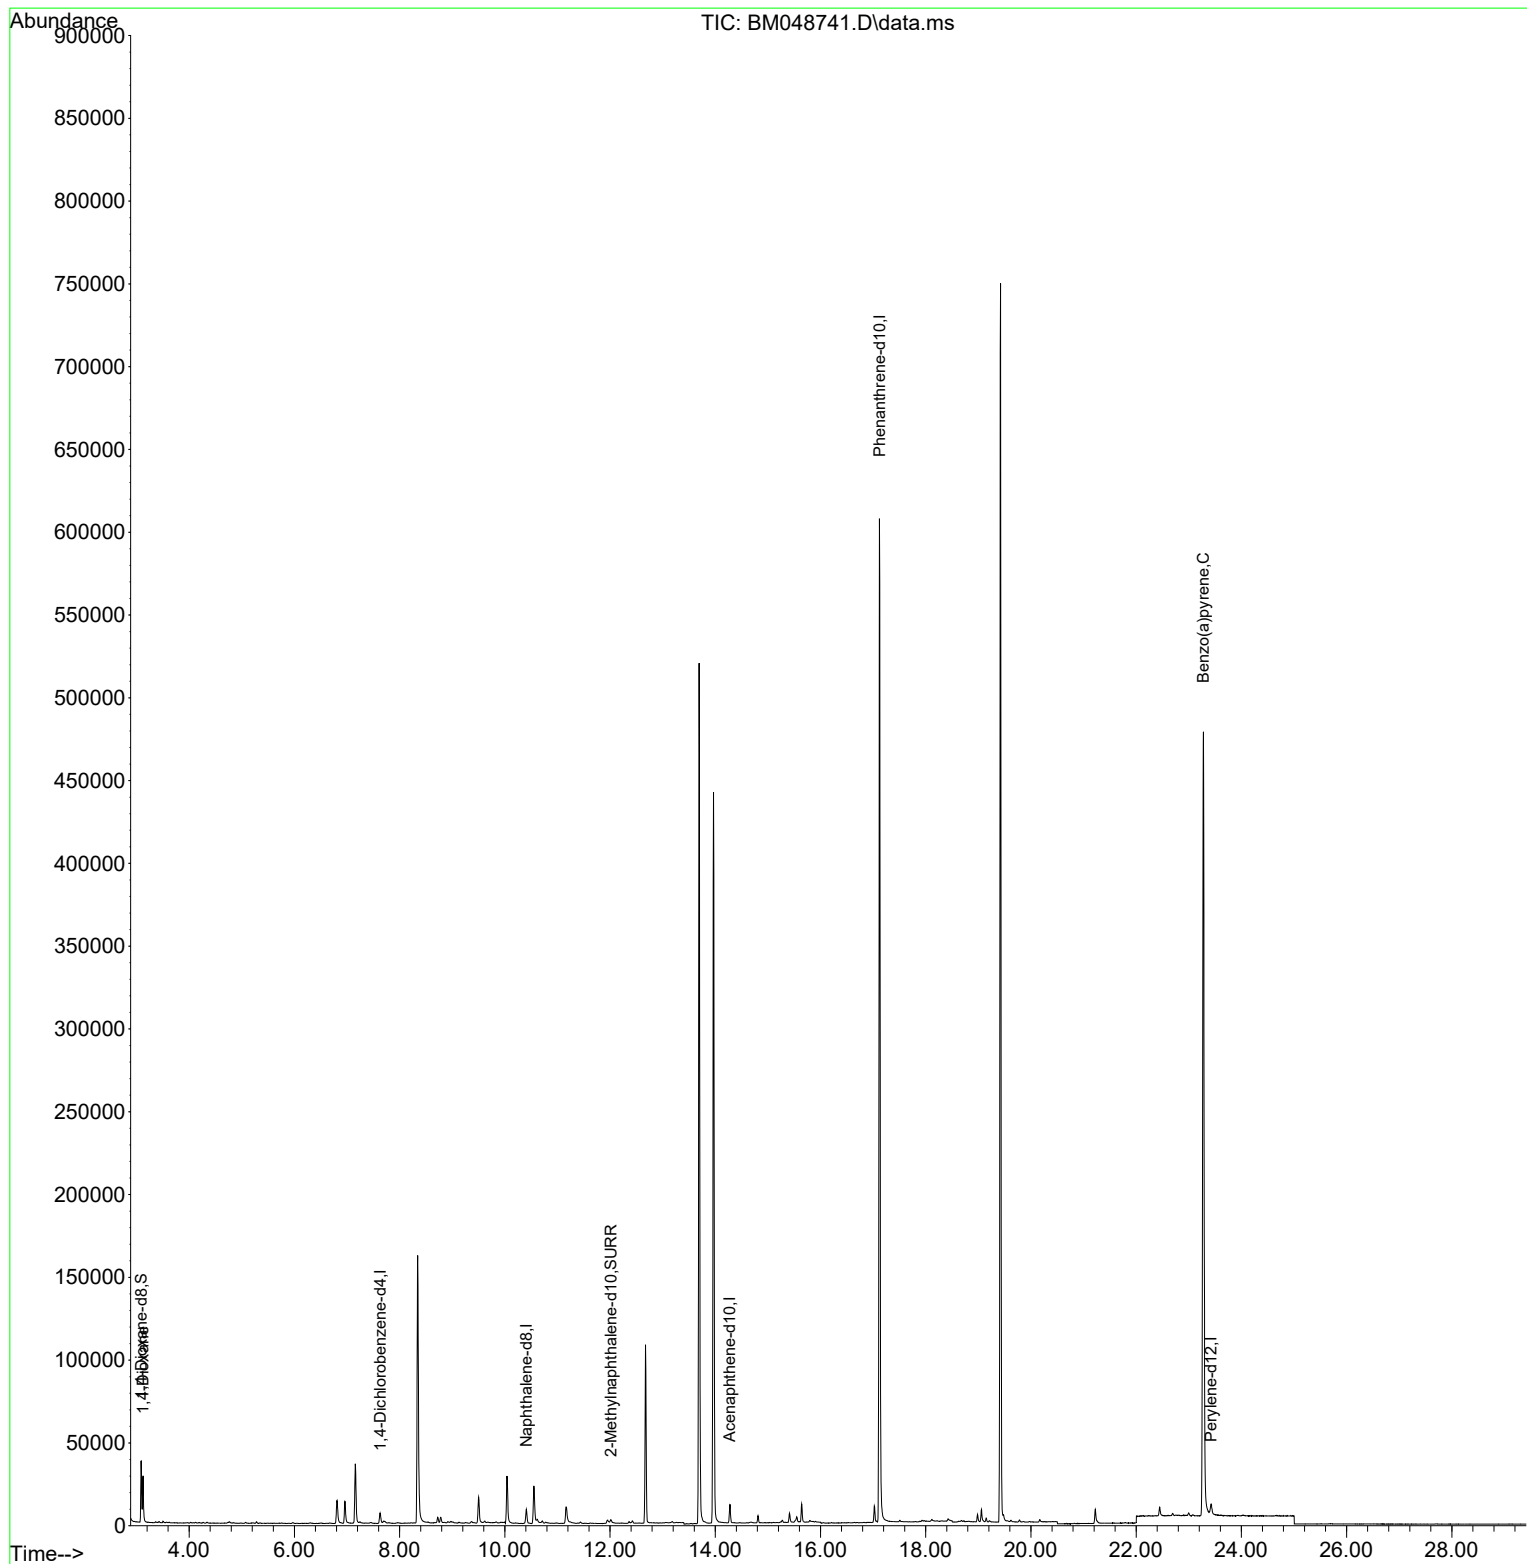


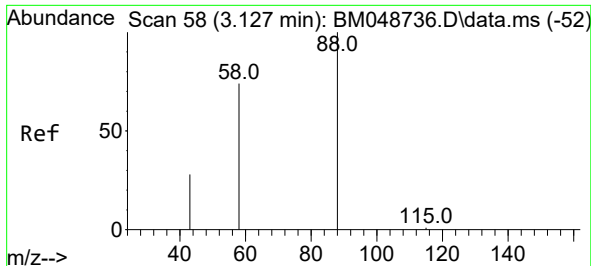

#2
1,4-Dioxane
Concen: 3.108 ng/ul
RT: 3.123 min Scan# 51
Delta R.T. -0.004 min
Lab File: BM048741.D
Acq: 16 Nov 2024 14:39

Instrument :
BNA_M
ClientSampleId :
A0AP6

Tgt Ion: 88 Resp: 17436
Ion Ratio Lower Upper
88 100
43 32.1 60.2 90.4#
58 69.6 44.2 66.2#

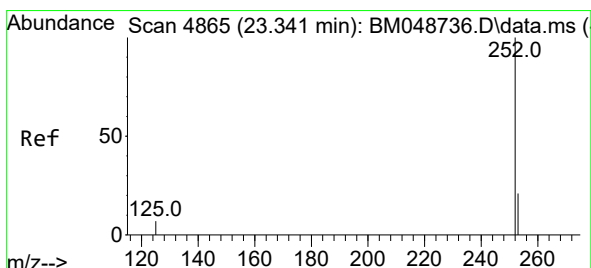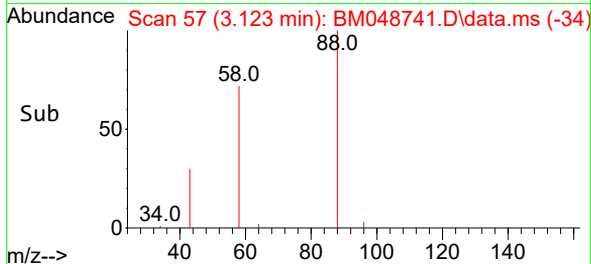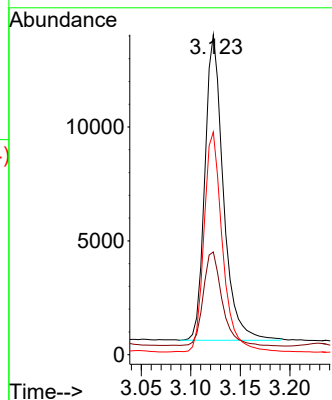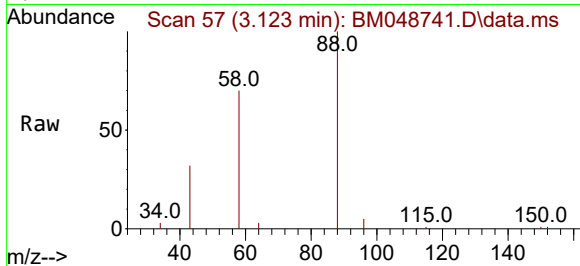

#26
Benzo(a)pyrene
Concen: 0.062 ng/ul
RT: 23.274 min Scan# 4842
Delta R.T. -0.067 min
Lab File: BM048741.D
Acq: 16 Nov 2024 14:39

Tgt Ion: 252 Resp: 2417
Ion Ratio Lower Upper
252 100
253 65.8 29.6 44.4#
125 63.9 23.9 35.9#

