

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111624\
 Data File : BM048747.D
 Acq On : 16 Nov 2024 18:16
 Operator : RC/JU
 Sample : P4803-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A0AQ9

Quant Time: Nov 17 22:49:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Nov 17 22:31:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.629	152	3109	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.410	136	9207	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.276	164	4900	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.121	188	804540	0.400	ng/ul	0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.23
23) Perylene-d12	23.420	264	12235	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.089	96	23577	6.286	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.026	152	4511	0.379	ng/ul	-0.02
18) Fluoranthene-d10	19.059	212	9904	0.000	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.123	88	743	0.172	ng/ul#	78
26) Benzo(a)pyrene	23.274	252	3202	0.086	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111624\
Data File : BM048747.D
Acq On : 16 Nov 2024 18:16
Operator : RC/JU
Sample : P4803-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A0AQ9

Quant Time: Nov 17 22:49:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 17 22:31:02 2024
Response via : Initial Calibration




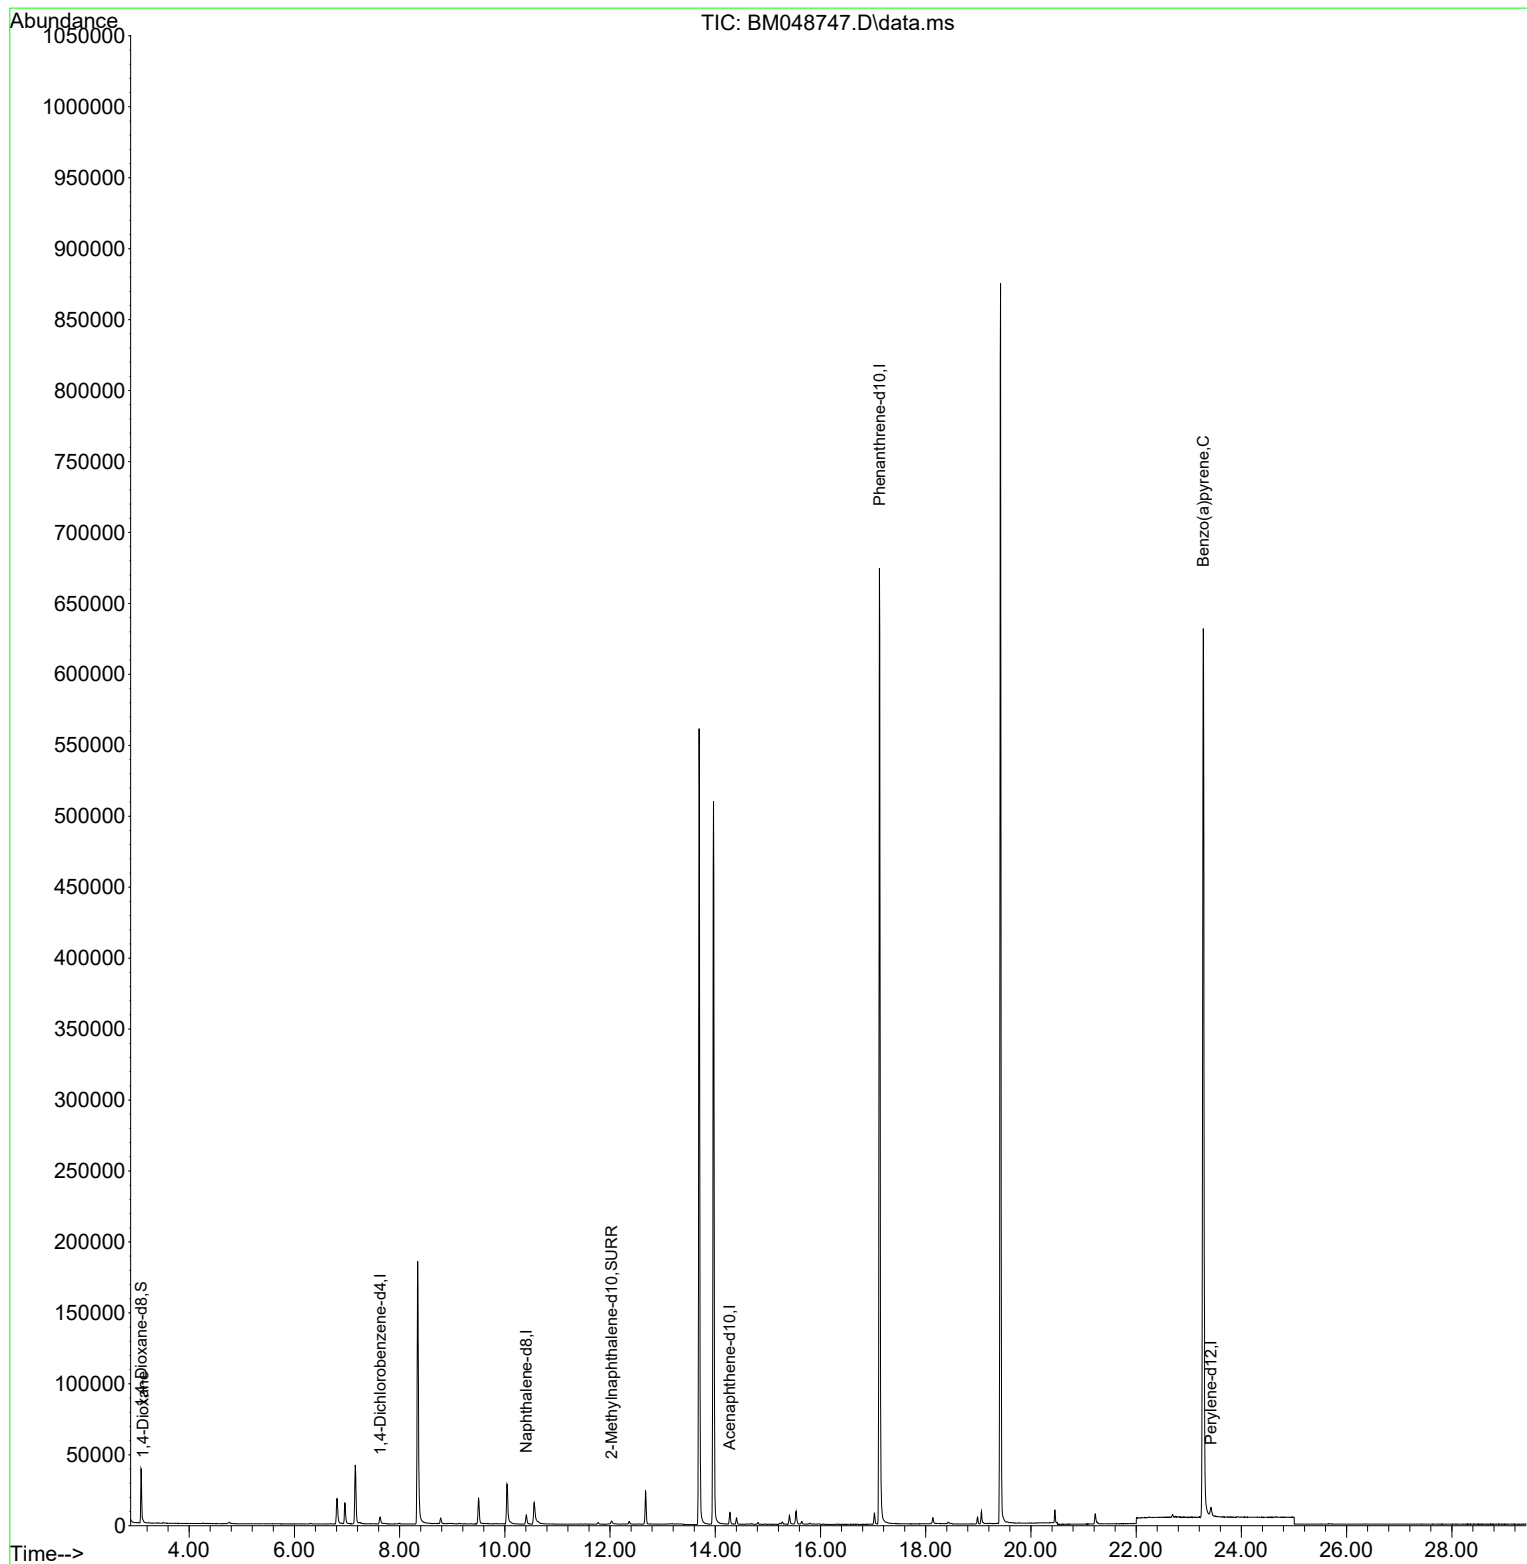


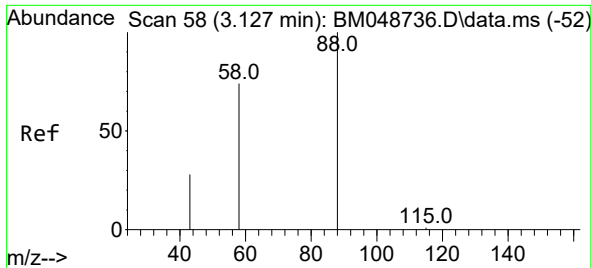

#2
1,4-Dioxane
Concen: 0.172 ng/ul
RT: 3.123 min Scan# 51
Delta R.T. -0.004 min
Lab File: BM048747.D
Acq: 16 Nov 2024 18:16

Instrument :
BNA_M
ClientSampleId :
A0AQ9

Tgt Ion: 88 Resp: 743
Ion Ratio Lower Upper
88 100
43 54.0 60.2 90.4#
58 41.5 44.2 66.2#

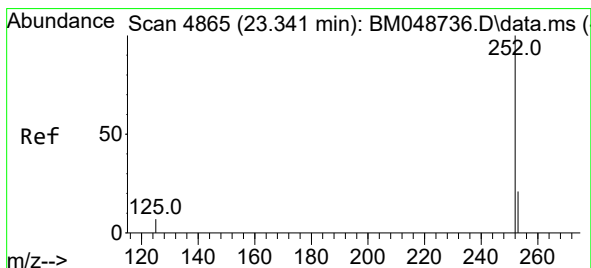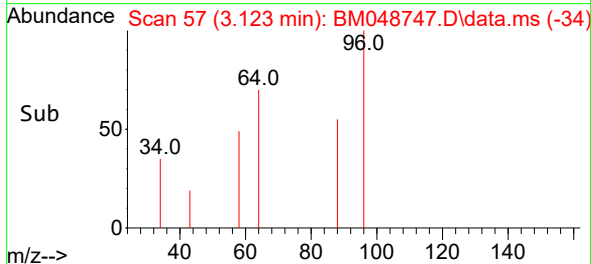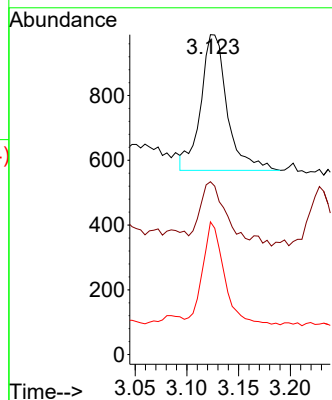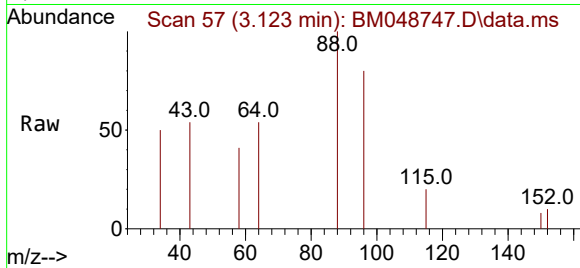

#26
Benzo(a)pyrene
Concen: 0.086 ng/ul
RT: 23.274 min Scan# 4842
Delta R.T. -0.067 min
Lab File: BM048747.D
Acq: 16 Nov 2024 18:16

Tgt Ion: 252 Resp: 3202
Ion Ratio Lower Upper
252 100
253 57.5 29.6 44.4#
125 52.2 23.9 35.9#

