

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111624\
 Data File : BM048756.D
 Acq On : 17 Nov 2024 00:19
 Operator : RC/JU
 Sample : PB164843BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK843

Quant Time: Nov 17 22:50:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Nov 17 22:31:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.629	152	2911	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.410	136	8633	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.276	164	4361	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.121	188	675834	0.400	ng/ul	0.08
17) Chrysene-d12	21.243	240	6548	0.400	ng/ul	0.01
23) Perylene-d12	23.429	264	13868	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.085	96	24082	6.857	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.043	152	3998	0.358	ng/ul	0.00
18) Fluoranthene-d10	19.064	212	7985	0.434	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.123	88	463	0.115	ng/ul#	60
20) Pyrene	19.421	202	1214	0.046	ng/ul#	1
26) Benzo(a)pyrene	23.274	252	2851	0.068	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111624\
Data File : BM048756.D
Acq On : 17 Nov 2024 00:19
Operator : RC/JU
Sample : PB164843BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK843

Quant Time: Nov 17 22:50:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 17 22:31:02 2024
Response via : Initial Calibration




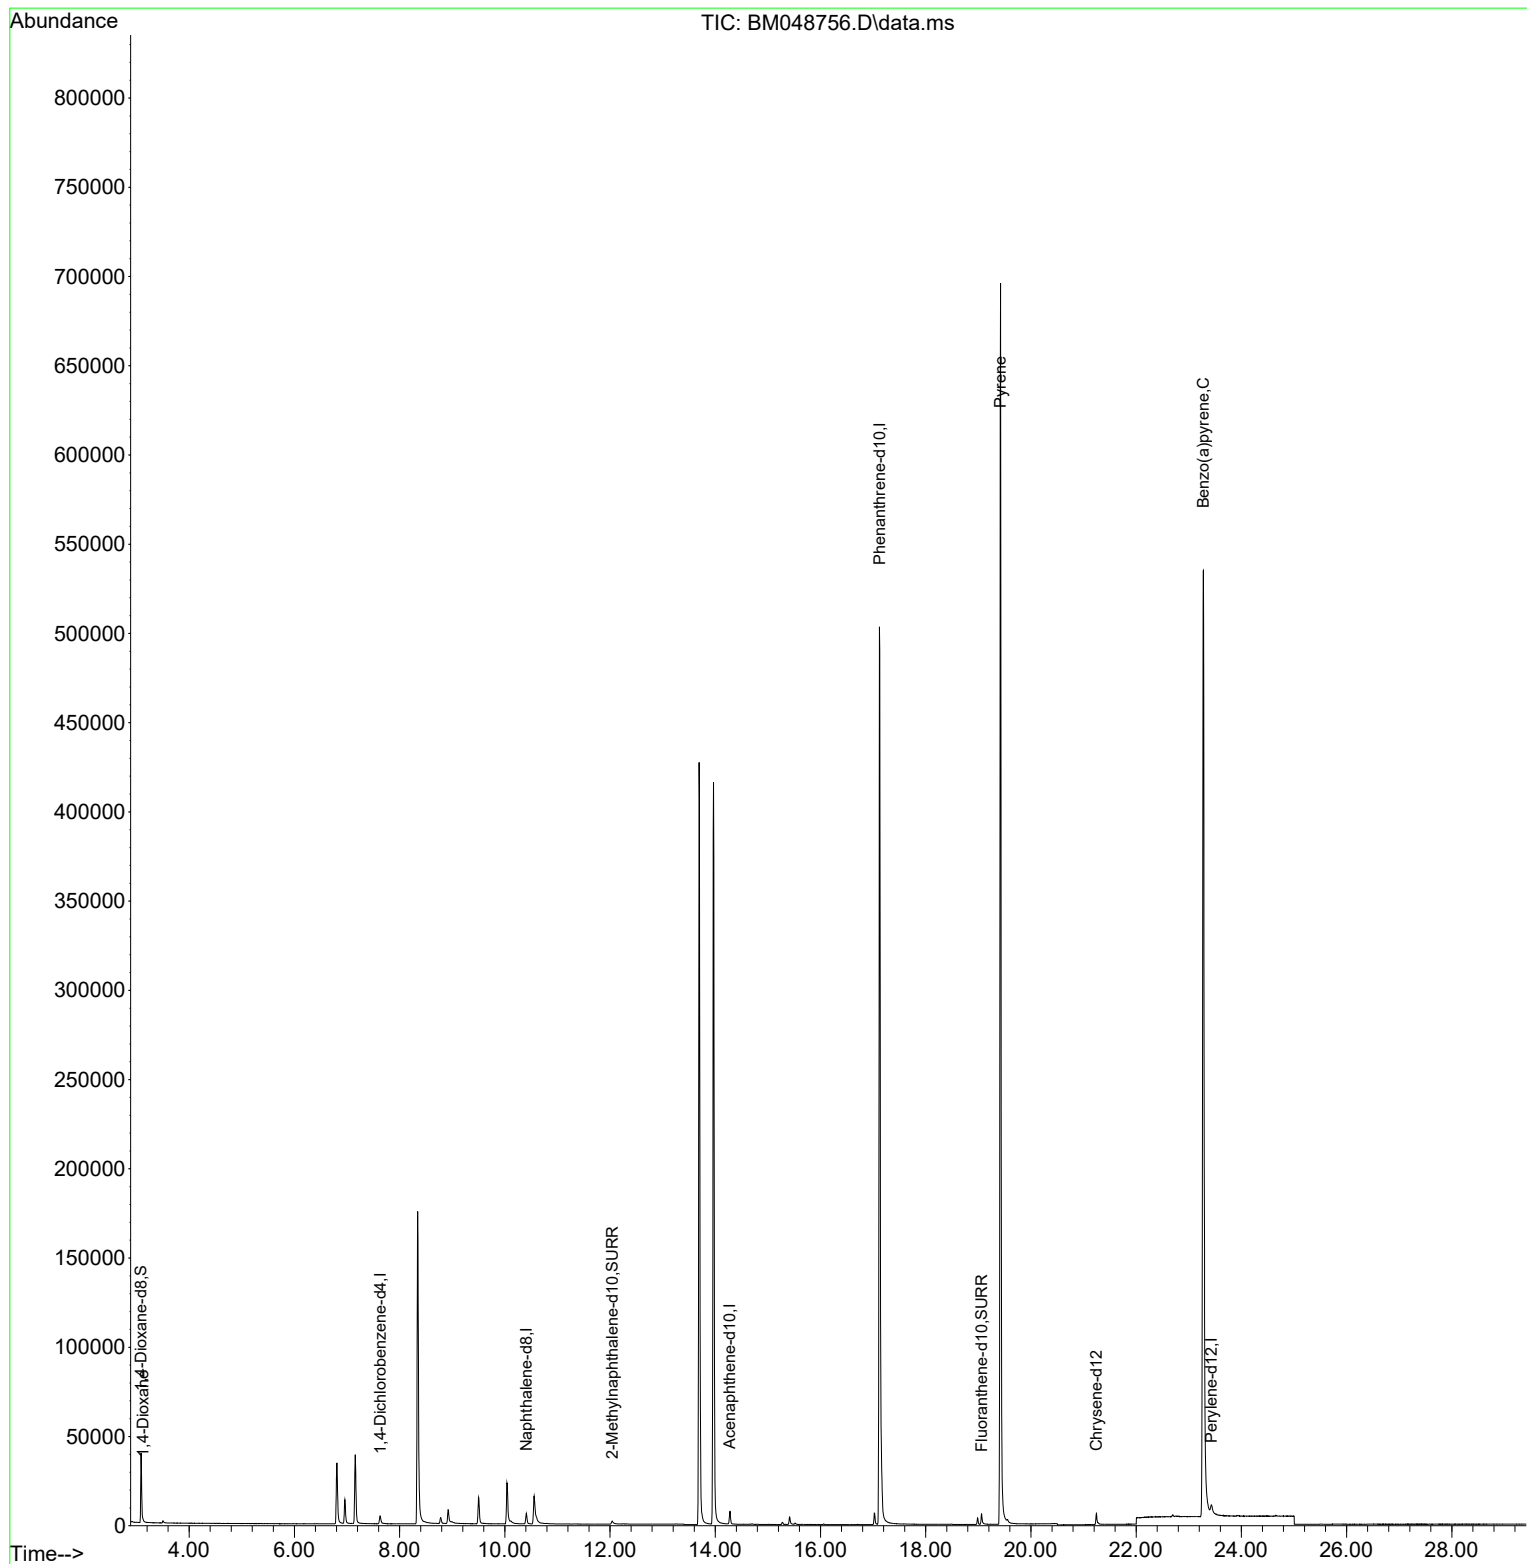


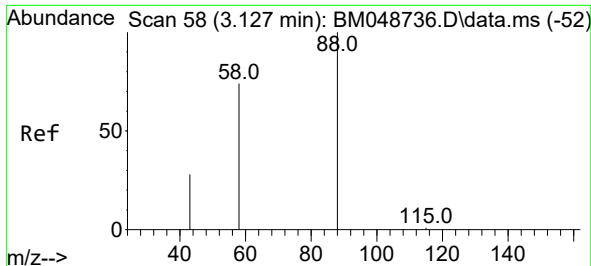

#2
1,4-Dioxane
Concen: 0.115 ng/ul
RT: 3.123 min Scan# 51
Delta R.T. -0.004 min
Lab File: BM048756.D
Acq: 17 Nov 2024 00:19




Instrument :
BNA_M
ClientSampleId :
SBLK843


Tgt Ion: 88 Resp: 463
Ion Ratio Lower Upper
88 100
43 37.8 60.2 90.4#
58 30.2 44.2 66.2#

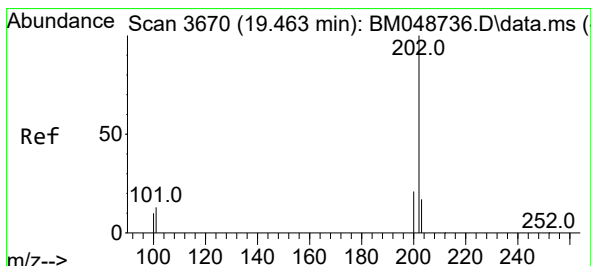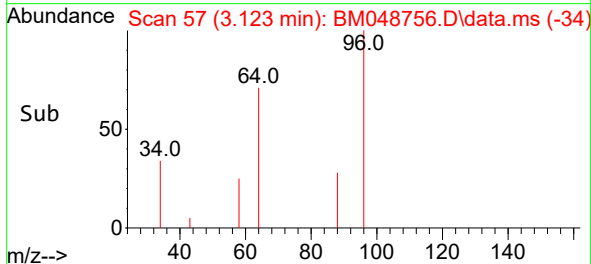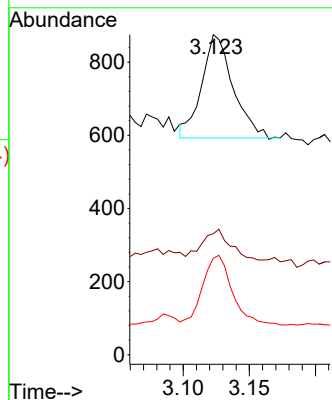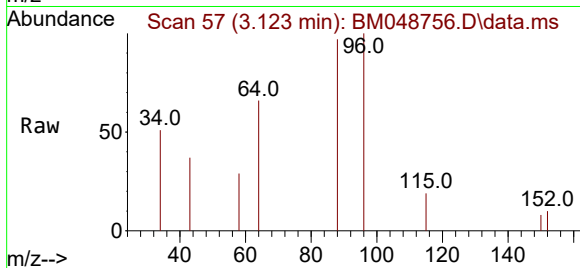

#20
Pyrene
Concen: 0.046 ng/ul
RT: 19.421 min Scan# 3661
Delta R.T. -0.042 min
Lab File: BM048756.D
Acq: 17 Nov 2024 00:19


Tgt Ion: 202 Resp: 1214
Ion Ratio Lower Upper
202 100
101 133.4 11.4 17.2#
100 933.4 8.5 12.7#

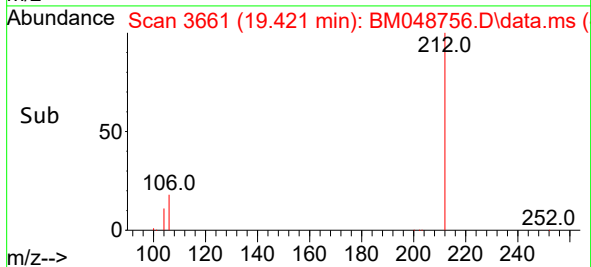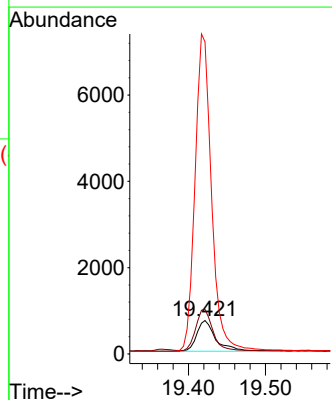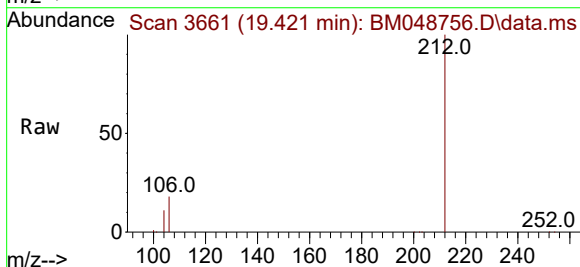

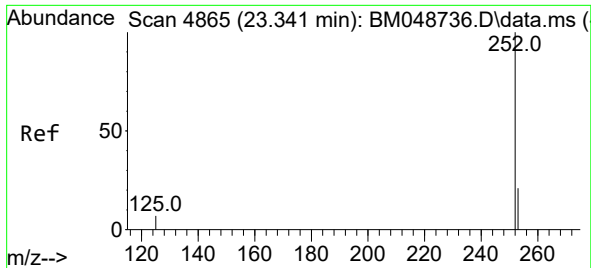

#26
Benzo(a)pyrene
Concen: 0.068 ng/ul
RT: 23.274 min Scan# 41
Delta R.T. -0.067 min
Lab File: BM048756.D
Acq: 17 Nov 2024 00:19

Instrument :
BNA_M
ClientSampleId :
SBLK843

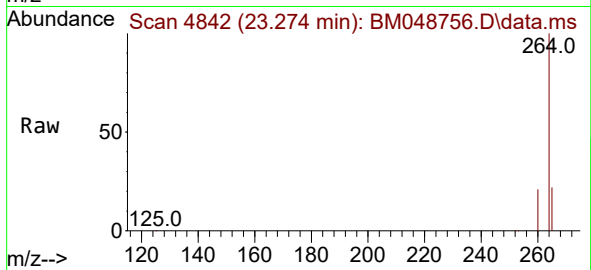

Tgt Ion	Ratio	Lower	Upper
252	100		
253	57.0	29.6	44.4#
125	50.8	23.9	35.9#

