

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111624\
 Data File : BM048761.D
 Acq On : 17 Nov 2024 03:21
 Operator : RC/JU
 Sample : P4828-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CBA06

Quant Time: Nov 17 22:51:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Nov 17 22:31:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.629	152	3408	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.410	136	10442	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.277	164	5762	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.121	188	1069955	0.400	ng/ul	0.08
17) Chrysene-d12	21.240	240	8328	0.400	ng/ul	0.01
23) Perylene-d12	23.424	264	17315	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.085	96	19014	4.625	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.032	152	5234	0.388	ng/ul	-0.02
18) Fluoranthene-d10	19.059	212	12645	0.541	ng/ul	-0.01
Target Compounds						
					Qvalue	
20) Pyrene	19.422	202	1802	0.054	ng/ul#	1
26) Benzo(a)pyrene	23.272	252	4201	0.080	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111624\
Data File : BM048761.D
Acq On : 17 Nov 2024 03:21
Operator : RC/JU
Sample : P4828-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CBA06

Quant Time: Nov 17 22:51:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 17 22:31:02 2024
Response via : Initial Calibration




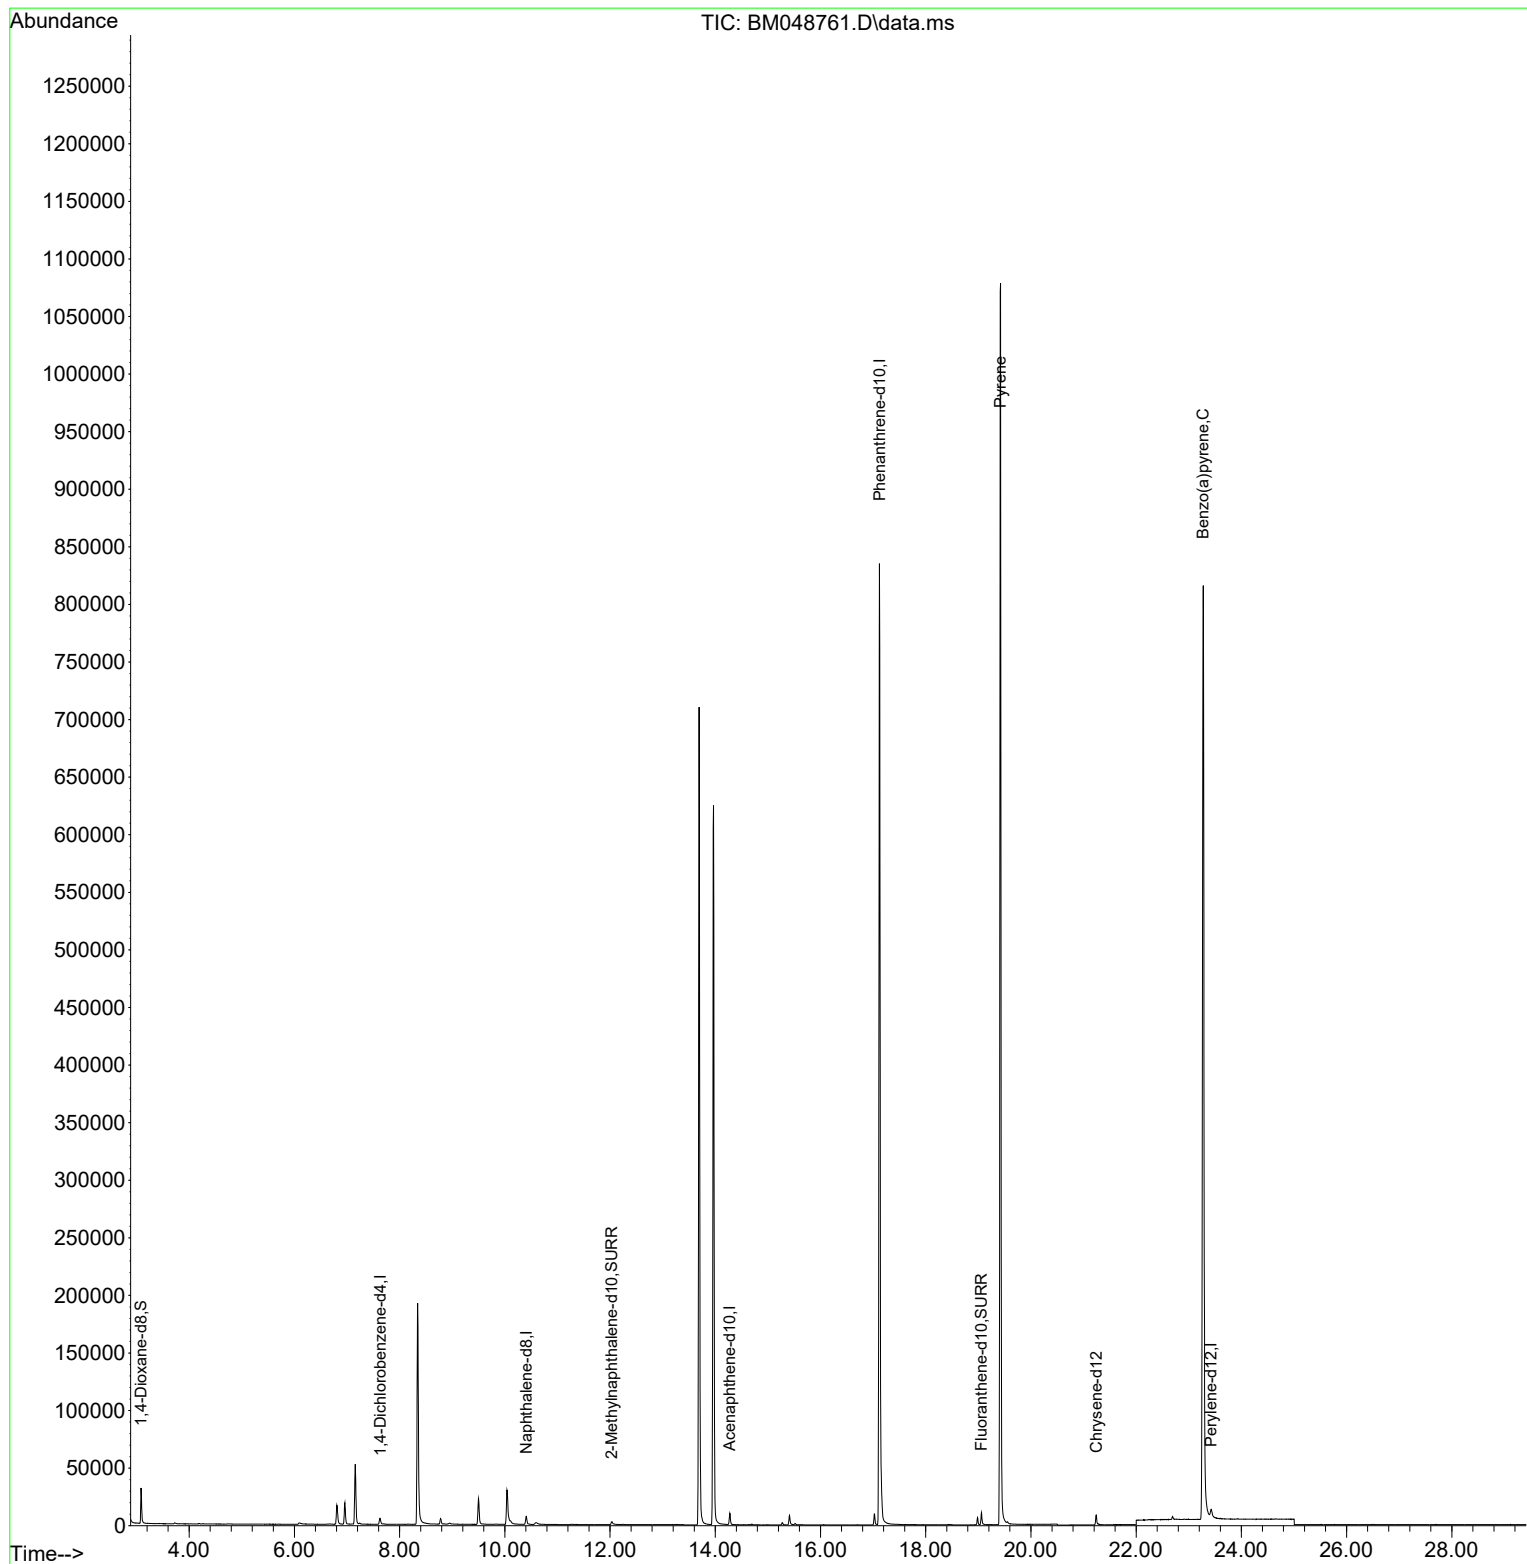


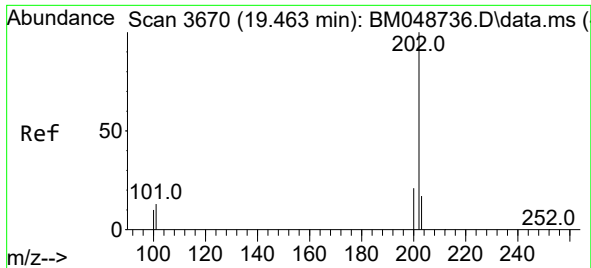

#20
Pyrene
Concen: 0.054 ng/ul
RT: 19.422 min Scan# 3
Delta R.T. -0.042 min
Lab File: BM048761.D
Acq: 17 Nov 2024 03:21

Instrument :
BNA_M
ClientSampleId :
CBA06

Tgt Ion:202 Resp: 1802
Ion Ratio Lower Upper
202 100
101 128.9 11.4 17.2#
100 879.7 8.5 12.7#

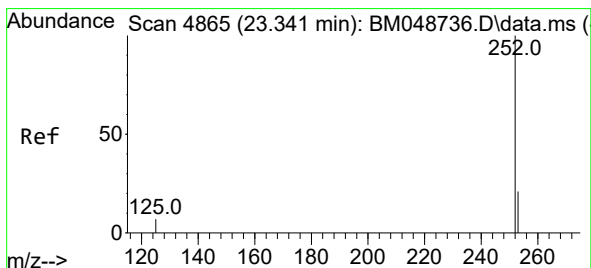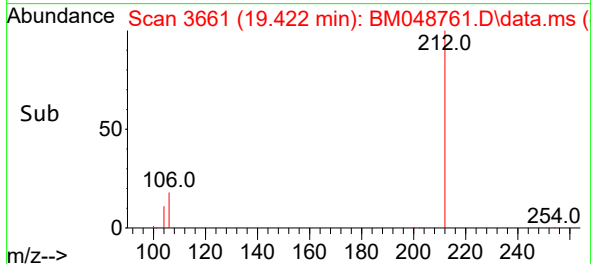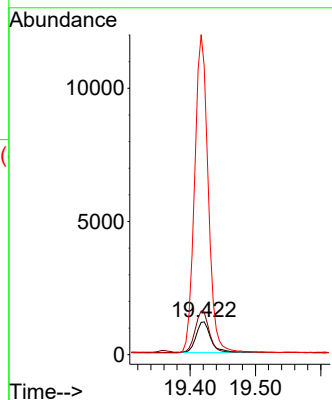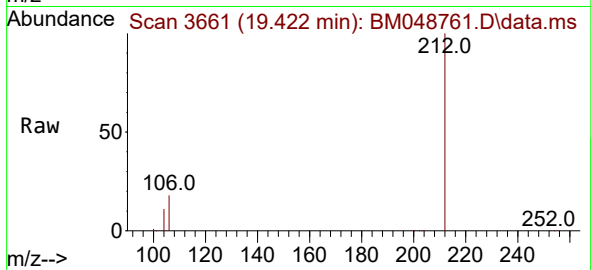

#26
Benzo(a)pyrene
Concen: 0.080 ng/ul
RT: 23.272 min Scan# 4841
Delta R.T. -0.070 min
Lab File: BM048761.D
Acq: 17 Nov 2024 03:21

Tgt Ion:252 Resp: 4201
Ion Ratio Lower Upper
252 100
253 49.2 29.6 44.4#
125 41.2 23.9 35.9#

