

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111624\
 Data File : BM048764.D
 Acq On : 17 Nov 2024 05:10
 Operator : RC/JU
 Sample : P4829-05
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E29T2

Quant Time: Nov 17 22:51:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Nov 17 22:31:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.629	152	3622	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.410	136	10961	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.277	164	5815	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.121	188	938840	0.400	ng/ul	0.08
17) Chrysene-d12	21.234	240	6791	0.400	ng/ul	0.00
23) Perylene-d12	23.421	264	16662	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.085	96	18612	4.259	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.032	152	4013	0.283	ng/ul	-0.02
18) Fluoranthene-d10	19.059	212	11227	0.589	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.123	88	283	0.056	ng/ul#	66
20) Pyrene	19.417	202	1670	0.061	ng/ul#	1
26) Benzo(a)pyrene	23.271	252	3713	0.073	ng/ul#	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111624\
Data File : BM048764.D
Acq On : 17 Nov 2024 05:10
Operator : RC/JU
Sample : P4829-05
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29T2

Quant Time: Nov 17 22:51:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 17 22:31:02 2024
Response via : Initial Calibration




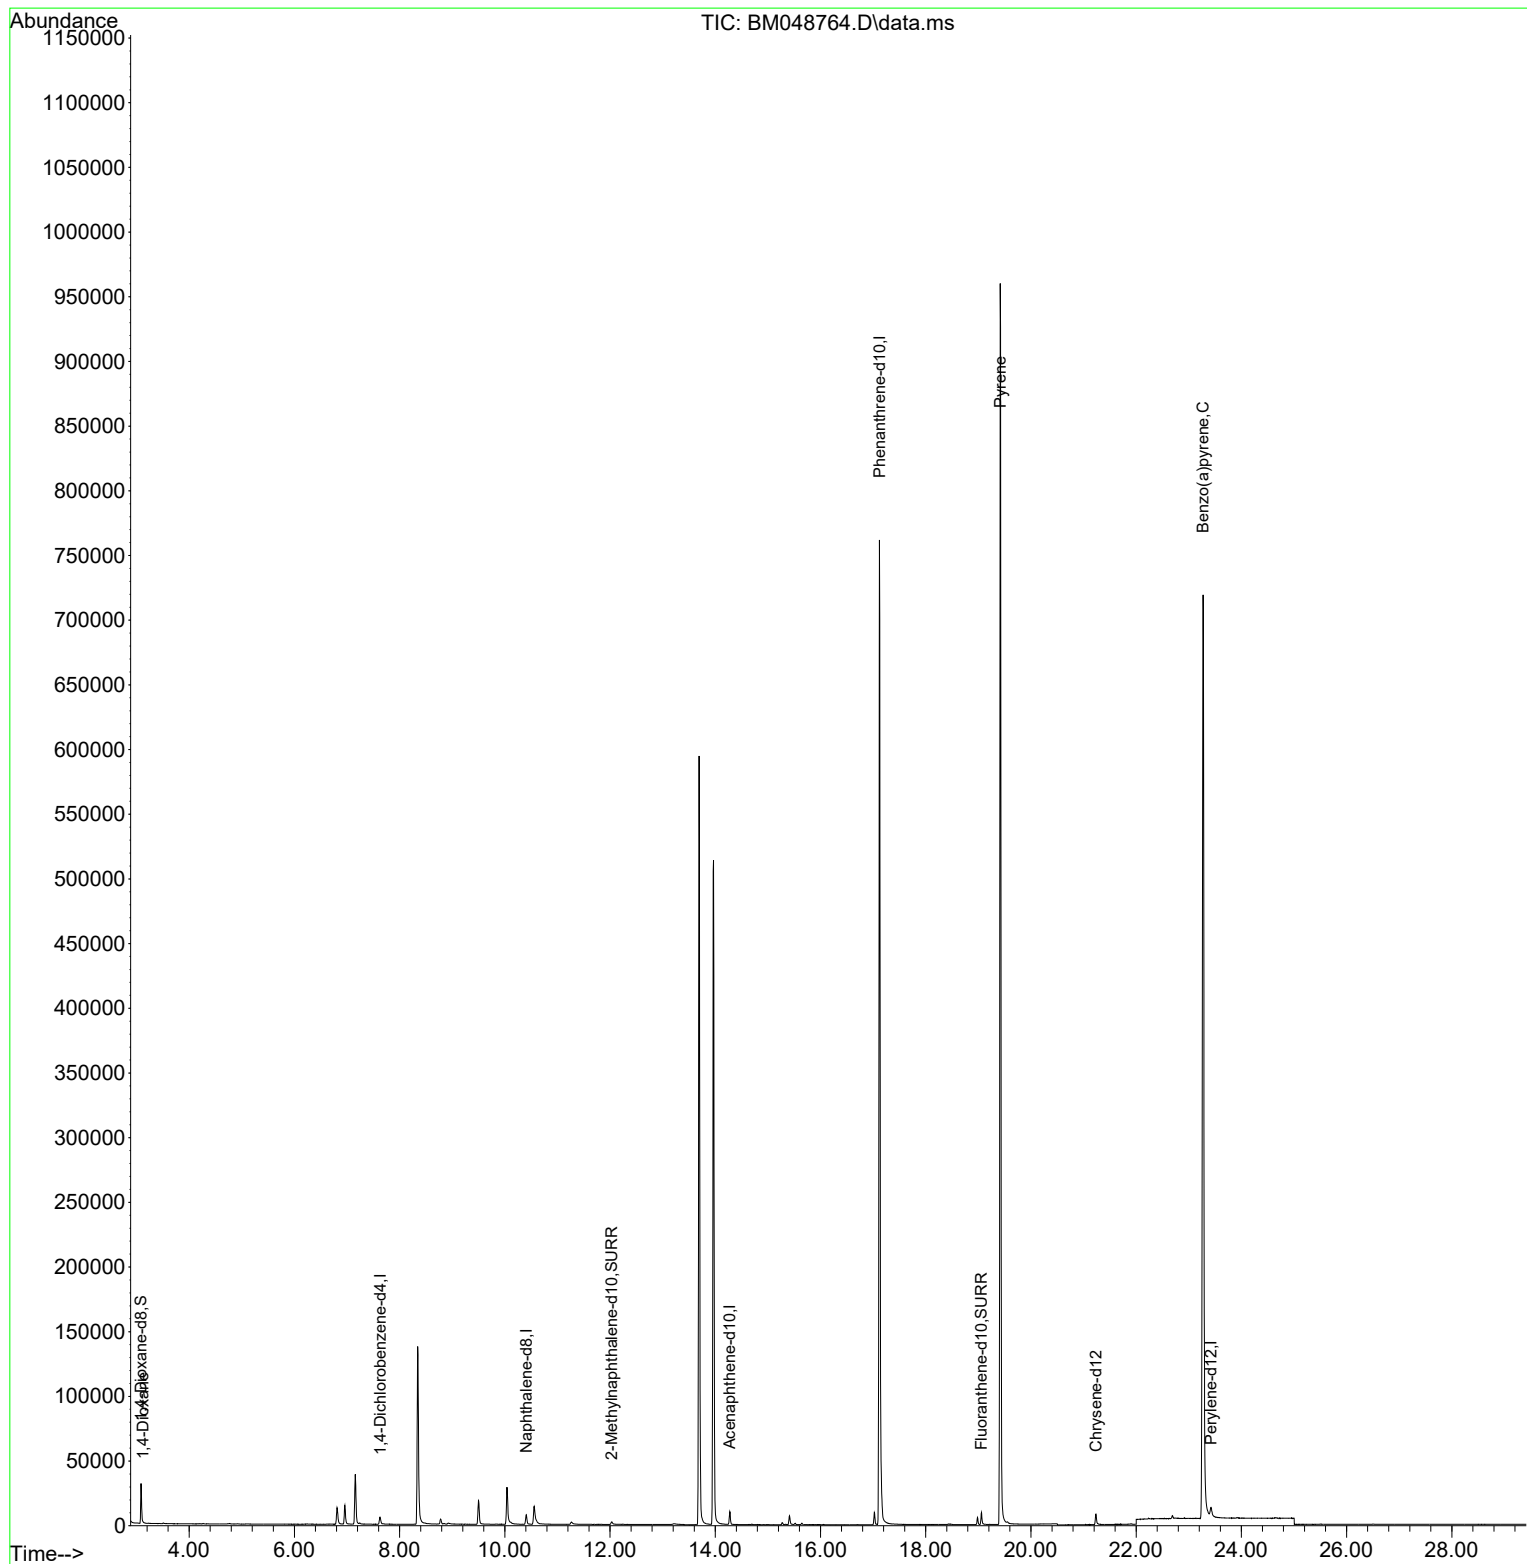


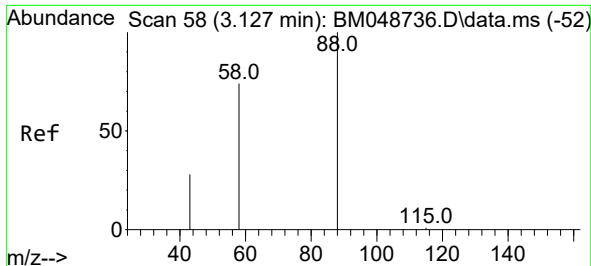

#2
1,4-Dioxane
Concen: 0.056 ng/ul
RT: 3.123 min Scan# 51
Delta R.T. -0.004 min
Lab File: BM048764.D
Acq: 17 Nov 2024 05:10




Instrument :
BNA_M
ClientSampleId :
E29T2


Tgt Ion: 88 Resp: 283
Ion Ratio Lower Upper
88 100
43 51.6 60.2 90.4#
58 23.8 44.2 66.2#

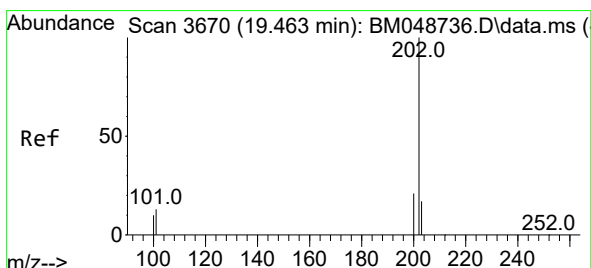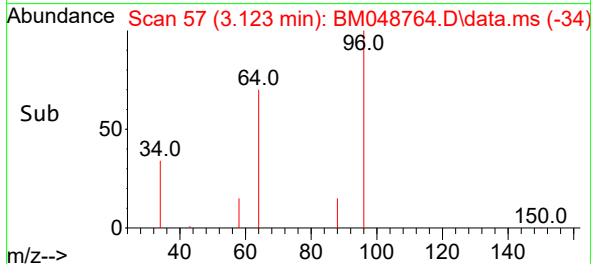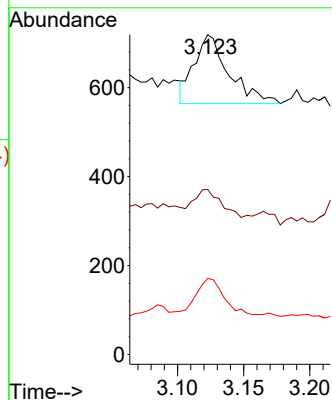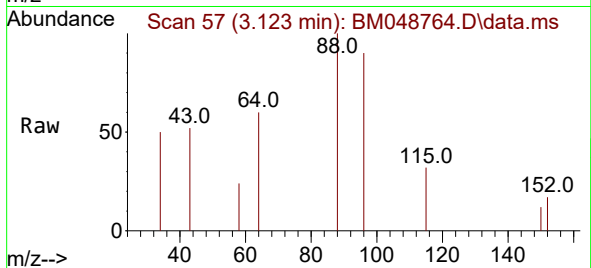

#20
Pyrene
Concen: 0.061 ng/ul
RT: 19.417 min Scan# 3660
Delta R.T. -0.046 min
Lab File: BM048764.D
Acq: 17 Nov 2024 05:10


Tgt Ion: 202 Resp: 1670
Ion Ratio Lower Upper
202 100
101 131.5 11.4 17.2#
100 954.4 8.5 12.7#

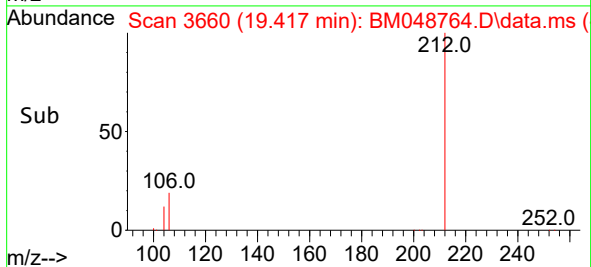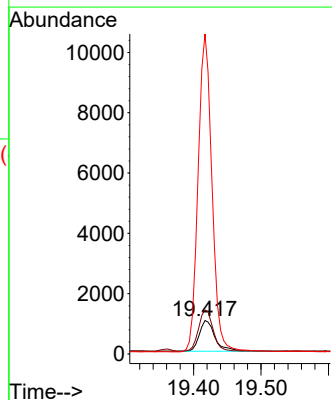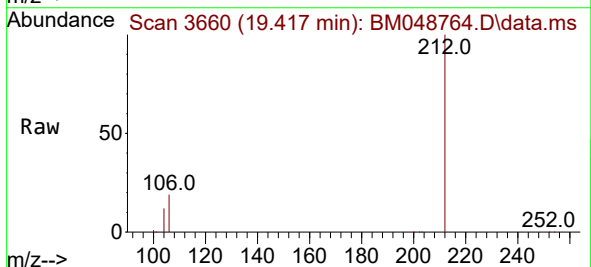

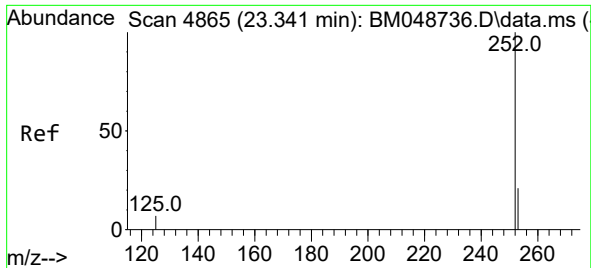

#26
Benzo(a)pyrene
Concen: 0.073 ng/ul
RT: 23.271 min Scan# 4841
Delta R.T. -0.070 min
Lab File: BM048764.D
Acq: 17 Nov 2024 05:10

Instrument :
BNA_M
ClientSampleId :
E29T2

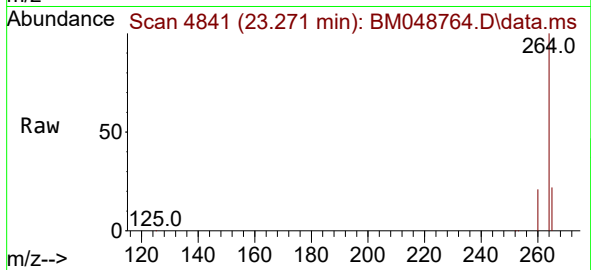

Tgt Ion:252 Resp: 3713
Ion Ratio Lower Upper
252 100
253 52.5 29.6 44.4#
125 48.5 23.9 35.9#

