

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111624\
 Data File : BM048741.D
 Acq On : 16 Nov 2024 14:39
 Operator : RC/JU
 Sample : P4803-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A0AP6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :mohammad ahmed 11/19/2024

Quant Time: Nov 17 22:48:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Nov 17 22:31:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.629	152	4045	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.410	136	12312	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.276	164	6671	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.024	188	12162m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.223	240	9648m	0.400	ng/ul	0.00
23) Perylene-d12	23.423	264	7859m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.089	96	22388	4.588	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.015	152	3772	0.237	ng/ul	-0.03
18) Fluoranthene-d10	19.059	212	8654	0.319	ng/ul	-0.01
Target Compounds					Qvalue	
22) Chrysene	21.261	228	1189	0.031	ng/ul#	68

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111624\
Data File : BM048741.D
Acq On : 16 Nov 2024 14:39
Operator : RC/JU
Sample : P4803-04
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
A0AP6

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

Quant Time: Nov 17 22:48:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 17 22:31:02 2024
Response via : Initial Calibration

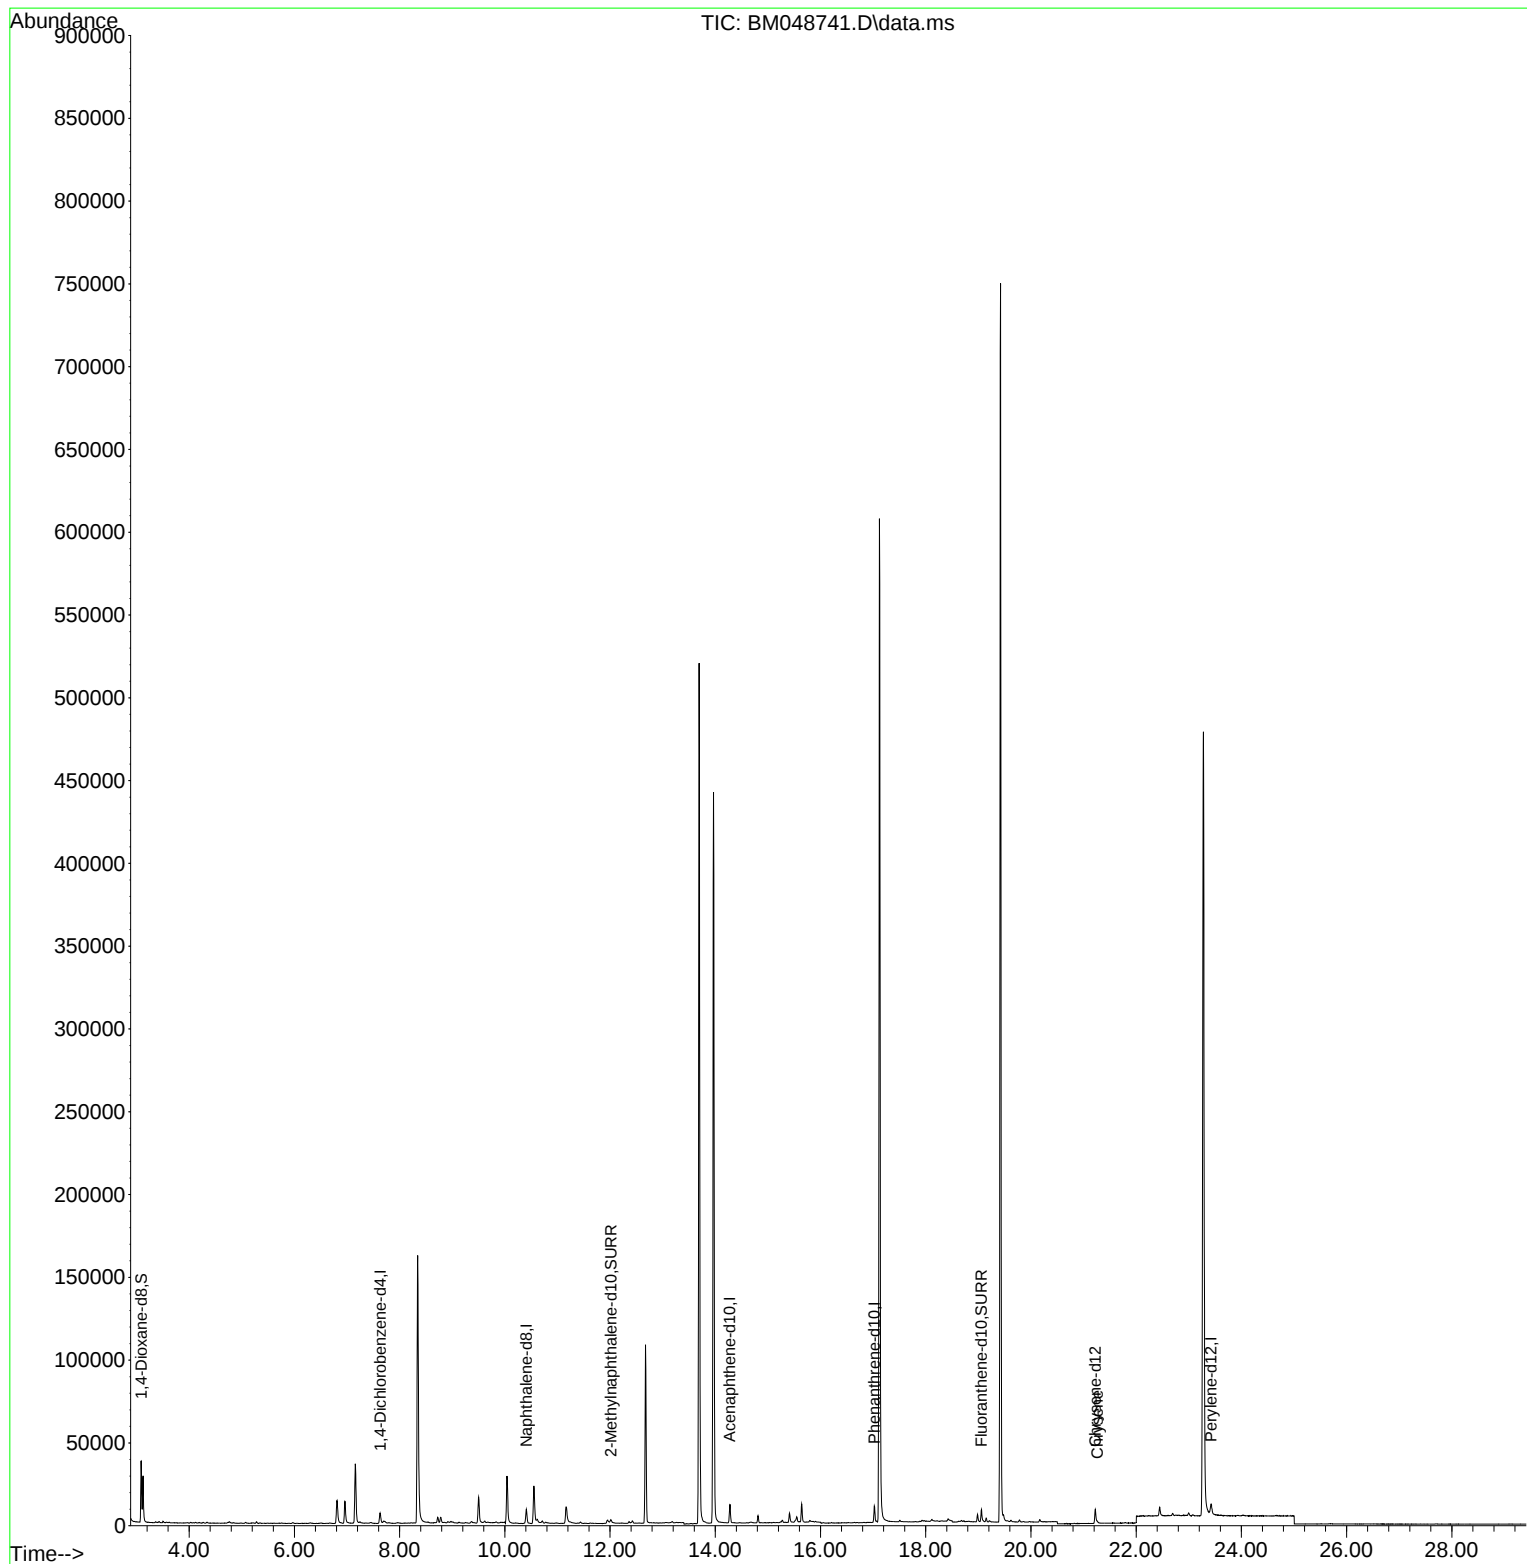

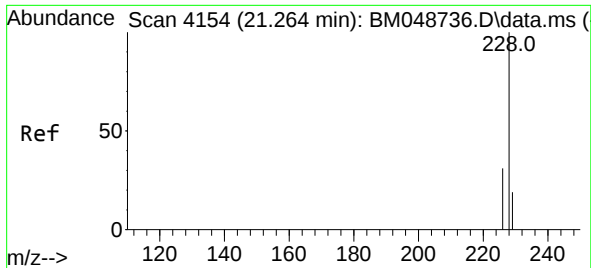

#22

Chrysene

Concen: 0.031 ng/ul

RT: 21.261 min Scan# 41

Delta R.T. -0.003 min

Lab File: BM048741.D


Acq: 16 Nov 2024 14:39

Instrument :

BNA_M

ClientSampleId :

A0AP6

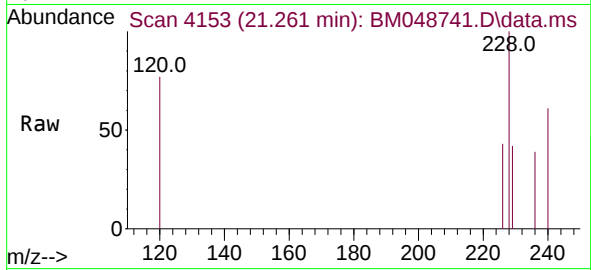

Tgt Ion:228 Resp: 1189

Ion Ratio Lower Upper

228 100

226 43.3 24.4 36.6

229 41.7 16.5 24.7

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 11/19/2024

Supervised By :mohammad ahmed 11/19/2024

