

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111624\
 Data File : BM048747.D
 Acq On : 16 Nov 2024 18:16
 Operator : RC/JU
 Sample : P4803-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A0AQ9

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :mohammad ahmed 11/19/2024

Quant Time: Nov 17 22:49:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Nov 17 22:31:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.629	152	3109	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.410	136	9207	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.276	164	4900	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.024	188	9466m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.223	240	8213m	0.400	ng/ul	0.00
23) Perylene-d12	23.420	264	7048m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.089	96	23577	6.286	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.026	152	4511	0.379	ng/ul	-0.02
18) Fluoranthene-d10	19.059	212	9904	0.430	ng/ul	-0.01
Target Compounds						Qvalue
22) Chrysene	21.261	228	911	0.028	ng/ul#	60

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111624\
Data File : BM048747.D
Acq On : 16 Nov 2024 18:16
Operator : RC/JU
Sample : P4803-14
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
A0AQ9

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024


Quant Time: Nov 17 22:49:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 17 22:31:02 2024
Response via : Initial Calibration

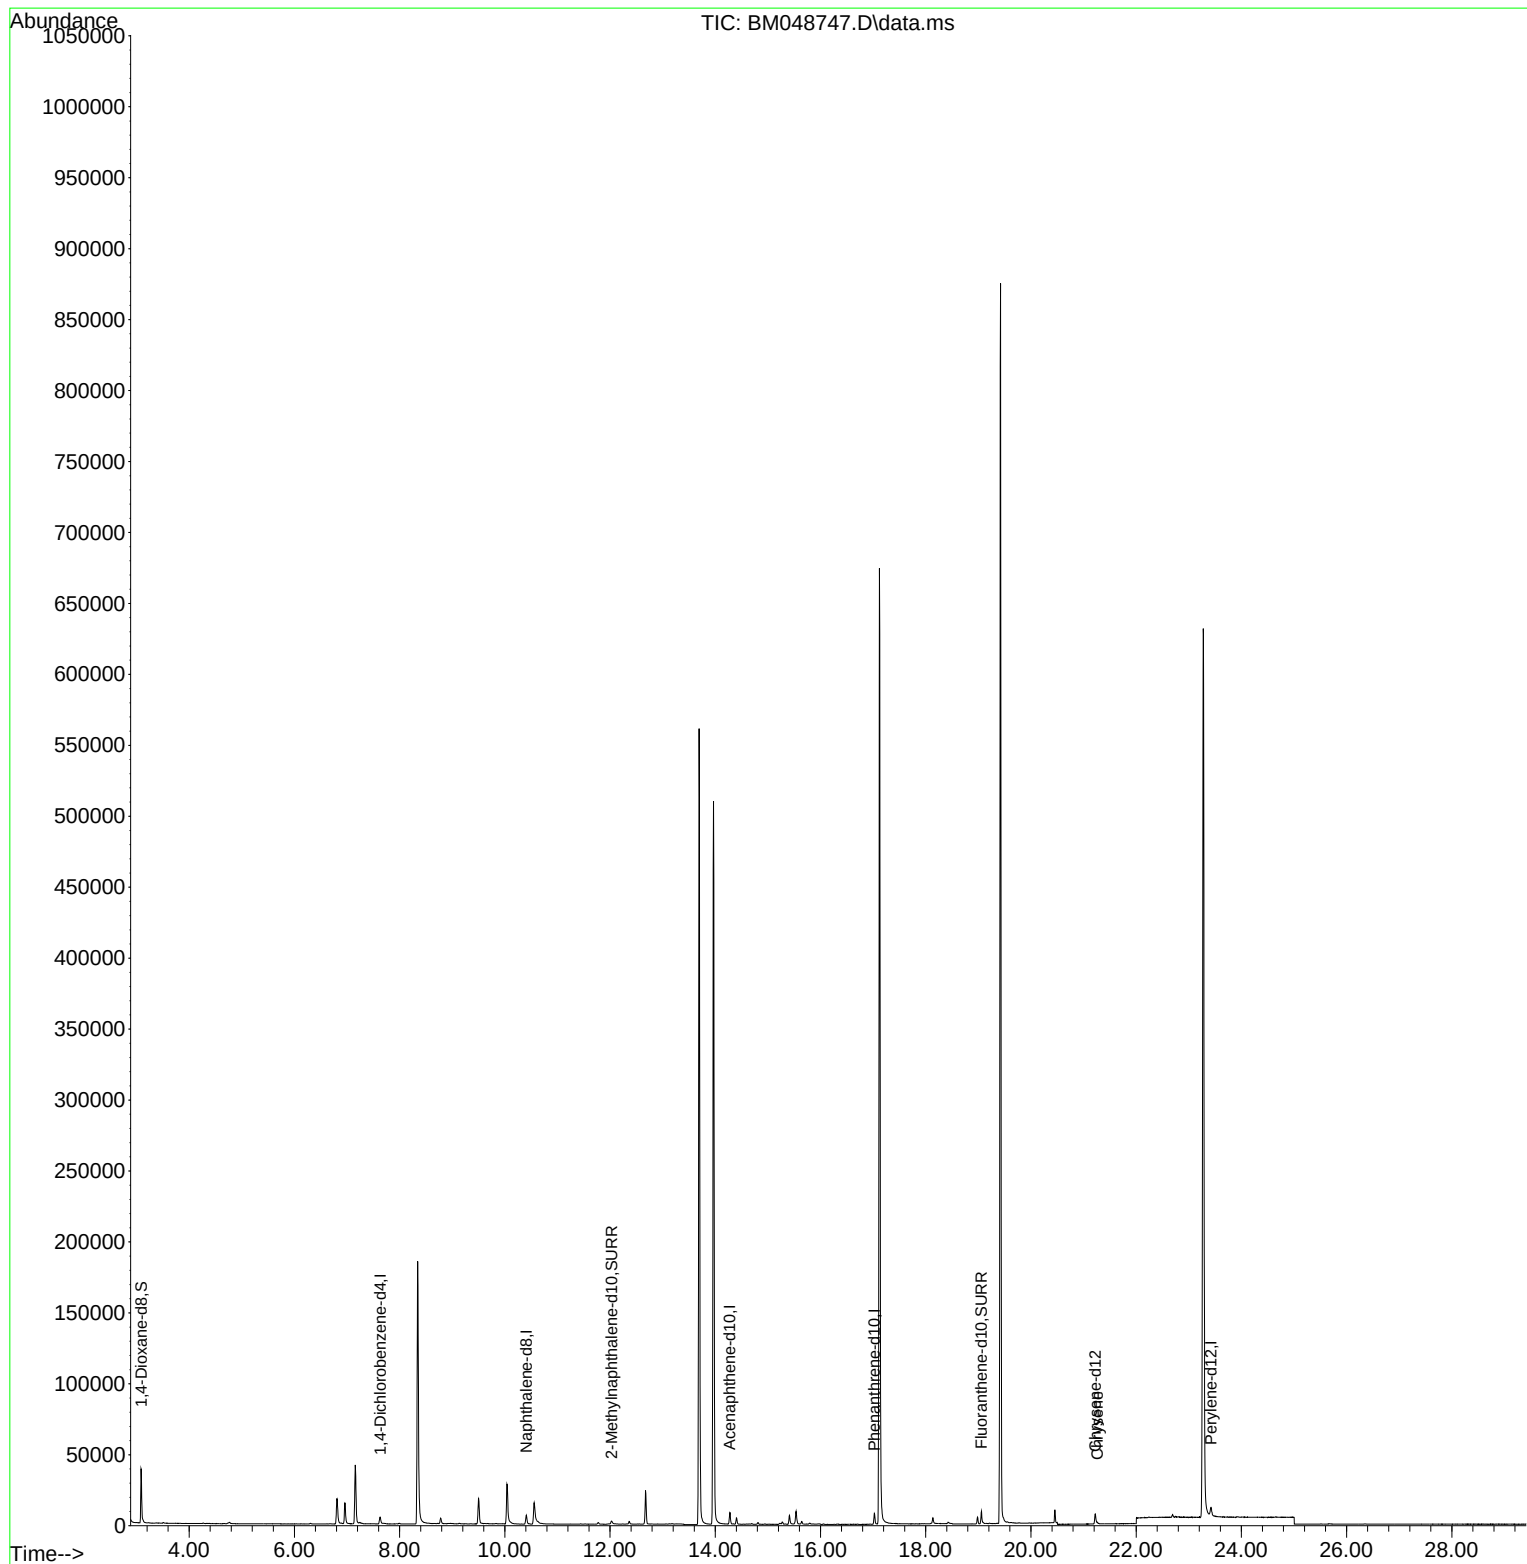

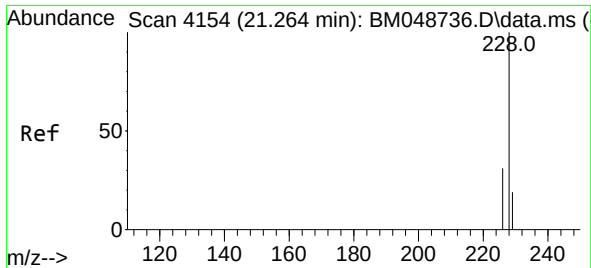

#22
Chrysene
Concen: 0.028 ng/ul
RT: 21.261 min Scan# 4153
Delta R.T. -0.003 min
Lab File: BM048747.D
Acq: 16 Nov 2024 18:16

Instrument :
BNA_M
ClientSampleId :
A0AQ9

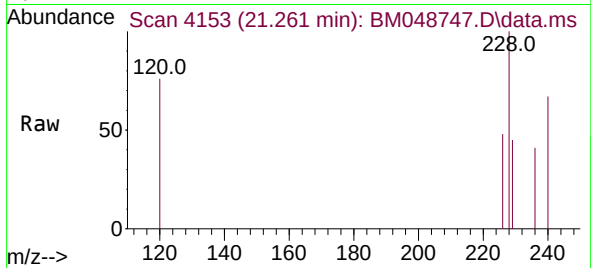

Tgt Ion:228 Resp: 91
Ion Ratio Lower Upper
228 100
226 47.8 24.4 36.6
229 45.2 16.5 24.7

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

