

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111624\
 Data File : BM048760.D
 Acq On : 17 Nov 2024 02:44
 Operator : RC/JU
 Sample : P4828-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CBA04

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :mohammad ahmed 11/19/2024

Quant Time: Nov 17 22:51:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Nov 17 22:31:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.629	152	4951	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.410	136	15323	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.276	164	7968	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.024	188	15517m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.217	240	11043m	0.400	ng/ul	-0.01
23) Perylene-d12	23.420	264	10731m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.089	96	21843	3.657	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.015	152	3847	0.194	ng/ul	-0.03
18) Fluoranthene-d10	19.059	212	7736	0.250	ng/ul	-0.01
Target Compounds						Qvalue
2) 1,4-Dioxane	3.118	88	71184	10.367	ng/ul#	59

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111624\
Data File : BM048760.D
Acq On : 17 Nov 2024 02:44
Operator : RC/JU
Sample : P4828-01
Misc :
ALS Vial : 27 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
CBA04

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024


Quant Time: Nov 17 22:51:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 17 22:31:02 2024
Response via : Initial Calibration

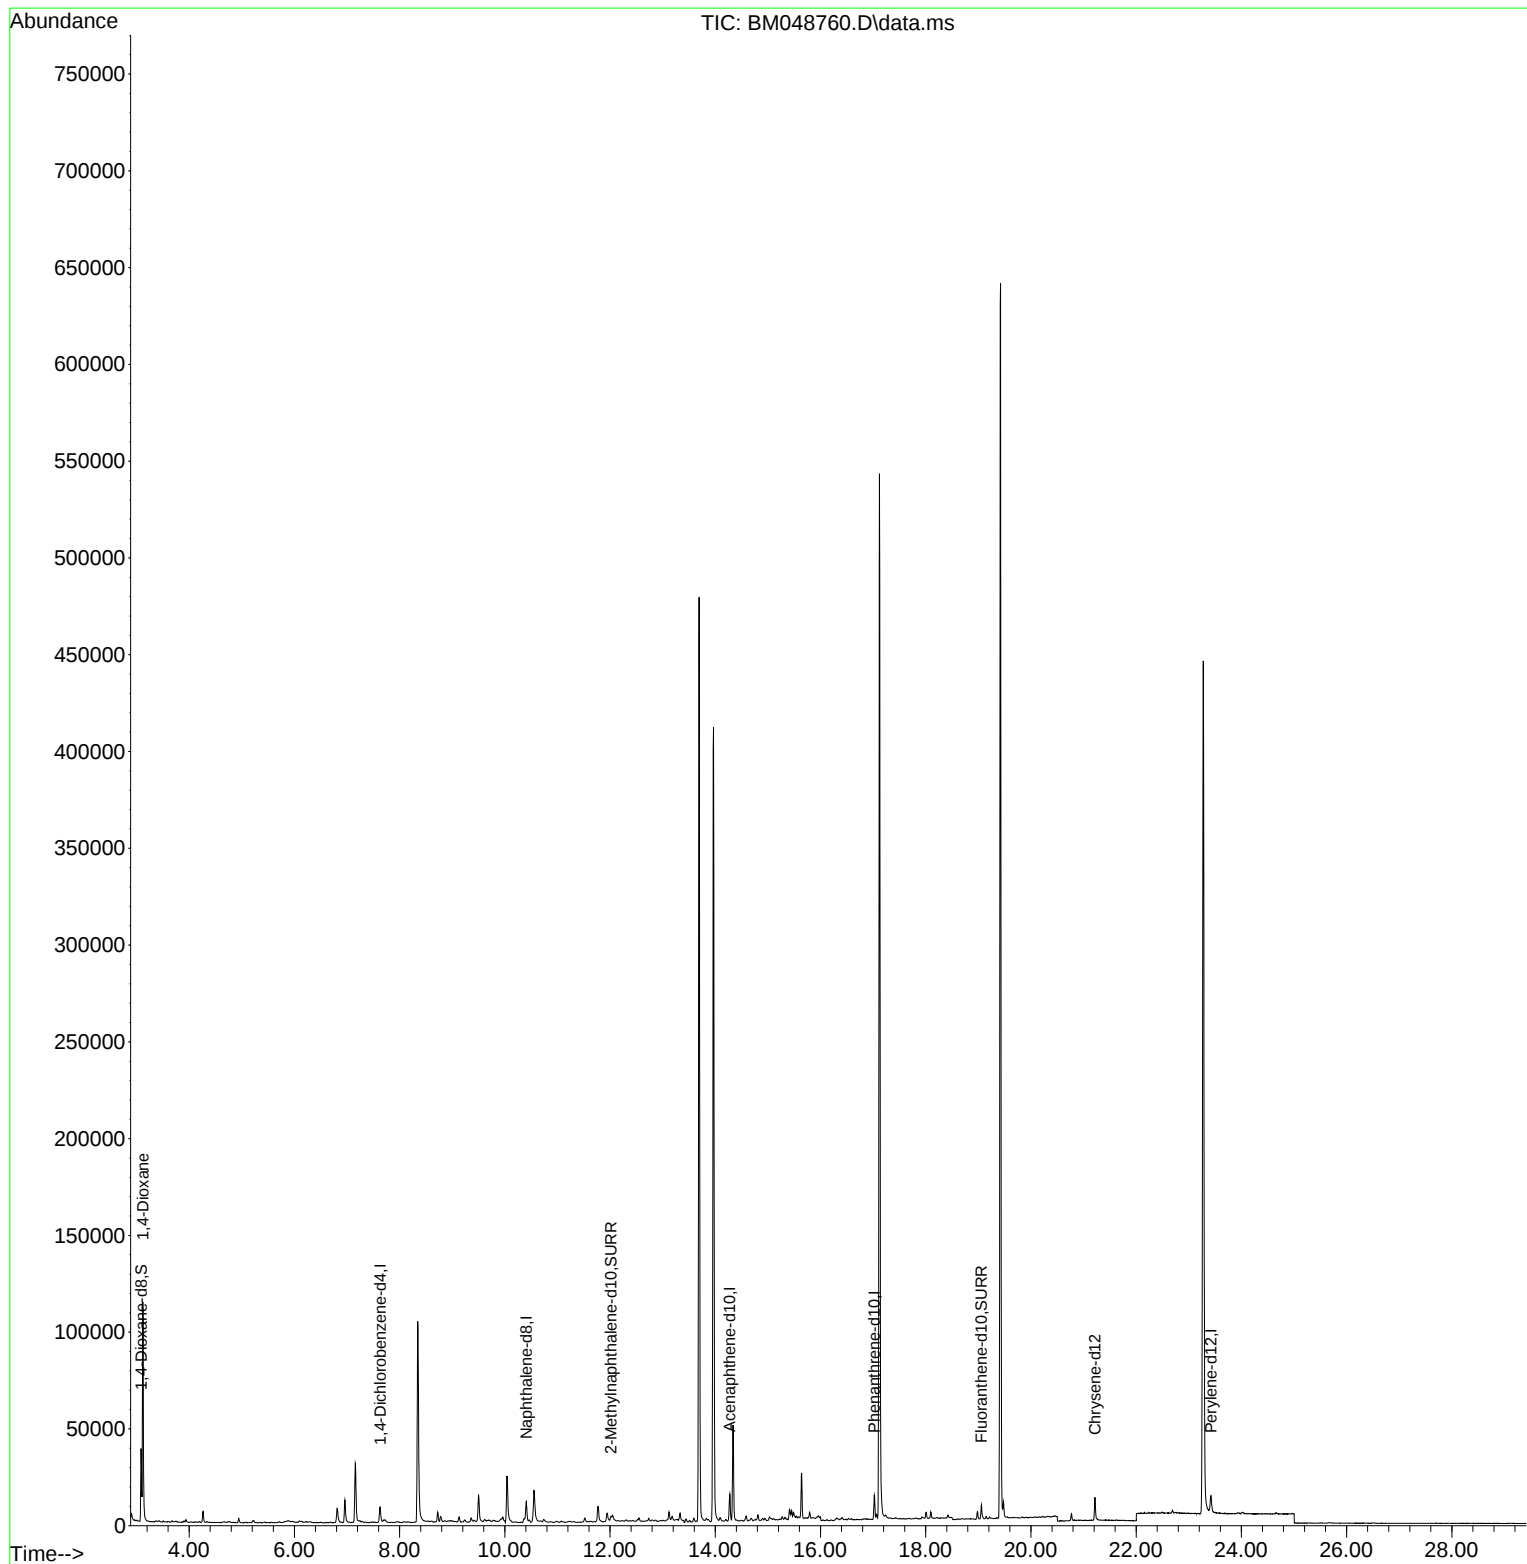

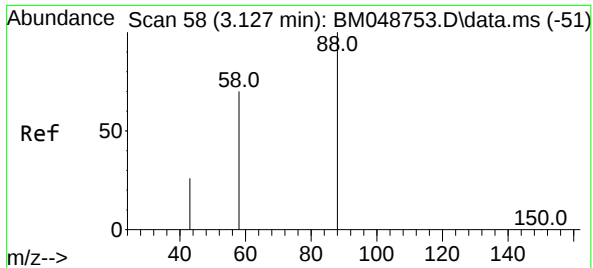

#2
1,4-Dioxane
Concen: 10.367 ng/ul
RT: 3.118 min Scan# 50
Delta R.T. -0.008 min
Lab File: BM048760.D
Acq: 17 Nov 2024 02:44

Instrument :
BNA_M
ClientSampleId :
CBA04

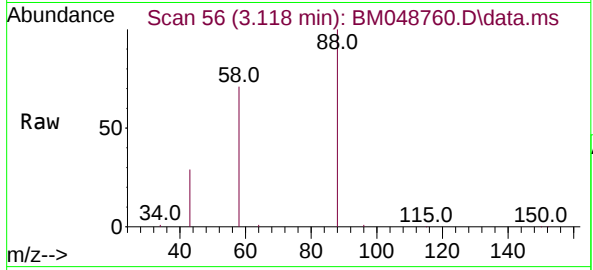

Tgt Ion: 88 Resp: 71184
Ion Ratio Lower Upper
88 100
43 28.8 60.2 90.4
58 71.1 44.2 66.2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

