

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM111721\  
 Data File : BM033147.D  
 Acq On : 18 Nov 2021 08:22  
 Operator : CG/JU  
 Sample : M4677-03  
 Misc :  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 H0AB2

Quant Time: Nov 18 10:12:54 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-BM111721.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Nov 17 14:14:11 2021  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units | Dev(Min)     |
|-------------------------------|--------|------|----------|--------|-------|--------------|
| -----                         |        |      |          |        |       |              |
| Internal Standards            |        |      |          |        |       |              |
| 1) 1,4-Dichlorobenzene-d4     | 7.972  | 152  | 132005   | 20.000 | ng/u1 | 0.00         |
| 20) Naphthalene-d8            | 10.766 | 136  | 533554   | 20.000 | ng/u1 | -0.01        |
| 38) Acenaphthene-d10          | 14.589 | 164  | 345431   | 20.000 | ng/u1 | 0.00         |
| 64) Phenanthrene-d10          | 17.324 | 188  | 701878   | 20.000 | ng/u1 | 0.00         |
| 79) Chrysene-d12              | 21.477 | 240  | 659213   | 20.000 | ng/u1 | 0.00         |
| 88) Perylene-d12              | 23.824 | 264  | 654130   | 20.000 | ng/u1 | -0.01        |
| System Monitoring Compounds   |        |      |          |        |       |              |
| 3) 1,4-Dioxane-d8             | 3.419  | 96   | 14665    | 4.283  | ng/uL | 0.00         |
| 4) Pyridine-d5                | 3.843  | 84   | 60939    | 6.461  | ng/u1 | 0.00         |
| 7) Phenol-d5                  | 7.119  | 99   | 55203    | 4.944  | ng/u1 | -0.01        |
| 9) Bis-(2-Chloroethyl)eth...  | 7.301  | 67   | 185500   | 26.192 | ng/u1 | 0.00         |
| 11) 2-Chlorophenol-d4         | 7.496  | 132  | 162587   | 19.225 | ng/u1 | -0.01        |
| 15) 4-Methylphenol-d8         | 8.660  | 113  | 104326   | 12.039 | ng/u1 | -0.01        |
| 21) Nitrobenzene-d5           | 9.125  | 128  | 110953   | 28.964 | ng/u1 | -0.01        |
| 24) 2-Nitrophenol-d4          | 9.848  | 143  | 105335   | 27.456 | ng/u1 | -0.01        |
| 28) 2,4-Dichlorophenol-d3     | 10.378 | 165  | 196835   | 22.404 | ng/u1 | -0.01        |
| 31) 4-Chloroaniline-d4        | 10.901 | 131  | 219891   | 18.820 | ng/u1 | 0.00         |
| 46) Dimethylphthalate-d6      | 13.995 | 166  | 754809   | 29.791 | ng/u1 | -0.01        |
| 49) Acenaphthylene-d8         | 14.283 | 160  | 864616   | 26.488 | ng/u1 | 0.00         |
| 54) 4-Nitrophenol-d4          | 14.766 | 143  | 17899    | 4.337  | ng/u1 | 0.00         |
| 60) Fluorene-d10              | 15.577 | 176  | 637850   | 28.063 | ng/u1 | 0.00         |
| 65) 4,6-Dinitro-2-methylph... | 15.683 | 200  | 92010    | 27.894 | ng/u1 | -0.01        |
| 73) Anthracene-d10            | 17.418 | 188  | 1059483  | 31.315 | ng/u1 | -0.01        |
| 81) Pyrene-d10                | 19.701 | 212  | 1253231  | 32.170 | ng/u1 | 0.00         |
| 92) Benzo(a)pyrene-d12        | 23.671 | 264  | 1157241  | 32.964 | ng/u1 | -0.01        |
| Target Compounds              |        |      |          |        |       |              |
| 47) Dimethylphthalate         | 14.042 | 163  | 61754    | 2.501  | ng/u1 | Qvalue<br>97 |
| -----                         |        |      |          |        |       |              |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM111721\  
Data File : BM033147.D  
Acq On : 18 Nov 2021 08:22  
Operator : CG/JU  
Sample : M4677-03  
Misc :  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
H0AB2

Quant Time: Nov 18 10:12:54 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-BM111721.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Nov 17 14:14:11 2021  
Response via : Initial Calibration

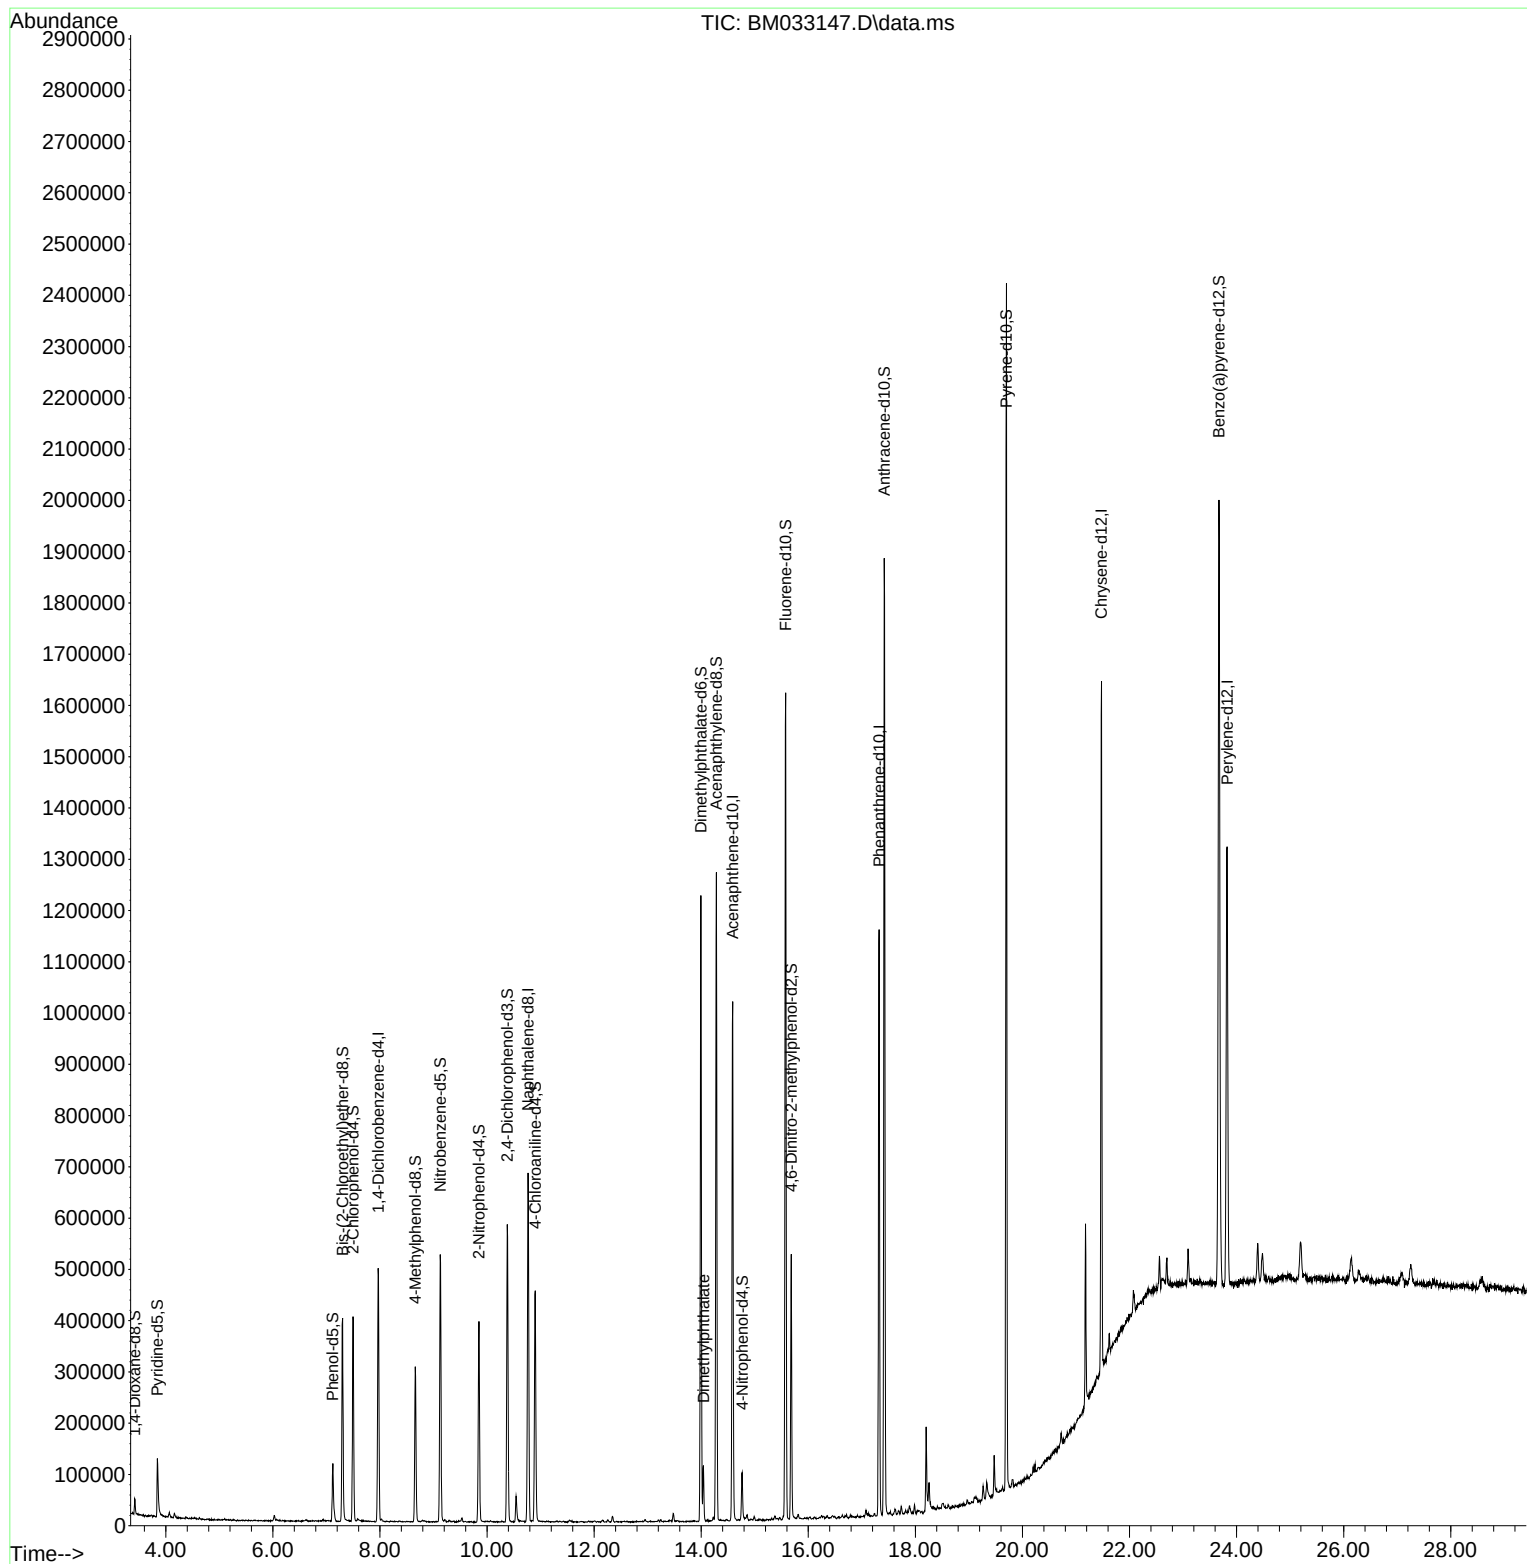

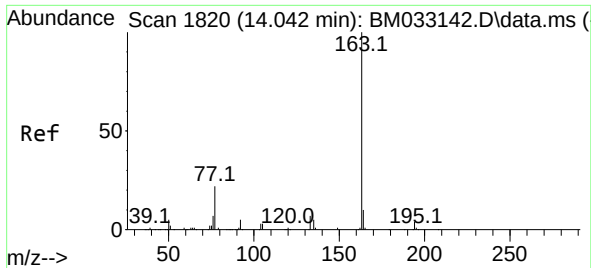

#47  
 Dimethylphthalate  
 Concen: 2.501 ng/ul  
 RT: 14.042 min Scan# 11  
 Delta R.T. -0.012 min  
 Lab File: BM033147.D  
 Acq: 18 Nov 2021 08:22

Instrument :  
 BNA\_M  
 ClientSampleId :  
 H0AB2

|             |       |             |
|-------------|-------|-------------|
| Tgt Ion:163 | Resp: | 61754       |
| Ion         | Ratio | Lower Upper |
| 163         | 100   |             |
| 194         | 4.0   | 3.1 4.7     |
| 164         | 11.2  | 7.7 11.5    |

