

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033152.D
 Acq On : 18 Nov 2021 13:42
 Operator : CG/JU
 Sample : M4677-13
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AA7

Quant Time: Nov 18 14:23:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 17 14:14:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.966	152	108356	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.766	136	420819	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.583	164	261284	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.324	188	531959	20.000	ng/u1	0.00
79) Chrysene-d12	21.477	240	551955	20.000	ng/u1	0.00
88) Perylene-d12	23.830	264	563212	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.419	96	15680	5.579	ng/uL	0.00
4) Pyridine-d5	3.843	84	73753	9.526	ng/u1	0.00
7) Phenol-d5	7.119	99	62702	6.841	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.296	67	188018	32.342	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.496	132	173337	24.969	ng/u1	-0.01
15) 4-Methylphenol-d8	8.660	113	111826	15.721	ng/u1	-0.01
21) Nitrobenzene-d5	9.125	128	108215	35.817	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.848	143	108159	35.745	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.378	165	196485	28.356	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.895	131	252164	27.364	ng/u1	-0.01
46) Dimethylphthalate-d6	13.995	166	624868	32.605	ng/u1	-0.01
49) Acenaphthylene-d8	14.278	160	779322	31.564	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.766	143	18271	5.853	ng/u1	0.00
60) Fluorene-d10	15.572	176	549823	31.981	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.683	200	77684	31.074	ng/u1	-0.01
73) Anthracene-d10	17.418	188	898842	35.053	ng/u1	-0.01
81) Pyrene-d10	19.701	212	1089149	33.392	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.677	264	1091502	36.111	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.455	88	20151	7.061	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033152.D
Acq On : 18 Nov 2021 13:42
Operator : CG/JU
Sample : M4677-13
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AA7

Quant Time: Nov 18 14:23:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 17 14:14:11 2021
Response via : Initial Calibration

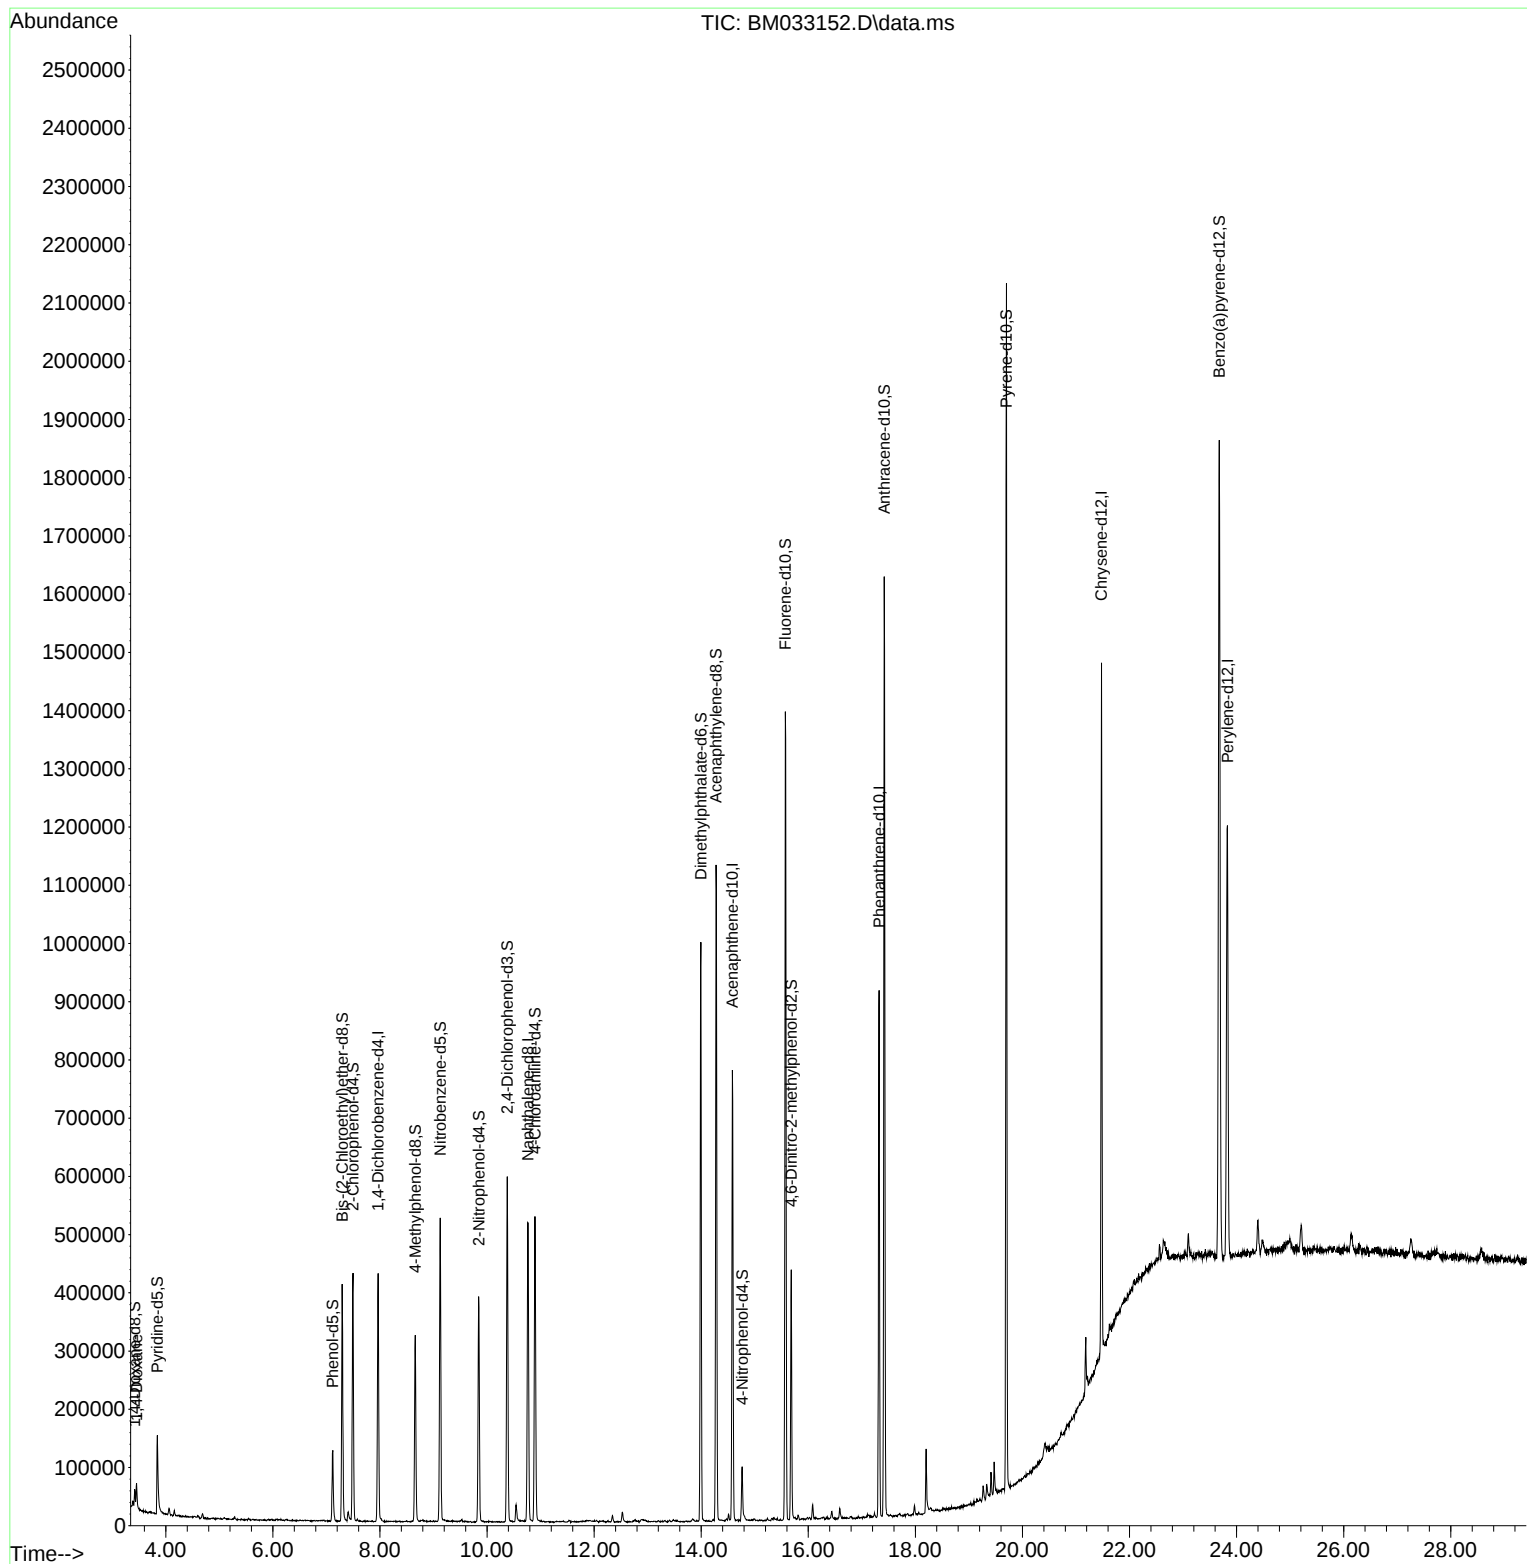

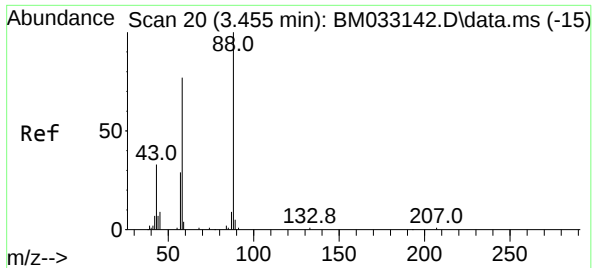

1,4-Dioxane
 Concen: 7.061 ng/uL
 RT: 3.455 min Scan# 20
 Delta R.T. -0.005 min
 Lab File: BM033152.D
 Acq: 18 Nov 2021 13:42

Instrument :
 BNA_M
 ClientSampleId :
 H0AA7

Tgt Ion: 88	Resp:	20151
Ion	Ratio	Lower Upper
88	100	
43	40.8	34.9 52.3
58	85.4	70.0 105.0

