

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033156.D
 Acq On : 18 Nov 2021 16:08
 Operator : CG/JU
 Sample : M4615-05ME
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COV04ME

Quant Time: Nov 18 16:42:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 17 14:14:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.972	152	113633	20.000	ng/u1	0.00
20) Naphthalene-d8	10.766	136	501484	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.589	164	336681	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.324	188	688088	20.000	ng/u1	0.00
79) Chrysene-d12	21.477	240	563014	20.000	ng/u1	0.00
88) Perylene-d12	23.824	264	490710	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.425	96	7809	2.649	ng/uL	0.00
4) Pyridine-d5	3.843	84	108174	13.323	ng/u1	0.00
7) Phenol-d5	7.137	99	172314	17.927	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.307	67	99995	16.402	ng/u1	0.00
11) 2-Chlorophenol-d4	7.501	132	120924	16.610	ng/u1	0.00
15) 4-Methylphenol-d8	8.660	113	145989	19.571	ng/u1	-0.01
21) Nitrobenzene-d5	9.131	128	62663	17.404	ng/u1	0.00
24) 2-Nitrophenol-d4	9.848	143	79307	21.994	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.384	165	138253	16.743	ng/u1	0.00
31) 4-Chloroaniline-d4	10.901	131	79110	7.204	ng/u1	0.00
46) Dimethylphthalate-d6	13.995	166	468265	18.962	ng/u1	-0.01
49) Acenaphthylene-d8	14.283	160	539500	16.958	ng/u1	0.00
54) 4-Nitrophenol-d4	14.766	143	60770	15.107	ng/u1	0.00
60) Fluorene-d10	15.572	176	394209	17.795	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.683	200	50835	15.720	ng/u1	-0.01
73) Anthracene-d10	17.418	188	617619	18.621	ng/u1	-0.01
81) Pyrene-d10	19.701	212	705471	21.204	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.671	264	492737	18.710	ng/u1	-0.01
Target Compounds						
					Qvalue	
8) Phenol	7.184	94	7428932	776.131	ng/u1	99
16) Acetophenone	8.796	105	29391	2.496	ng/u1	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033156.D
Acq On : 18 Nov 2021 16:08
Operator : CG/JU
Sample : M4615-05ME
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0V04ME

Quant Time: Nov 18 16:42:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 17 14:14:11 2021
Response via : Initial Calibration




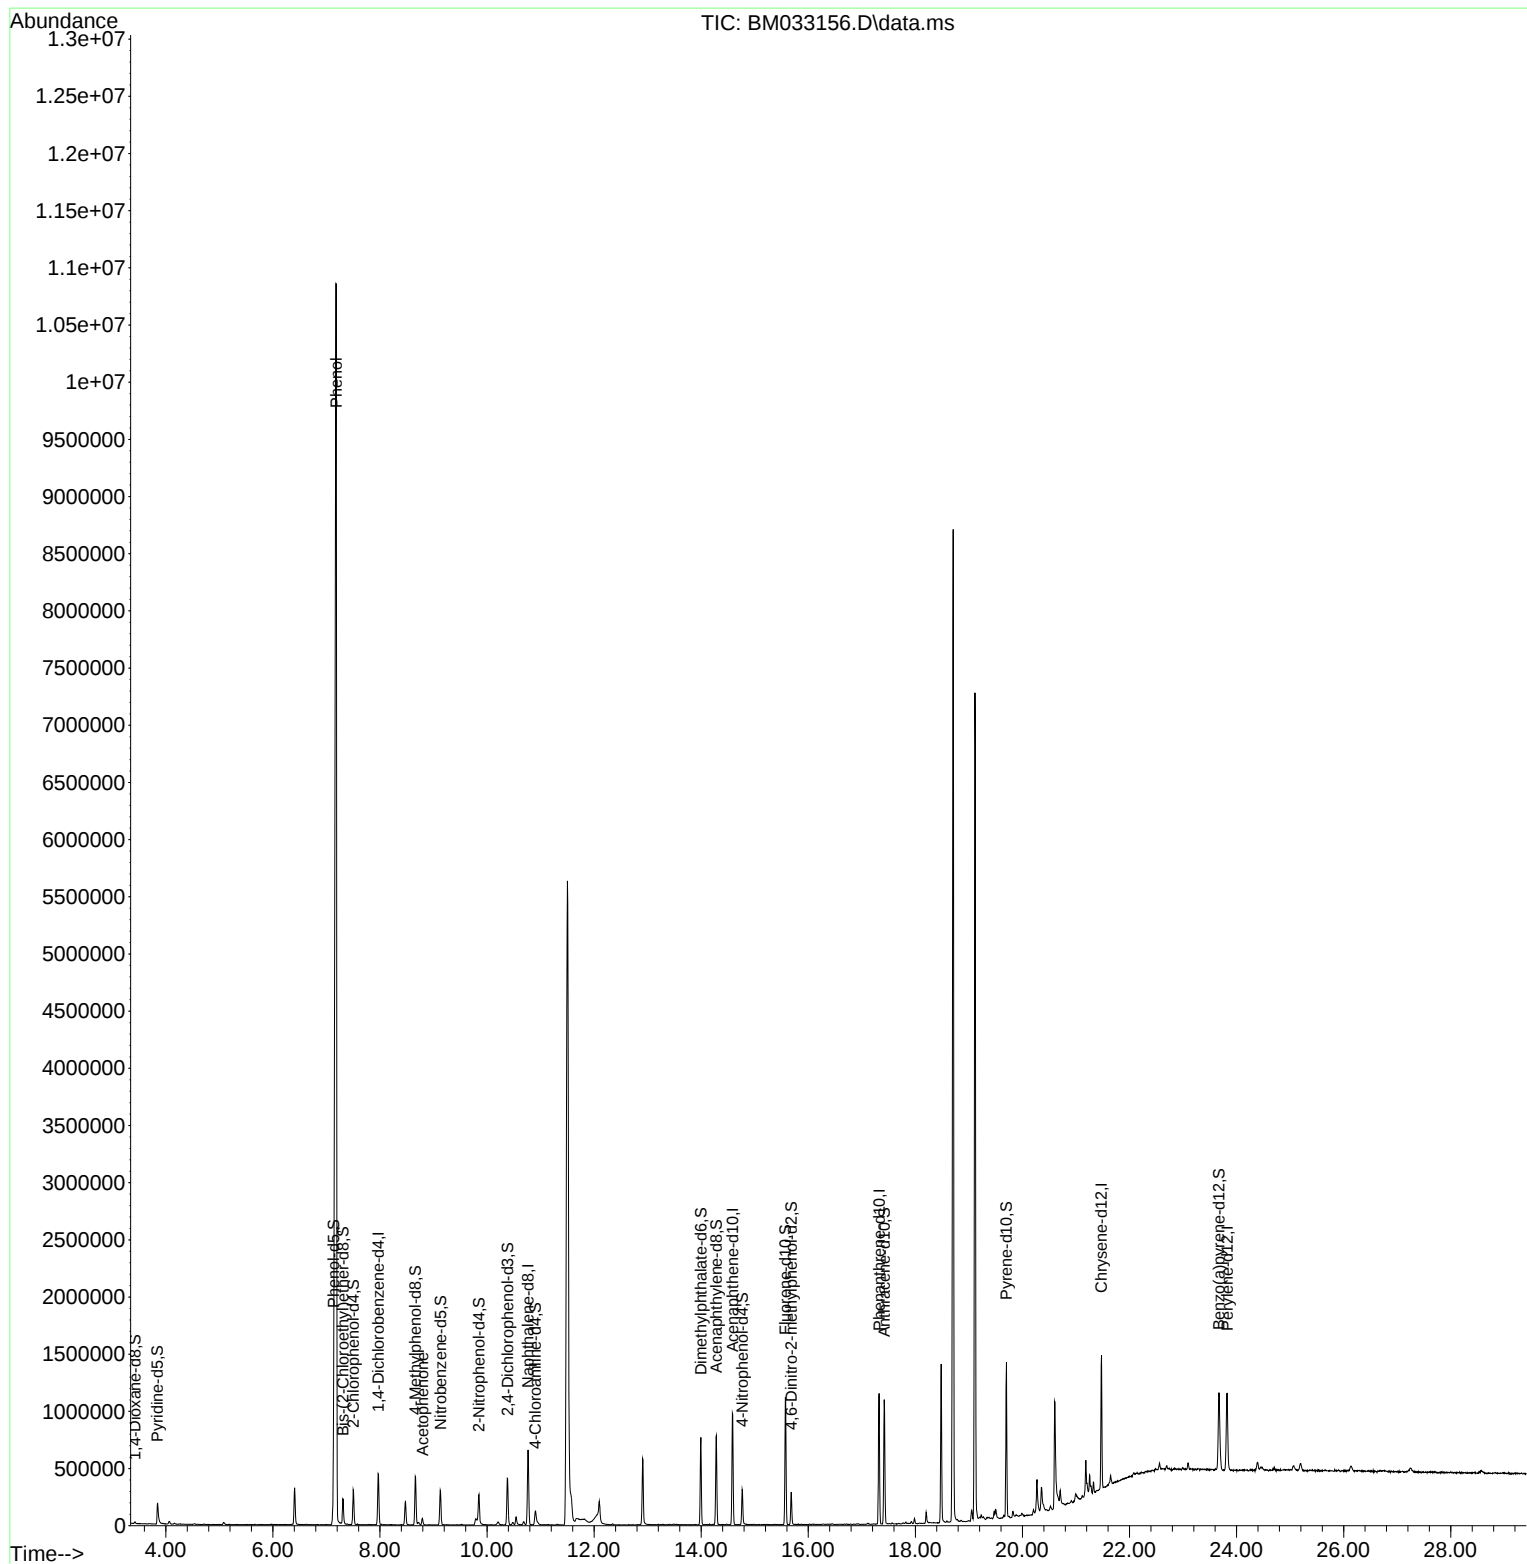


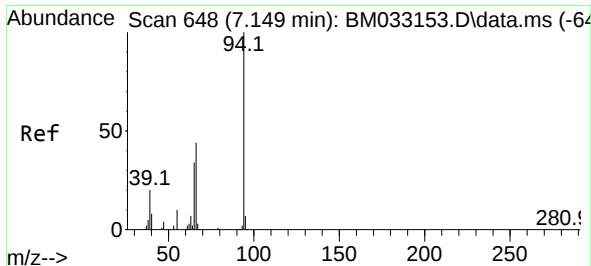

#8
Phenol
Concen: 776.131 ng/ul
RT: 7.184 min Scan# 61
Delta R.T. 0.030 min
Lab File: BM033156.D
Acq: 18 Nov 2021 16:08

Instrument :
BNA_M
ClientSampleId :
COV04ME

Tgt Ion: 94 Resp: 7428932
Ion Ratio Lower Upper
94 100
65 34.0 27.1 40.7
66 48.1 39.4 59.2

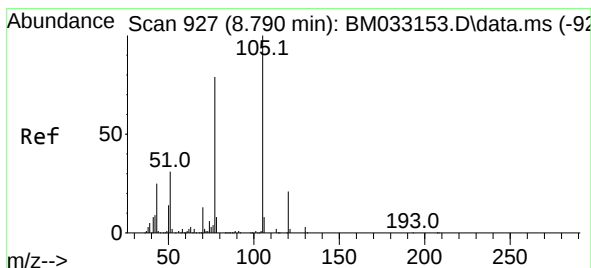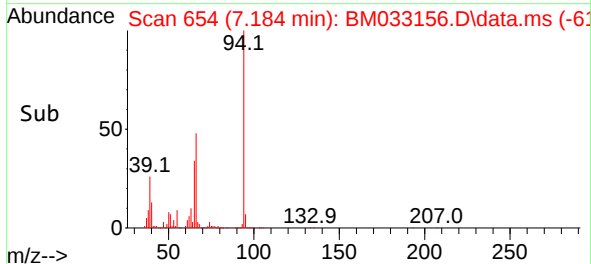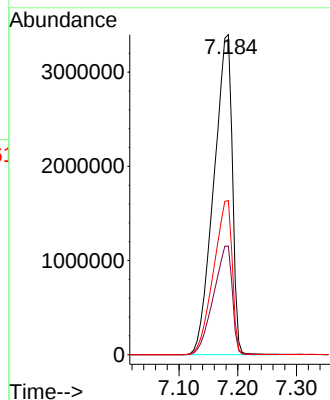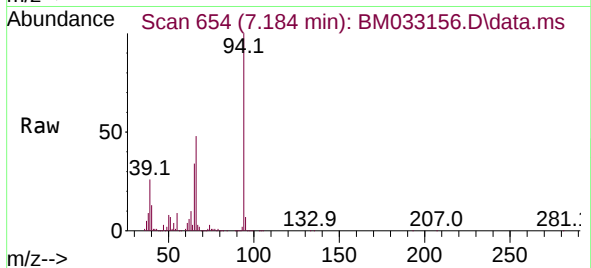

#16
Acetophenone
Concen: 2.496 ng/ul
RT: 8.796 min Scan# 928
Delta R.T. -0.006 min
Lab File: BM033156.D
Acq: 18 Nov 2021 16:08

Tgt Ion: 105 Resp: 29391
Ion Ratio Lower Upper
105 100
77 82.7 68.0 102.0
51 32.0 27.8 41.8

