

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033159.D
 Acq On : 18 Nov 2021 17:58
 Operator : CG/JU
 Sample : M4615-05MEDL 10X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COV04MEDL

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/19/2021
 Supervised By :mohammad ahmed 11/26/2021

Quant Time: Nov 19 00:47:42 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 17 14:14:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.966	152	117679	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.766	136	507020	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.583	164	350533	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.318	188	727994	20.000	ng/u1	-0.01
79) Chrysene-d12	21.477	240	580827	20.000	ng/u1	0.00
88) Perylene-d12	23.824	264	485363	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.425	96	1194m	0.391	ng/uL	0.00
4) Pyridine-d5	3.860	84	7675	0.913	ng/u1	0.01
7) Phenol-d5	7.125	99	17146	1.723	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.295	67	10217	1.618	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.495	132	11830	1.569	ng/u1	-0.01
15) 4-Methylphenol-d8	8.666	113	13847	1.792	ng/u1	0.00
21) Nitrobenzene-d5	9.131	128	6266	1.721	ng/u1	0.00
24) 2-Nitrophenol-d4	9.842	143	5454	1.496	ng/u1	-0.02
28) 2,4-Dichlorophenol-d3	10.389	165	13186	1.579	ng/u1	0.00
31) 4-Chloroaniline-d4	10.901	131	9563	0.861	ng/u1	0.00
46) Dimethylphthalate-d6	13.995	166	50563	1.967	ng/u1	-0.01
49) Acenaphthylene-d8	14.277	160	52150	1.574	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.771	143	4998	1.193	ng/u1	0.00
60) Fluorene-d10	15.571	176	41198	1.786	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.683	200	3854	1.126	ng/u1	-0.01
73) Anthracene-d10	17.418	188	67289m	1.917	ng/u1	-0.01
81) Pyrene-d10	19.695	212	75883	2.211	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.671	264	48120	1.847	ng/u1	-0.01
Target Compounds						Qvalue
8) Phenol	7.148	94	816427	82.363	ng/u1	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033159.D
Acq On : 18 Nov 2021 17:58
Operator : CG/JU
Sample : M4615-05MEDL 10X
Misc :
ALS Vial : 46 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0V04MEDL

Quant Time: Nov 19 00:47:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 17 14:14:11 2021
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/19/2021
Supervised By :mohammad ahmed 11/26/2021

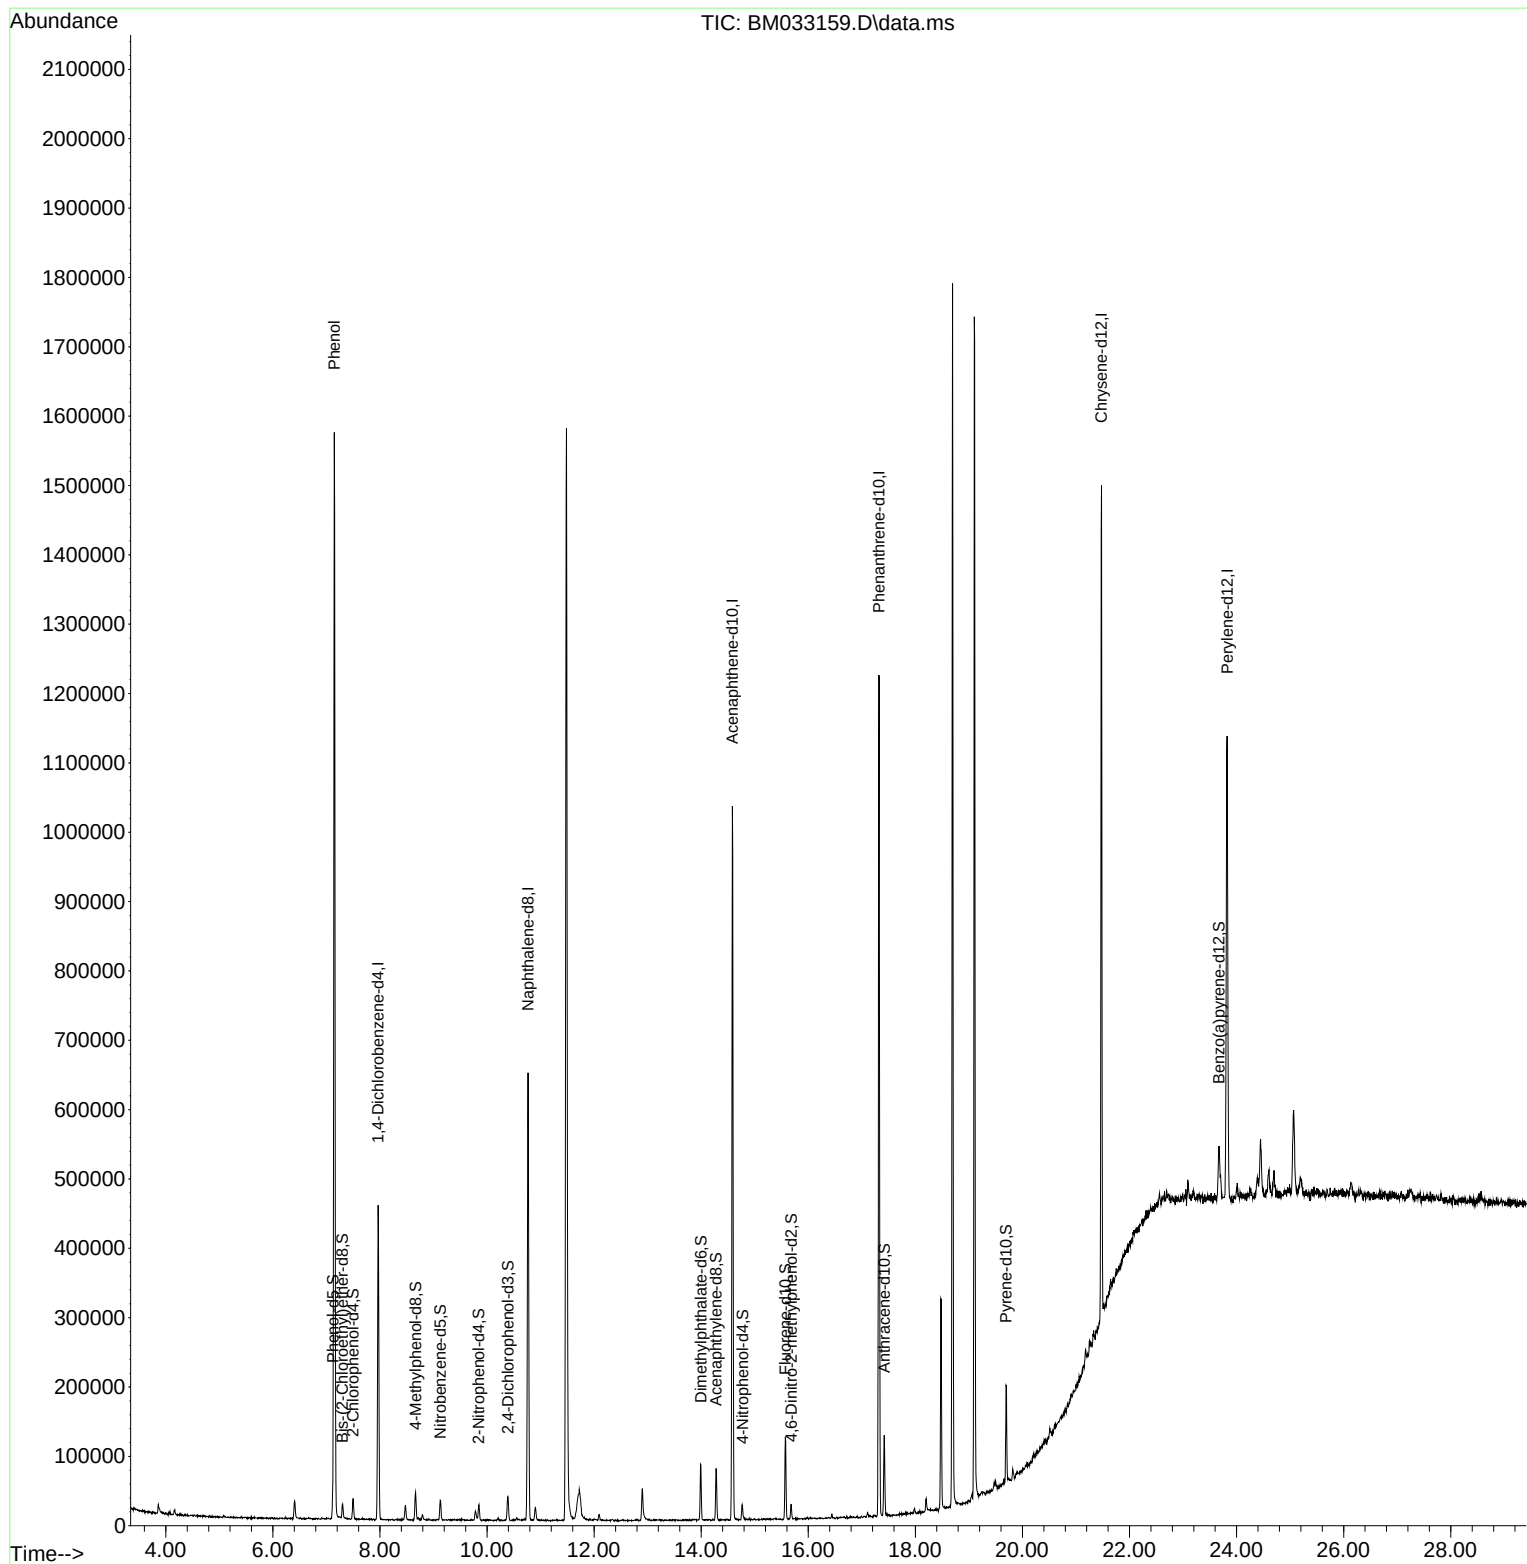

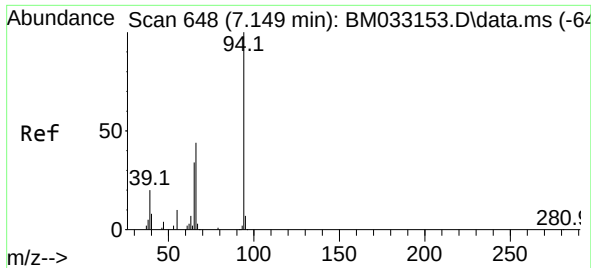

#8
Phenol
Concen: 82.363 ng/ul
RT: 7.148 min Scan# 64
Delta R.T. -0.006 min
Lab File: BM033159.D
Acq: 18 Nov 2021 17:58

Instrument :
BNA_M
ClientSampleId :
C0V04MEDL

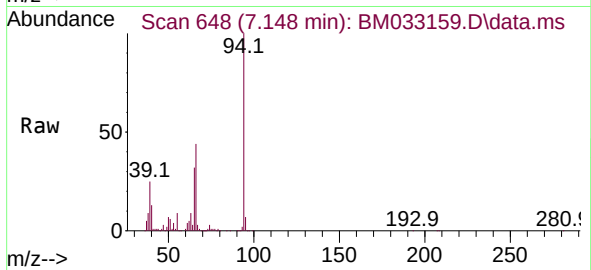

Tgt Ion: 94 Resp: 81642
Ion Ratio Lower Upper
94 100
65 32.2 27.1 40.7
66 44.3 39.4 59.2

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/19/2021
Supervised By :mohammad ahmed 11/26/2021

