

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033160.D
 Acq On : 18 Nov 2021 18:34
 Operator : CG/JU
 Sample : M4615-05MEDL2 20X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0V04MEDL2

Quant Time: Nov 19 00:48:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 17 14:14:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.966	152	110954	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.766	136	466174	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.583	164	328824	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.318	188	712272	20.000	ng/u1	-0.01
79) Chrysene-d12	21.477	240	653134	20.000	ng/u1	0.00
88) Perylene-d12	23.824	264	544656	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.431	96	530	0.184	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.119	99	7012	0.747	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.296	67	4502	0.756	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.495	132	4876	0.686	ng/u1	-0.01
15) 4-Methylphenol-d8	8.660	113	5675	0.779	ng/u1	-0.01
21) Nitrobenzene-d5	9.131	128	2684	0.802	ng/u1	0.00
24) 2-Nitrophenol-d4	9.848	143	2638	0.787	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.384	165	4852	0.632	ng/u1	0.00
31) 4-Chloroaniline-d4	10.907	131	4531	0.444	ng/u1	0.00
46) Dimethylphthalate-d6	13.995	166	21964	0.911	ng/u1	-0.01
49) Acenaphthylene-d8	14.283	160	21895	0.705	ng/u1	0.00
54) 4-Nitrophenol-d4	14.772	143	1962	0.499	ng/u1	0.00
60) Fluorene-d10	15.571	176	19062	0.881	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.683	200	1622	0.485	ng/u1	-0.01
73) Anthracene-d10	17.418	188	30853	0.899	ng/u1	-0.01
81) Pyrene-d10	19.701	212	35604	0.922	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.671	264	24990	0.855	ng/u1	-0.01
Target Compounds						
					Qvalue	
8) Phenol	7.148	94	350986	37.554	ng/u1	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033160.D
Acq On : 18 Nov 2021 18:34
Operator : CG/JU
Sample : M4615-05MEDL2 20X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0V04MEDL2

Quant Time: Nov 19 00:48:03 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 17 14:14:11 2021
Response via : Initial Calibration

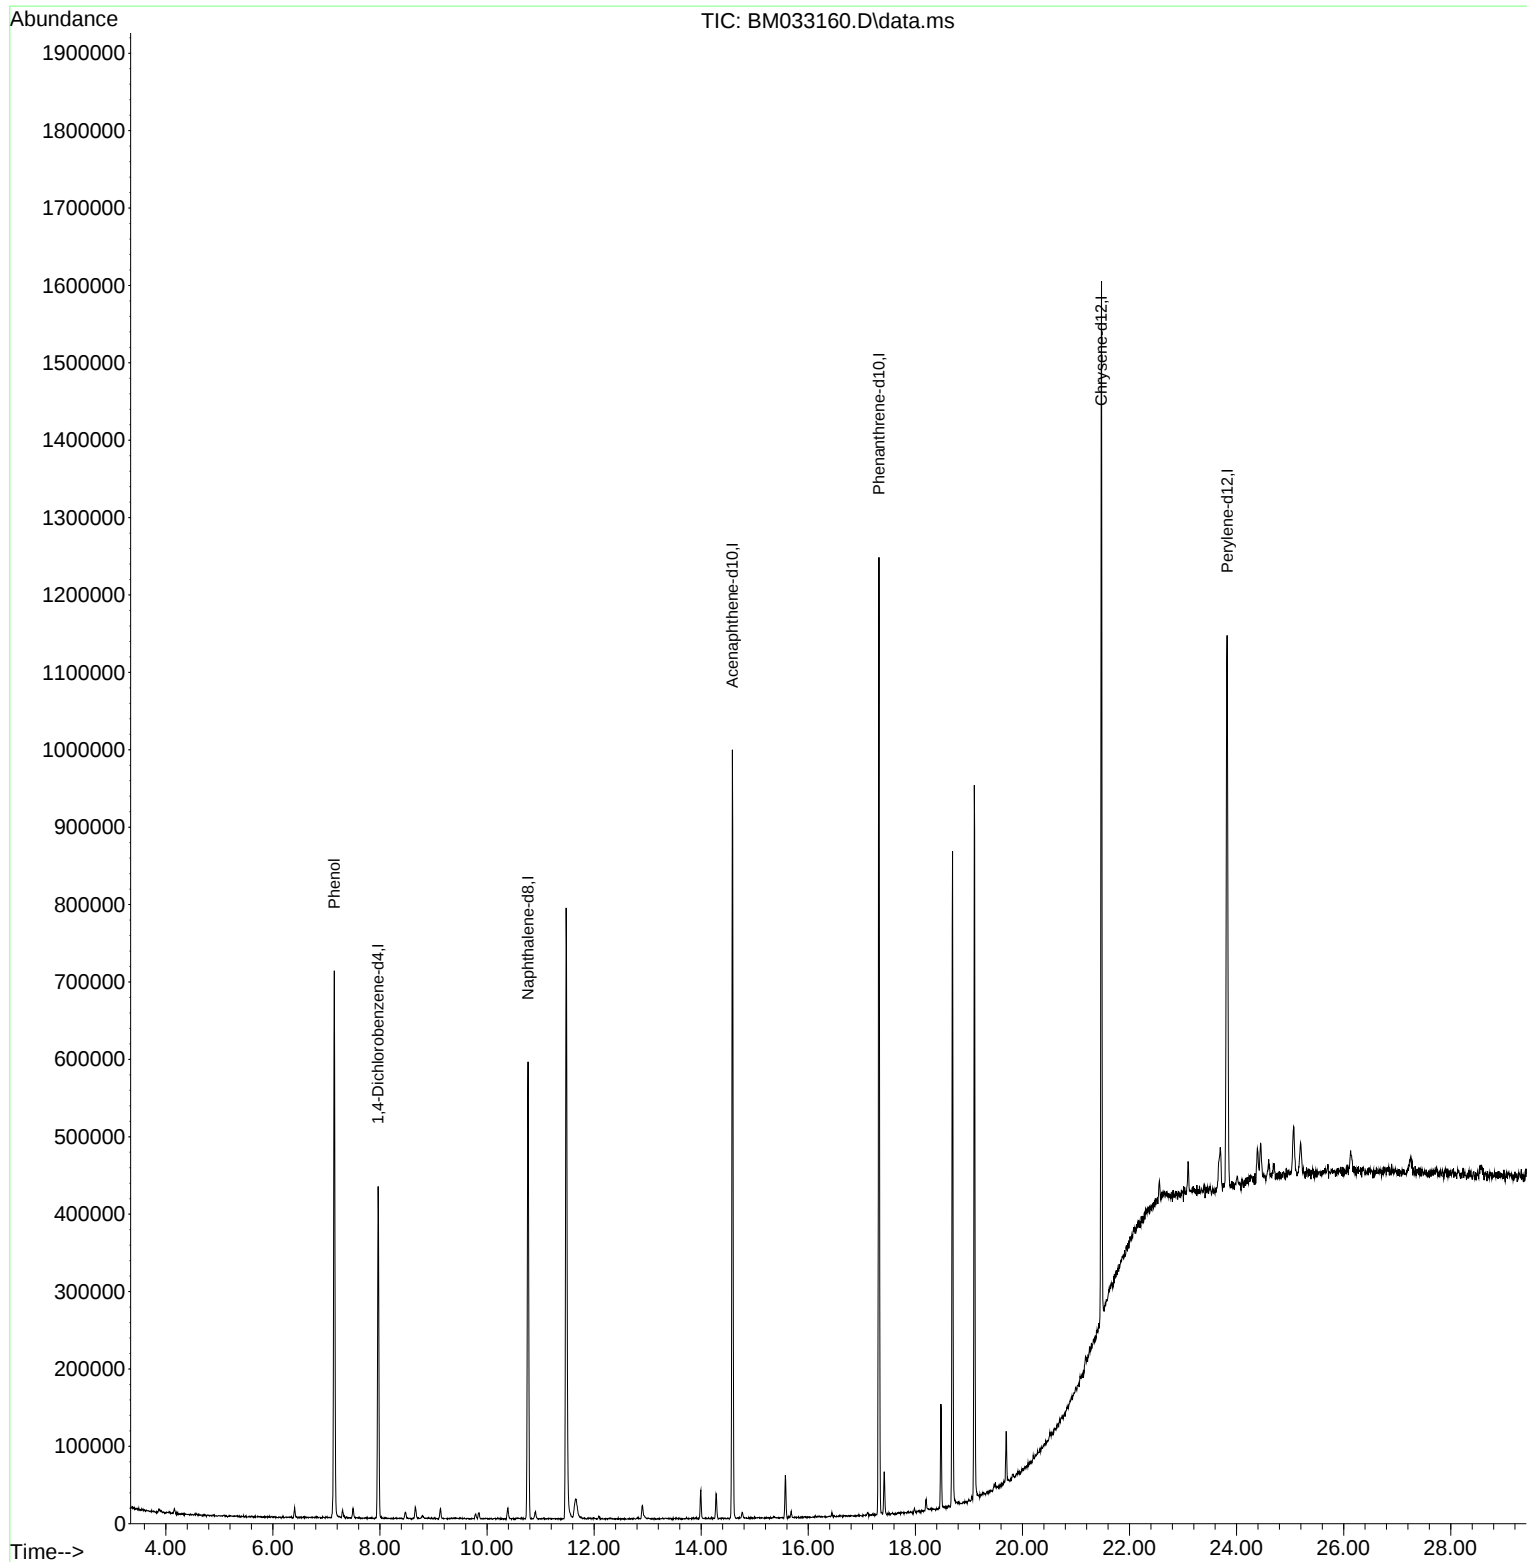

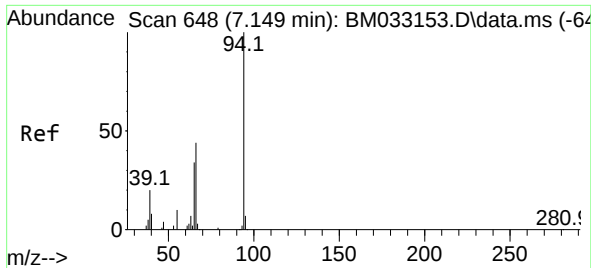

#8
Phenol
Concen: 37.554 ng/ul
RT: 7.148 min Scan# 64
Delta R.T. -0.006 min
Lab File: BM033160.D
Acq: 18 Nov 2021 18:34

Instrument :
BNA_M
ClientSampleId :
C0V04MEDL2

Tgt Ion: 94 Resp: 350986
Ion Ratio Lower Upper
94 100
65 32.8 27.1 40.7
66 46.0 39.4 59.2

