

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033168.D
 Acq On : 18 Nov 2021 23:24
 Operator : CG/JU
 Sample : M4669-09
 Misc : GCMS CONFIRMATION
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4272

Quant Time: Nov 19 01:06:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 17 14:14:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.966	152	116016	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.760	136	445654	20.000	ng/ul	#-0.02
38) Acenaphthene-d10	14.583	164	287769	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.318	188	632793	20.000	ng/ul	-0.01
79) Chrysene-d12	21.471	240	484528	20.000	ng/ul	-0.01
88) Perylene-d12	23.818	264	454844	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0	0.000	ng/ul	
7) Phenol-d5	0.000	99	0	0.000	ng/ul	
9) Bis-(2-Chloroethyl)eth...	0.000	67	0	0.000	ng/ul	
11) 2-Chlorophenol-d4	0.000	132	0	0.000	ng/ul	
15) 4-Methylphenol-d8	0.000	113	0	0.000	ng/ul	
21) Nitrobenzene-d5	0.000	128	0	0.000	ng/ul	
24) 2-Nitrophenol-d4	0.000	143	0	0.000	ng/ul	
28) 2,4-Dichlorophenol-d3	0.000	165	0	0.000	ng/ul	
31) 4-Chloroaniline-d4	0.000	131	0d	0.000	ng/ul	
46) Dimethylphthalate-d6	0.000	166	0	0.000	ng/ul	
49) Acenaphthylene-d8	0.000	160	0	0.000	ng/ul	
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	0.000	176	0d	0.000	ng/ul	
65) 4,6-Dinitro-2-methylph...	0.000	200	0	0.000	ng/ul	
73) Anthracene-d10	0.000	188	0d	0.000	ng/ul	
81) Pyrene-d10	0.000	212	0d	0.000	ng/ul	
92) Benzo(a)pyrene-d12	0.000	264	0d	0.000	ng/ul	
Target Compounds						
					Qvalue	
61) Fluorene	15.624	166	24292	1.158	ng/ul#	55
86) Bis(2-ethylhexyl)phtha...	21.377	149	22037	1.336	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033168.D
Acq On : 18 Nov 2021 23:24
Operator : CG/JU
Sample : M4669-09
Misc : GCMS CONFIRMATION
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4272

Quant Time: Nov 19 01:06:01 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 17 14:14:11 2021
Response via : Initial Calibration




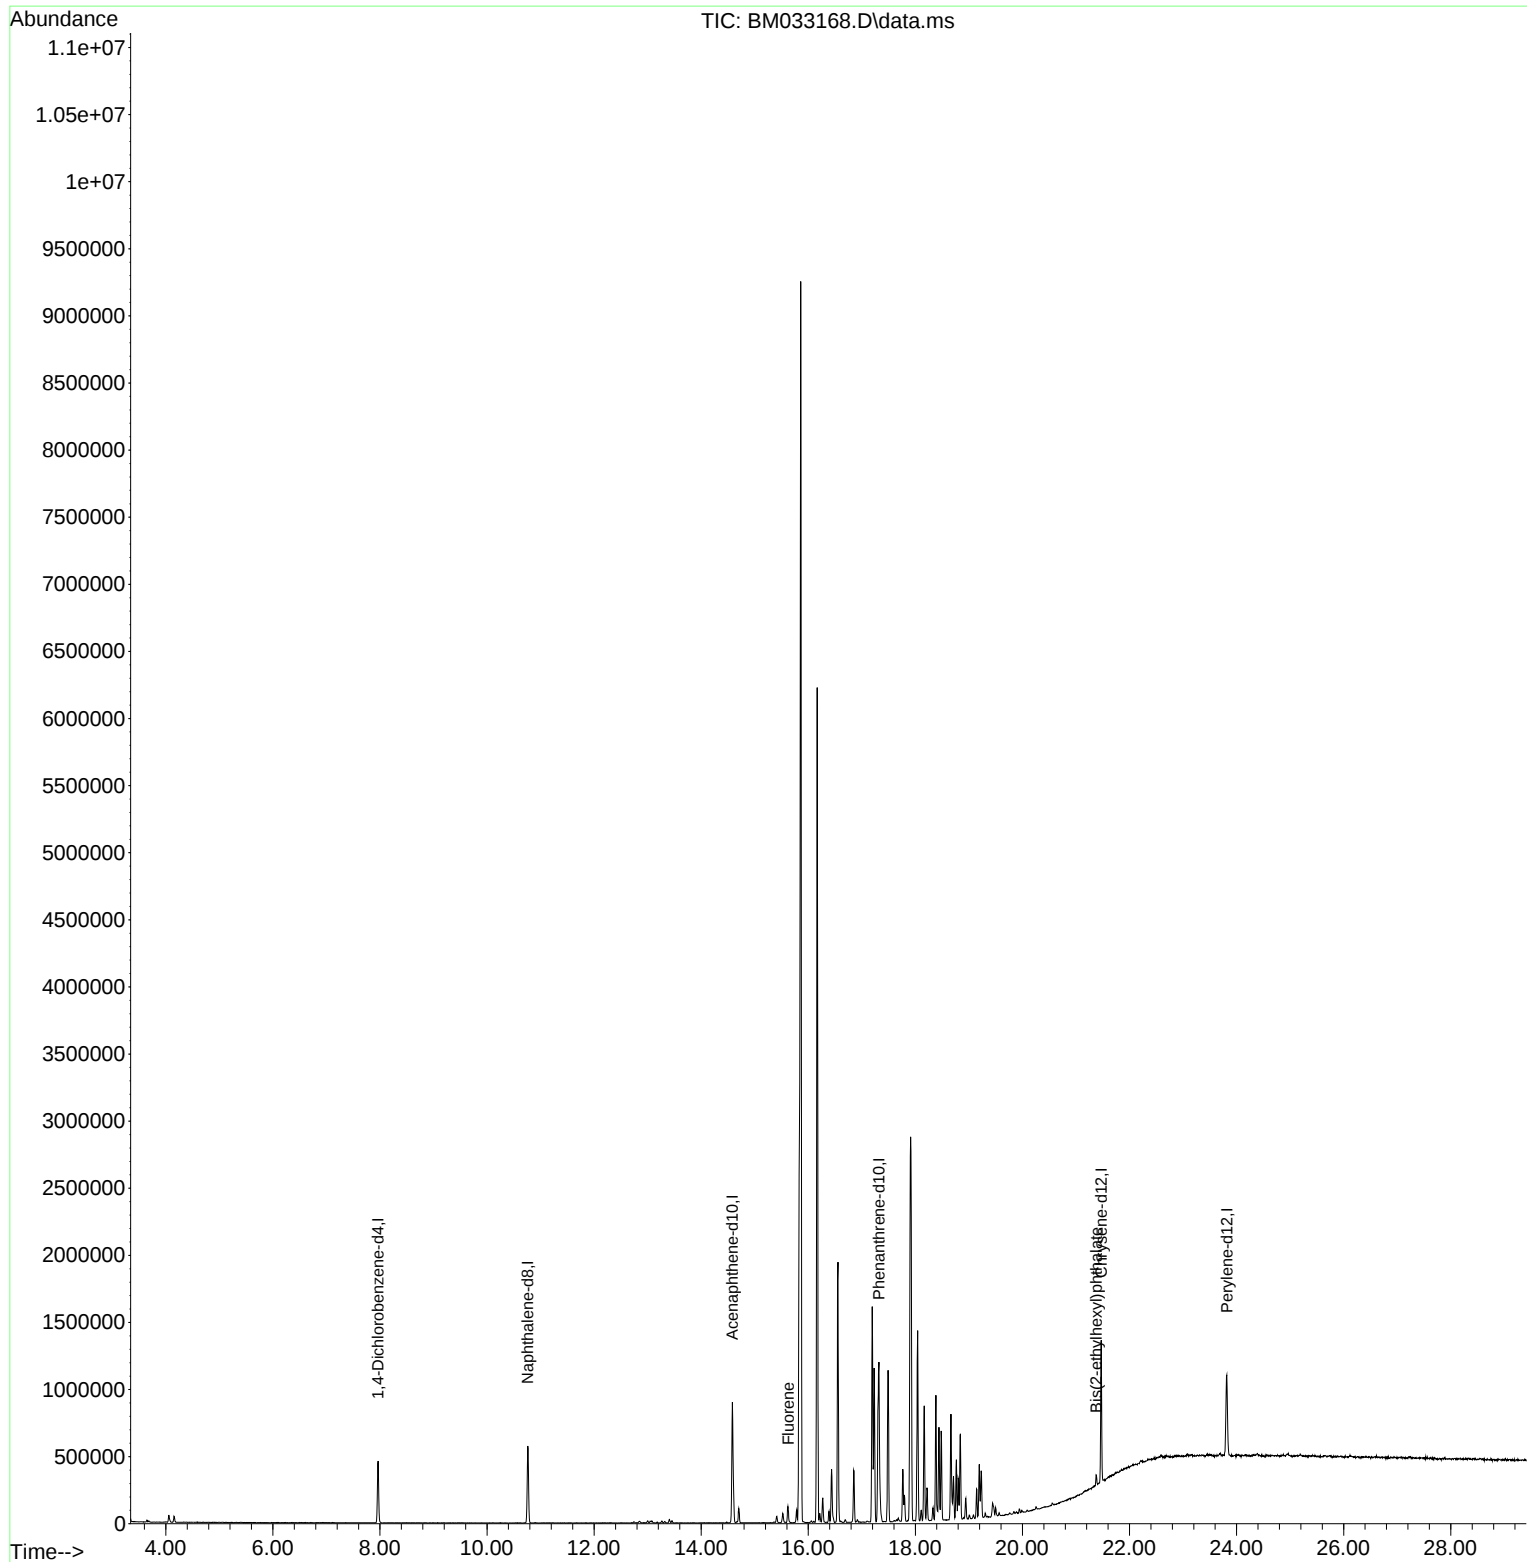


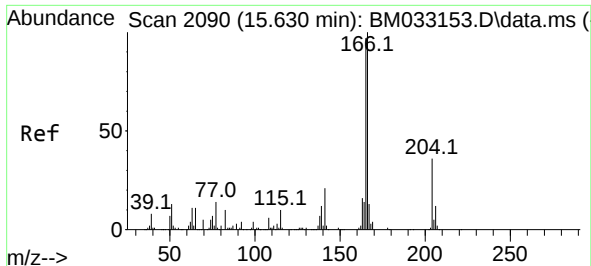

#61
Fluorene
Concen: 1.158 ng/ul
RT: 15.624 min Scan# 2090
Delta R.T. -0.012 min
Lab File: BM033168.D
Acq: 18 Nov 2021 23:24

Instrument :
BNA_M
ClientSampleId :
A4272

Tgt Ion:166 Resp: 24292
Ion Ratio Lower Upper
166 100
165 110.4 76.8 115.2
167 119.2 10.7 16.1#

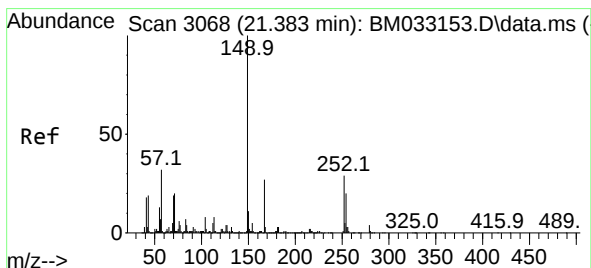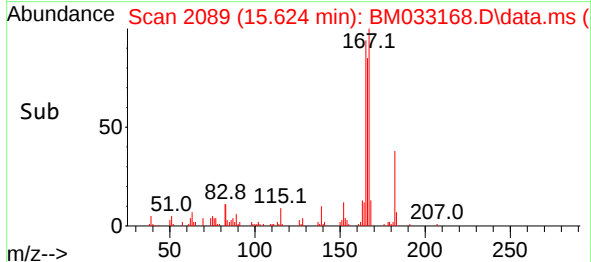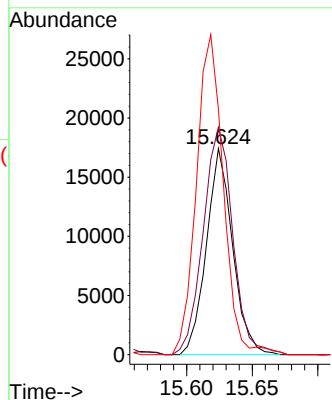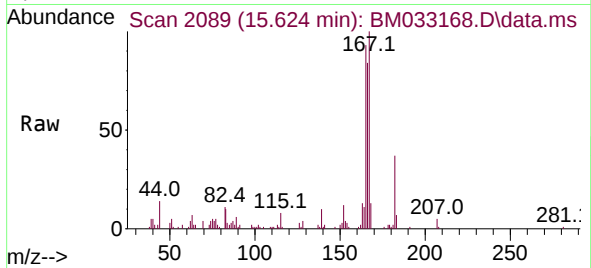

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.336 ng/ul
RT: 21.377 min Scan# 3067
Delta R.T. -0.018 min
Lab File: BM033168.D
Acq: 18 Nov 2021 23:24

Tgt Ion:149 Resp: 22037
Ion Ratio Lower Upper
149 100
167 27.7 22.1 33.1
279 4.6 3.4 5.2

