

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033123.D
 Acq On : 17 Nov 2021 15:12
 Operator : CG/JU
 Sample : PB140812BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK812

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033123.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.425	11	15	21	rVB	27873	37895	1.91%	0.171%
2	3.549	34	36	38	rBV2	3265	2495	0.13%	0.011%
3	3.843	83	86	102	rBV	345879	532553	26.82%	2.397%
4	4.037	117	119	121	rVB3	2384	2159	0.11%	0.010%
5	4.120	132	133	136	rVB3	3539	3204	0.16%	0.014%
6	4.149	136	138	139	rBV2	3261	3128	0.16%	0.014%
7	4.167	139	141	144	rVB3	5544	6176	0.31%	0.028%
8	4.790	245	247	251	rBV3	2090	2096	0.11%	0.009%
9	5.031	284	288	291	rVB5	1786	2469	0.12%	0.011%
10	5.172	310	312	317	rVB6	1723	2666	0.13%	0.012%
11	5.743	405	409	411	rVB5	1839	2818	0.14%	0.013%
12	5.931	440	441	447	rBV6	1591	2309	0.12%	0.010%
13	6.337	509	510	513	rBV3	2525	2093	0.11%	0.009%
14	6.872	599	601	604	rVB4	2444	2982	0.15%	0.013%
15	7.125	637	644	652	rBV	419953	669942	33.74%	3.015%
16	7.308	669	675	686	rVB	284024	472593	23.80%	2.127%
17	7.508	702	709	720	rBV	393370	663103	33.40%	2.984%
18	7.972	781	788	796	rBV	319070	528615	26.62%	2.379%
19	8.043	798	800	805	rVB4	2091	1986	0.10%	0.009%
20	8.313	842	846	847	rBV3	2238	2054	0.10%	0.009%
21	8.396	855	860	863	rBV6	2167	3687	0.19%	0.017%
22	8.566	885	889	891	rBV4	1321	2001	0.10%	0.009%
23	8.666	899	906	916	rVV	468670	775264	39.05%	3.489%
24	8.737	916	918	923	rVB5	2432	2967	0.15%	0.013%
25	8.807	928	930	935	rBV5	2677	2807	0.14%	0.013%
26	8.913	945	948	950	rBV3	2163	2136	0.11%	0.010%
27	8.937	950	952	956	rVV4	1820	2362	0.12%	0.011%
28	8.984	959	960	965	rVB4	2155	2508	0.13%	0.011%
29	9.019	965	966	970	rBV4	1999	2577	0.13%	0.012%
30	9.131	978	985	994	rBV	365637	630046	31.73%	2.836%
31	9.272	1006	1009	1012	rBV4	2019	2705	0.14%	0.012%
32	9.443	1036	1038	1041	rVB4	2173	2211	0.11%	0.010%
33	9.472	1041	1043	1046	rBV4	1794	2124	0.11%	0.010%
34	9.854	1099	1108	1119	rBV	280364	480502	24.20%	2.163%
35	10.072	1140	1145	1147	rBV6	1661	2673	0.13%	0.012%
36	10.384	1190	1198	1208	rBV	455428	790756	39.83%	3.559%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033123.D
 Acq On : 17 Nov 2021 15:12
 Operator : CG/JU
 Sample : PB140812BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK812

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Title : SVOA CALIBRATION

37	10.631	1239	1240	1244	rBV3	2112	2051	0.10%	0.009%
38	10.772	1257	1264	1272	rBV	413272	717362	36.13%	3.228%
39	10.907	1279	1287	1298	rBV	453617	795976	40.09%	3.582%
40	11.796	1436	1438	1442	rBV5	1824	2506	0.13%	0.011%
41	12.119	1491	1493	1496	rBV4	1795	2482	0.13%	0.011%
42	12.225	1508	1511	1513	rBV4	1441	1996	0.10%	0.009%
43	12.354	1527	1533	1538	rBV3	9522	16038	0.81%	0.072%
44	12.413	1541	1543	1545	rVB3	2525	2388	0.12%	0.011%
45	12.443	1545	1548	1550	rBV4	2661	3819	0.19%	0.017%
46	12.501	1555	1558	1559	rVB2	2947	2149	0.11%	0.010%
47	12.590	1570	1573	1579	rBV5	1571	2925	0.15%	0.013%
48	12.819	1608	1612	1617	rVB5	3051	3843	0.19%	0.017%
49	12.954	1631	1635	1636	rVB4	2763	2757	0.14%	0.012%
50	13.043	1647	1650	1654	rVV5	1759	2755	0.14%	0.012%
51	13.195	1675	1676	1679	rBV3	3203	2848	0.14%	0.013%
52	13.231	1679	1682	1684	rBV4	1934	2354	0.12%	0.011%
53	13.342	1697	1701	1704	rVB6	1802	2740	0.14%	0.012%
54	13.407	1710	1712	1715	rVB4	2095	2130	0.11%	0.010%
55	13.566	1733	1739	1743	rBV7	2245	4048	0.20%	0.018%
56	13.860	1787	1789	1793	rBV2	1549	2103	0.11%	0.009%
57	14.001	1806	1813	1819	rBV	799080	1118428	56.33%	5.033%
58	14.042	1819	1820	1827	rVB5	2376	3201	0.16%	0.014%
59	14.289	1855	1862	1872	rVV	893210	1321347	66.55%	5.947%
60	14.360	1872	1874	1878	rVB4	1688	2488	0.13%	0.011%
61	14.531	1901	1903	1907	rBV4	1795	2416	0.12%	0.011%
62	14.595	1907	1914	1924	rVB	596355	933264	47.00%	4.200%
63	14.772	1937	1944	1956	rBV	351852	533869	26.89%	2.403%
64	15.013	1984	1985	1990	rVB5	1560	1999	0.10%	0.009%
65	15.584	2075	2082	2088	rBV	1098054	1592193	80.19%	7.166%
66	15.689	2093	2100	2108	rBV	260038	371073	18.69%	1.670%
67	15.825	2117	2123	2126	rVB8	6017	11044	0.56%	0.050%
68	16.354	2212	2213	2217	rBV4	2819	3731	0.19%	0.017%
69	16.460	2225	2231	2232	rBV5	3256	5518	0.28%	0.025%
70	16.707	2271	2273	2277	rBV5	1594	2002	0.10%	0.009%
71	16.789	2284	2287	2290	rBV5	1694	2441	0.12%	0.011%
72	16.948	2312	2314	2318	rVB5	2269	2766	0.14%	0.012%
73	17.330	2372	2379	2385	rBV	763982	1081759	54.48%	4.868%
74	17.425	2389	2395	2407	rVB	1152398	1720702	86.66%	7.744%
75	17.772	2452	2454	2456	rBV3	2185	2019	0.10%	0.009%
76	17.854	2467	2468	2471	rVB3	3105	2771	0.14%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033123.D
 Acq On : 17 Nov 2021 15:12
 Operator : CG/JU
 Sample : PB140812BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK812

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Title : SVOA CALIBRATION

77	17.936	2481	2482	2485	rBV3	3712	2957	0.15%	0.013%
78	17.995	2490	2492	2495	rVV4	4593	5164	0.26%	0.023%
79	18.101	2507	2510	2511	rBV3	2612	3116	0.16%	0.014%
80	18.213	2525	2529	2538	rBV10	20033	39137	1.97%	0.176%
81	19.272	2706	2709	2714	rVB5	15969	22923	1.15%	0.103%
82	19.342	2718	2721	2725	rVV2	13918	18803	0.95%	0.085%
83	19.483	2742	2745	2748	rBV4	13433	18903	0.95%	0.085%
84	19.707	2777	2783	2792	rBV	1457260	1985505	100.00%	8.936%
85	21.483	3080	3085	3092	rBV	881134	1149622	57.90%	5.174%
86	23.683	3453	3459	3471	rVB2	928710	1924520	96.93%	8.661%
87	23.830	3479	3484	3492	rVB2	560745	1108087	55.81%	4.987%




Sum of corrected areas: 22219700

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033123.D
Acq On : 17 Nov 2021 15:12
Operator : CG/JU
Sample : PB140812BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK812

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

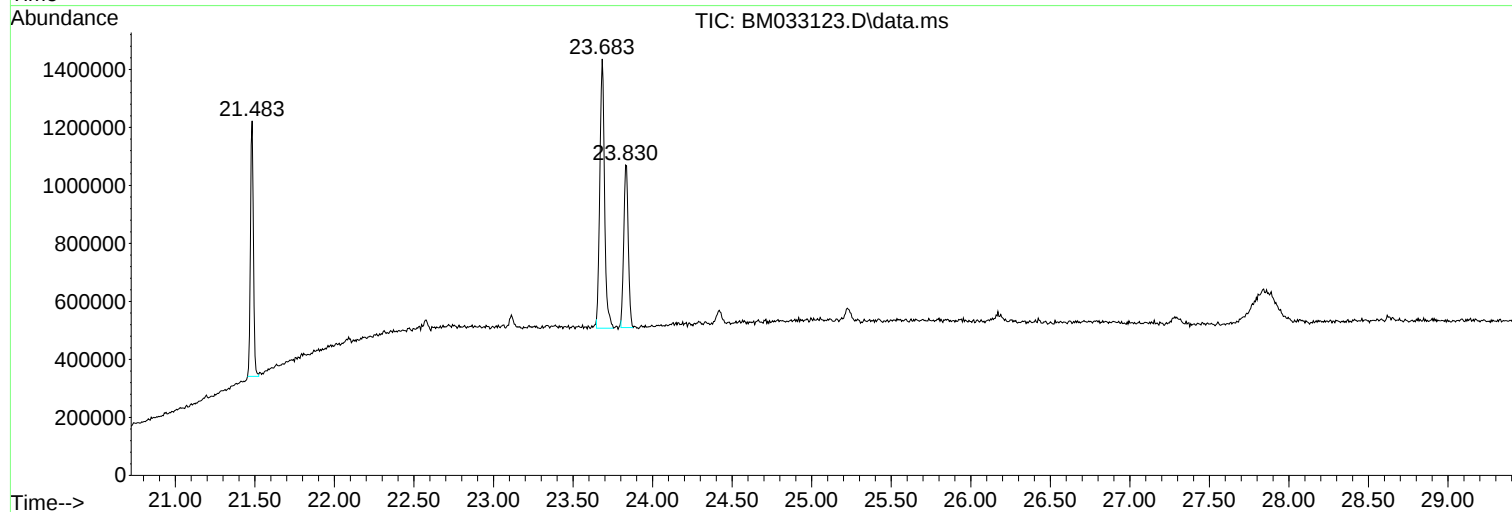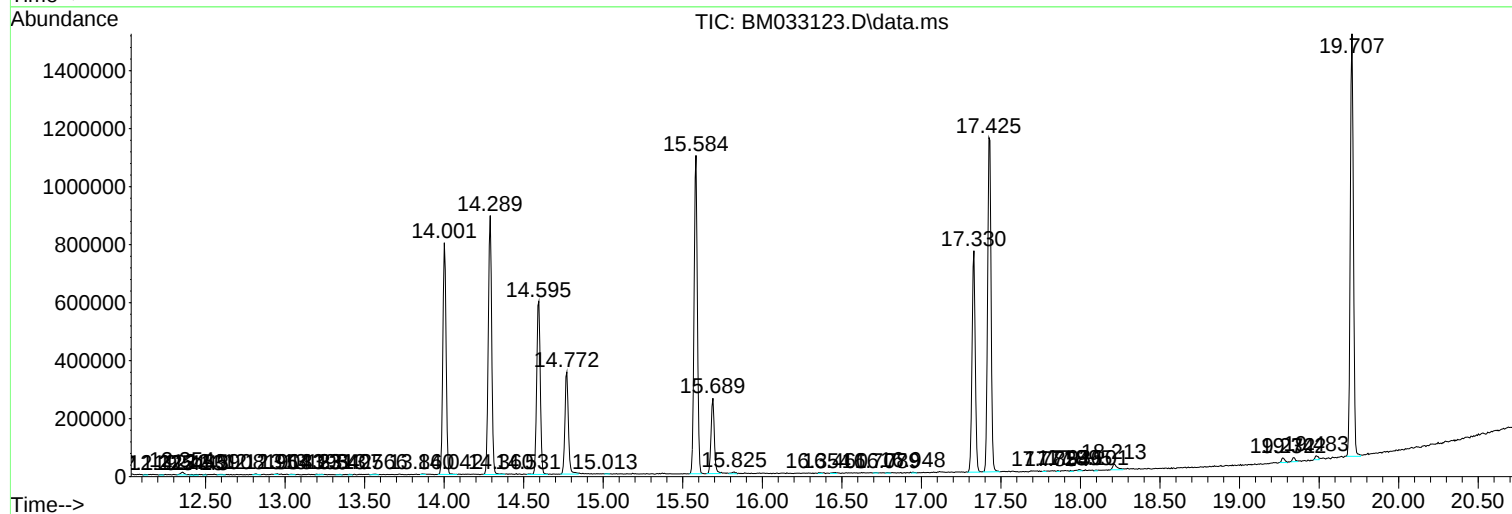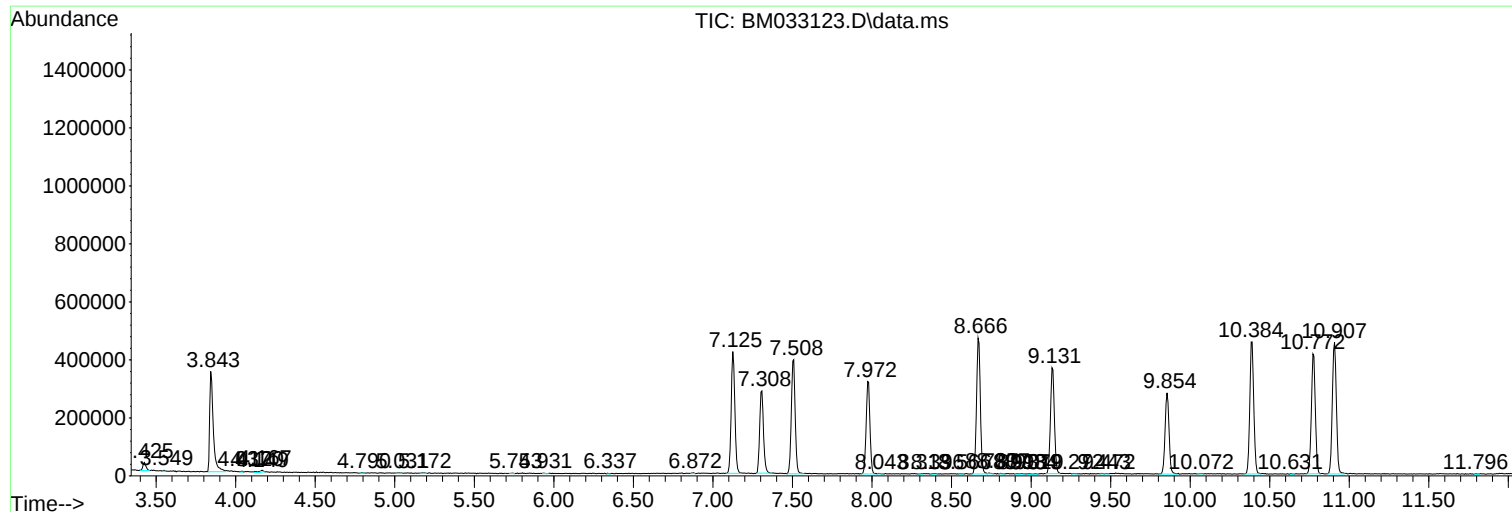

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033123.D
Acq On : 17 Nov 2021 15:12
Operator : CG/JU
Sample : PB140812BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK812

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033123.D
Acq On : 17 Nov 2021 15:12
Operator : CG/JU
Sample : PB140812BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK812

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc