

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033126.D
 Acq On : 17 Nov 2021 19:11
 Operator : CG/JU
 Sample : PB140762BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK762

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033126.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.425	11	15	21	rVB	26161	36087	1.78%	0.161%
2	3.843	82	86	98	rBV	314944	492363	24.35%	2.195%
3	4.160	137	140	145	rVB3	5680	9064	0.45%	0.040%
4	4.460	187	191	195	rVB6	1494	2265	0.11%	0.010%
5	4.684	227	229	235	rVB6	1894	3429	0.17%	0.015%
6	4.731	235	237	239	rBV3	1970	2393	0.12%	0.011%
7	5.025	283	287	290	rBV5	1911	2589	0.13%	0.012%
8	5.184	312	314	319	rVB5	2526	3619	0.18%	0.016%
9	5.301	331	334	335	rBV3	2561	2391	0.12%	0.011%
10	5.390	346	349	351	rBV2	2207	2135	0.11%	0.010%
11	7.125	638	644	653	rVV	396238	623872	30.86%	2.781%
12	7.301	668	674	685	rBV	264622	447079	22.11%	1.993%
13	7.507	700	709	716	rBV	366251	615581	30.45%	2.744%
14	7.637	727	731	732	rBV3	1830	2339	0.12%	0.010%
15	7.825	760	763	765	rBV4	2027	2217	0.11%	0.010%
16	7.972	781	788	796	rVB	343807	557453	27.57%	2.485%
17	8.136	813	816	819	rVB4	1862	2185	0.11%	0.010%
18	8.207	825	828	833	rVB5	2380	4398	0.22%	0.020%
19	8.254	833	836	839	rBV4	1948	2999	0.15%	0.013%
20	8.666	899	906	917	rVB	455113	738988	36.55%	3.294%
21	9.131	978	985	993	rBV	348364	597579	29.55%	2.664%
22	9.495	1041	1047	1049	rBV7	2615	4882	0.24%	0.022%
23	9.595	1063	1064	1069	rVB4	1423	2027	0.10%	0.009%
24	9.854	1101	1108	1117	rVB	266156	451443	22.33%	2.012%
25	10.307	1182	1185	1188	rVB5	1814	2590	0.13%	0.012%
26	10.383	1191	1198	1209	rVB	437563	753232	37.25%	3.357%
27	10.772	1255	1264	1272	rBV	446396	765570	37.86%	3.412%
28	10.848	1274	1277	1279	rBV4	1430	2034	0.10%	0.009%
29	10.907	1279	1287	1301	rVB	432369	768881	38.03%	3.427%
30	11.477	1379	1384	1387	rVB6	1639	2668	0.13%	0.012%
31	11.813	1439	1441	1446	rBV4	1604	2410	0.12%	0.011%
32	11.954	1460	1465	1466	rBV3	1729	2161	0.11%	0.010%
33	12.007	1472	1474	1477	rBV4	1910	2283	0.11%	0.010%
34	12.030	1477	1478	1482	rVB3	2715	2876	0.14%	0.013%
35	12.348	1526	1532	1537	rBV4	9707	15206	0.75%	0.068%
36	12.554	1564	1567	1572	rBV5	1780	3073	0.15%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033126.D
 Acq On : 17 Nov 2021 19:11
 Operator : CG/JU
 Sample : PB140762BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK762

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Title : SVOA CALIBRATION

37	12.877	1620	1622	1625	rBV2	1829	2297	0.11%	0.010%
38	12.948	1629	1634	1638	rVV6	2320	4241	0.21%	0.019%
39	13.089	1655	1658	1661	rBV5	2234	2685	0.13%	0.012%
40	13.389	1706	1709	1713	rVB4	1734	2898	0.14%	0.013%
41	13.424	1713	1715	1717	rBV3	2012	2064	0.10%	0.009%
42	13.860	1786	1789	1792	rVV4	2217	3015	0.15%	0.013%
43	13.895	1792	1795	1798	rVB5	1867	2228	0.11%	0.010%
44	14.001	1807	1813	1822	rBV	810835	1133963	56.08%	5.055%
45	14.236	1849	1853	1855	rBV5	1196	2109	0.10%	0.009%
46	14.289	1855	1862	1870	rVV	856231	1271470	62.88%	5.667%
47	14.448	1887	1889	1895	rBV6	2252	3794	0.19%	0.017%
48	14.507	1897	1899	1901	rBV2	1739	2122	0.10%	0.009%
49	14.595	1907	1914	1923	rBV	666298	1018764	50.39%	4.541%
50	14.771	1937	1944	1957	rBV	347168	542887	26.85%	2.420%
51	14.901	1963	1966	1968	rVB4	2322	2062	0.10%	0.009%
52	14.948	1973	1974	1979	rVB5	2810	2806	0.14%	0.013%
53	15.001	1979	1983	1990	rBV8	2616	6548	0.32%	0.029%
54	15.077	1994	1996	1999	rBV4	2351	2495	0.12%	0.011%
55	15.371	2042	2046	2049	rBV4	2951	5048	0.25%	0.023%
56	15.577	2074	2081	2090	rBV	1069044	1582826	78.28%	7.055%
57	15.689	2093	2100	2110	rBV	277075	407736	20.17%	1.817%
58	15.818	2118	2122	2131	rVB9	5452	10574	0.52%	0.047%
59	16.083	2163	2167	2168	rBV4	1498	2067	0.10%	0.009%
60	16.448	2226	2229	2231	rVB3	3861	3888	0.19%	0.017%
61	16.512	2238	2240	2244	rBV5	1290	2084	0.10%	0.009%
62	16.589	2251	2253	2256	rBV3	1727	2095	0.10%	0.009%
63	16.954	2311	2315	2316	rBV3	1509	2065	0.10%	0.009%
64	17.118	2338	2343	2346	rBV6	3572	6683	0.33%	0.030%
65	17.189	2353	2355	2359	rVB4	3149	2487	0.12%	0.011%
66	17.324	2372	2378	2387	rVB	813981	1177047	58.21%	5.247%
67	17.424	2389	2395	2403	rBV	1244253	1751695	86.64%	7.808%
68	17.995	2488	2492	2495	rVB6	6073	9710	0.48%	0.043%
69	18.212	2524	2529	2538	rBV7	18007	38352	1.90%	0.171%
70	19.342	2718	2721	2728	rVB2	14893	18079	0.89%	0.081%
71	19.483	2742	2745	2747	rBV4	11186	15182	0.75%	0.068%
72	19.706	2777	2783	2789	rBV	1447155	2016520	99.73%	8.988%
73	21.483	3080	3085	3090	rBV	912115	1227882	60.73%	5.473%
74	23.677	3452	3458	3471	rVB	951206	2021925	100.00%	9.013%
75	23.830	3478	3484	3494	rVB2	608557	1189843	58.85%	5.304%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033126.D
Acq On : 17 Nov 2021 19:11
Operator : CG/JU
Sample : PB140762BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK762

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Title : SVOA CALIBRATION




Sum of corrected areas: 22434597

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033126.D
Acq On : 17 Nov 2021 19:11
Operator : CG/JU
Sample : PB140762BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK762

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

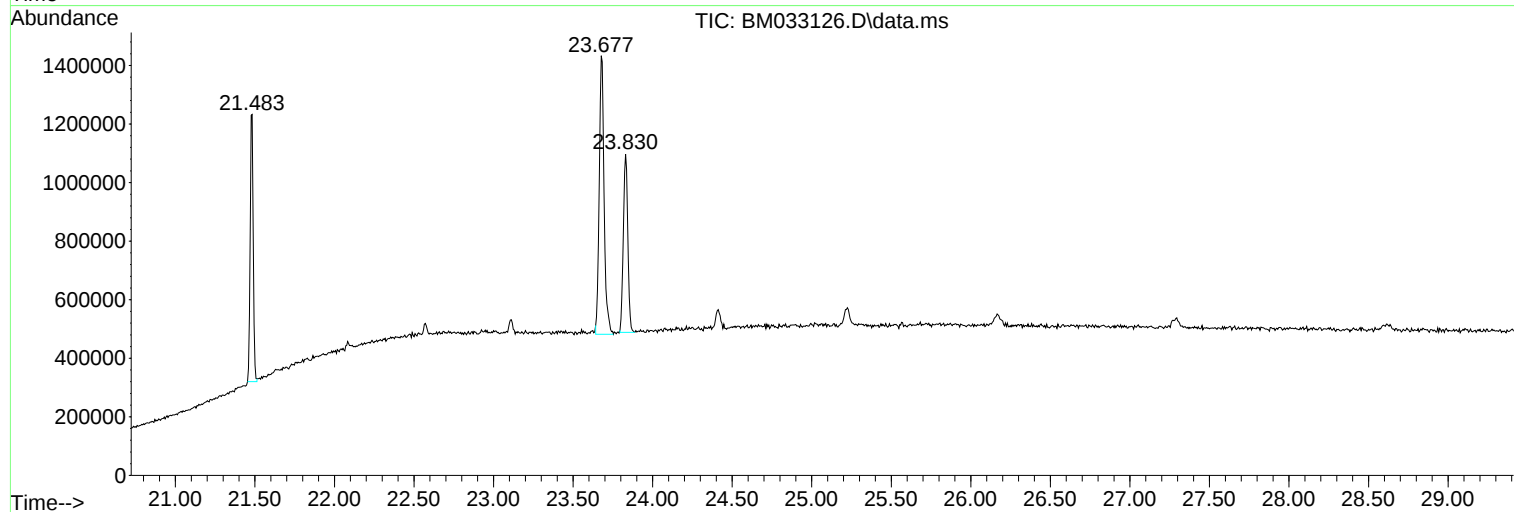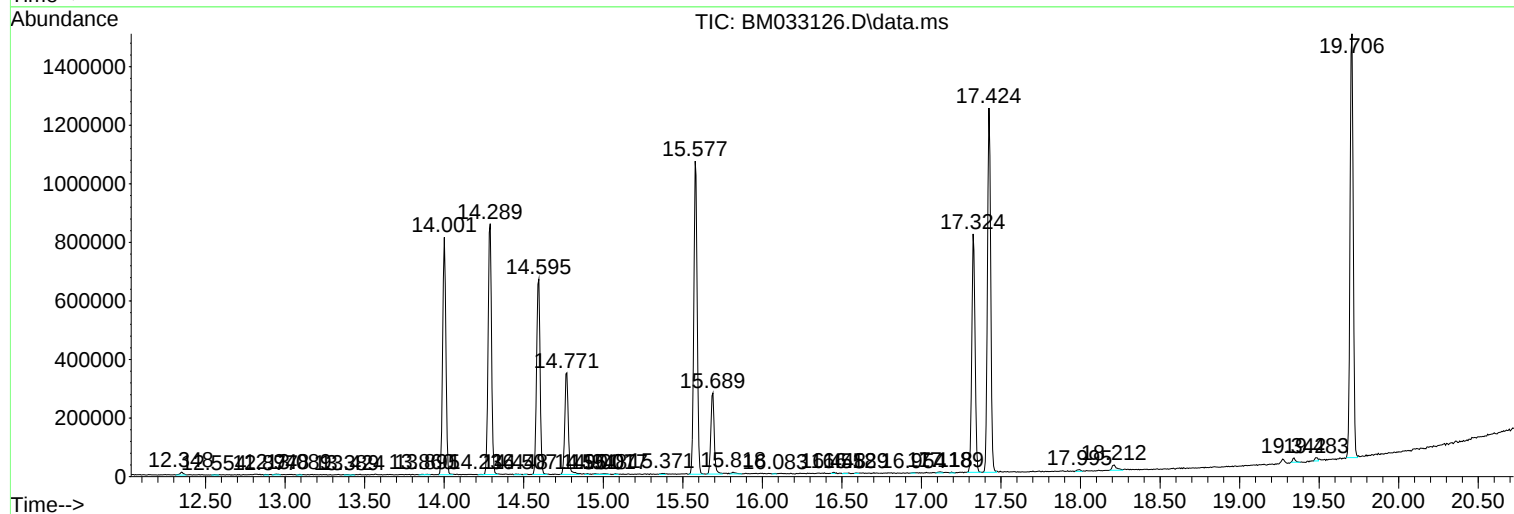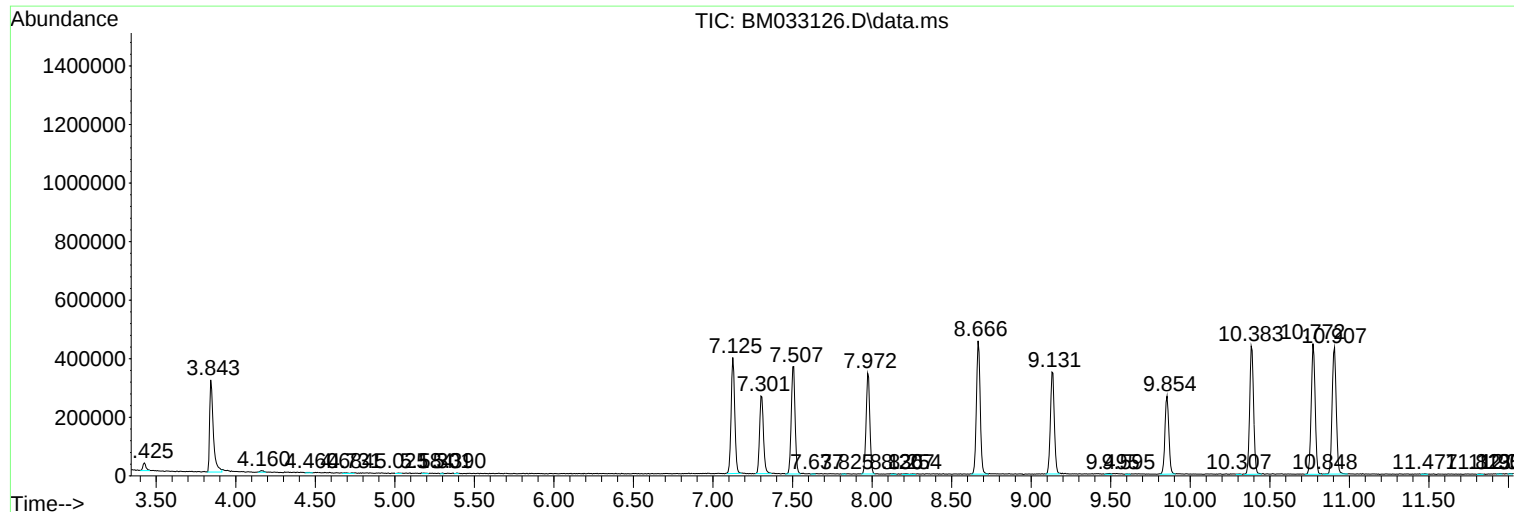

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033126.D
Acq On : 17 Nov 2021 19:11
Operator : CG/JU
Sample : PB140762BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK762

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033126.D
Acq On : 17 Nov 2021 19:11
Operator : CG/JU
Sample : PB140762BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK762

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc