

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033127.D
 Acq On : 17 Nov 2021 19:47
 Operator : CG/JU
 Sample : PB140791BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK791

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033127.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.425	11	15	20	rVB	25237	32597	1.68%	0.158%
2	3.843	82	86	98	rBV	325381	498092	25.68%	2.416%
3	4.160	136	140	144	rBV4	5992	8808	0.45%	0.043%
4	4.231	148	152	154	rBV4	2135	3013	0.16%	0.015%
5	4.619	216	218	221	rVB3	2131	2283	0.12%	0.011%
6	4.678	225	228	231	rVB3	1769	2310	0.12%	0.011%
7	5.007	281	284	287	rVV4	1939	2367	0.12%	0.011%
8	5.278	328	330	333	rBV3	1973	1981	0.10%	0.010%
9	5.725	404	406	408	rBV2	2110	2002	0.10%	0.010%
10	5.837	422	425	428	rBV5	1780	2110	0.11%	0.010%
11	6.484	531	535	539	rBV6	1966	3161	0.16%	0.015%
12	7.125	638	644	652	rBV	397373	618763	31.90%	3.002%
13	7.301	667	674	685	rBV	258925	439014	22.63%	2.130%
14	7.501	702	708	716	rBV	372234	612793	31.59%	2.973%
15	7.666	733	736	737	rBV3	2233	2078	0.11%	0.010%
16	7.972	781	788	797	rVB	281692	466952	24.07%	2.265%
17	8.554	884	887	890	rVV4	1343	1978	0.10%	0.010%
18	8.666	899	906	915	rBV	439494	716710	36.95%	3.477%
19	8.831	933	934	936	rVB2	3182	2027	0.10%	0.010%
20	8.854	936	938	942	rBV4	2788	4711	0.24%	0.023%
21	8.884	942	943	947	rBV3	1514	2086	0.11%	0.010%
22	9.048	970	971	976	rVB3	1532	2133	0.11%	0.010%
23	9.131	976	985	994	rBV	336201	588162	30.32%	2.853%
24	9.854	1100	1108	1119	rBV	261961	447107	23.05%	2.169%
25	10.384	1192	1198	1209	rBV	427927	724262	37.34%	3.514%
26	10.772	1257	1264	1271	rBV	366544	621203	32.02%	3.014%
27	10.901	1280	1286	1300	rVB	415747	740512	38.18%	3.593%
28	11.336	1356	1360	1362	rBV4	1557	2047	0.11%	0.010%
29	11.425	1372	1375	1377	rBV3	1797	2234	0.12%	0.011%
30	11.519	1387	1391	1392	rBV5	1598	2143	0.11%	0.010%
31	12.348	1527	1532	1538	rVB4	8717	15081	0.78%	0.073%
32	12.730	1593	1597	1600	rBV3	2008	3365	0.17%	0.016%
33	12.819	1606	1612	1615	rBV5	2842	3710	0.19%	0.018%
34	12.948	1631	1634	1638	rBV4	2437	3596	0.19%	0.017%
35	13.730	1764	1767	1770	rBV5	2355	2651	0.14%	0.013%
36	14.001	1806	1813	1821	rBV	769247	1059369	54.61%	5.139%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033127.D
 Acq On : 17 Nov 2021 19:47
 Operator : CG/JU
 Sample : PB140791BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK791

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Title : SVOA CALIBRATION

37	14.289	1854	1862	1873	rBV	778464	1194979	61.60%	5.797%
38	14.589	1907	1913	1920	rBV	531886	798660	41.17%	3.875%
39	14.701	1927	1932	1933	rVB5	1444	2045	0.11%	0.010%
40	14.766	1936	1943	1955	rBV	337218	523003	26.96%	2.537%
41	15.195	2013	2016	2017	rBV3	2242	1973	0.10%	0.010%
42	15.219	2017	2020	2024	rVV5	1674	2234	0.12%	0.011%
43	15.371	2043	2046	2049	rBV5	3510	4434	0.23%	0.022%
44	15.583	2075	2082	2089	rVB	988855	1485472	76.58%	7.207%
45	15.683	2092	2099	2112	rBV	255303	387181	19.96%	1.878%
46	15.818	2119	2122	2125	rVB4	3493	3115	0.16%	0.015%
47	16.042	2156	2160	2162	rVB4	2132	2903	0.15%	0.014%
48	16.113	2167	2172	2173	rBV3	1968	2616	0.13%	0.013%
49	16.354	2210	2213	2215	rBV4	2217	2917	0.15%	0.014%
50	16.448	2226	2229	2233	rBV6	4413	5324	0.27%	0.026%
51	16.536	2239	2244	2245	rBV4	1311	2179	0.11%	0.011%
52	16.942	2310	2313	2315	rBV5	2207	2328	0.12%	0.011%
53	17.042	2328	2330	2333	rVB4	1987	2139	0.11%	0.010%
54	17.118	2339	2343	2345	rBV5	2859	3110	0.16%	0.015%
55	17.248	2362	2365	2368	rBV5	2539	3577	0.18%	0.017%
56	17.324	2372	2378	2385	rVV	639659	930232	47.96%	4.513%
57	17.424	2388	2395	2407	rVV	1182521	1664598	85.81%	8.076%
58	17.695	2439	2441	2446	rBV5	2217	2613	0.13%	0.013%
59	17.877	2470	2472	2475	rVB4	3759	3092	0.16%	0.015%
60	17.995	2490	2492	2494	rVB3	3486	2093	0.11%	0.010%
61	18.207	2524	2528	2541	rBV8	19686	37757	1.95%	0.183%
62	19.265	2706	2708	2713	rVB5	11395	16423	0.85%	0.080%
63	19.342	2717	2721	2725	rVV2	12957	18527	0.96%	0.090%
64	19.477	2742	2744	2749	rBV6	13549	19572	1.01%	0.095%
65	19.706	2777	2783	2789	rBV	1391094	1939778	100.00%	9.411%
66	21.477	3080	3084	3091	rBV	746814	1000600	51.58%	4.854%
67	23.677	3452	3458	3470	rVB	974241	1934741	99.74%	9.386%
68	23.830	3479	3484	3492	rVB	515346	968753	49.94%	4.700%




Sum of corrected areas: 20612379

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033127.D
Acq On : 17 Nov 2021 19:47
Operator : CG/JU
Sample : PB140791BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK791

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

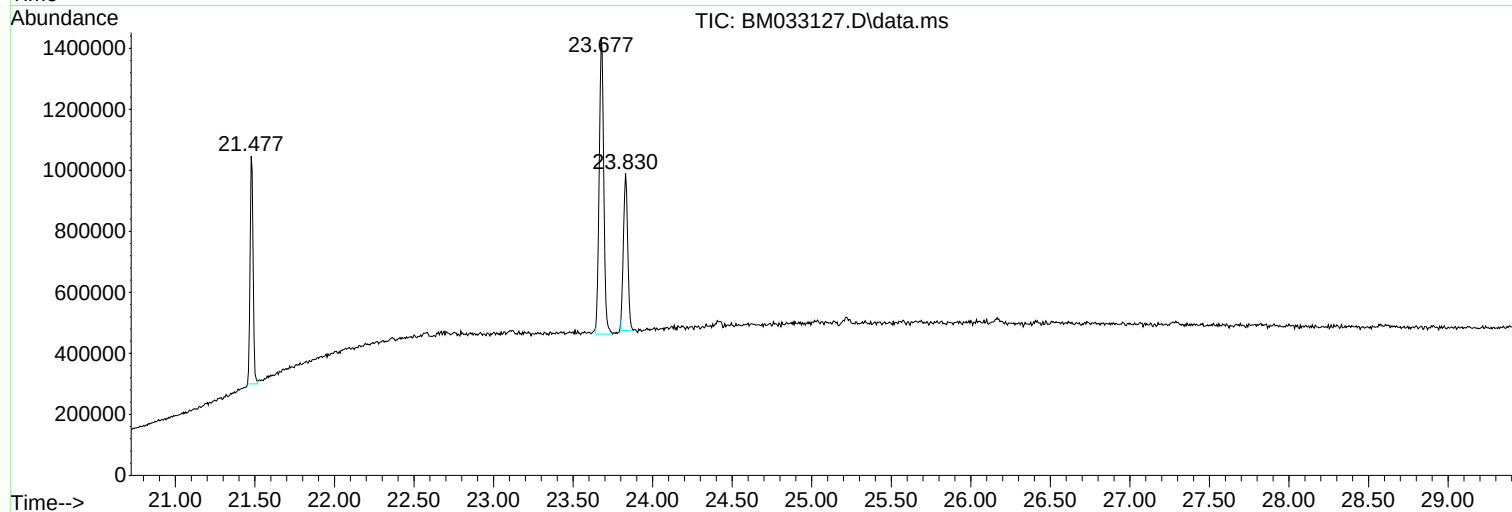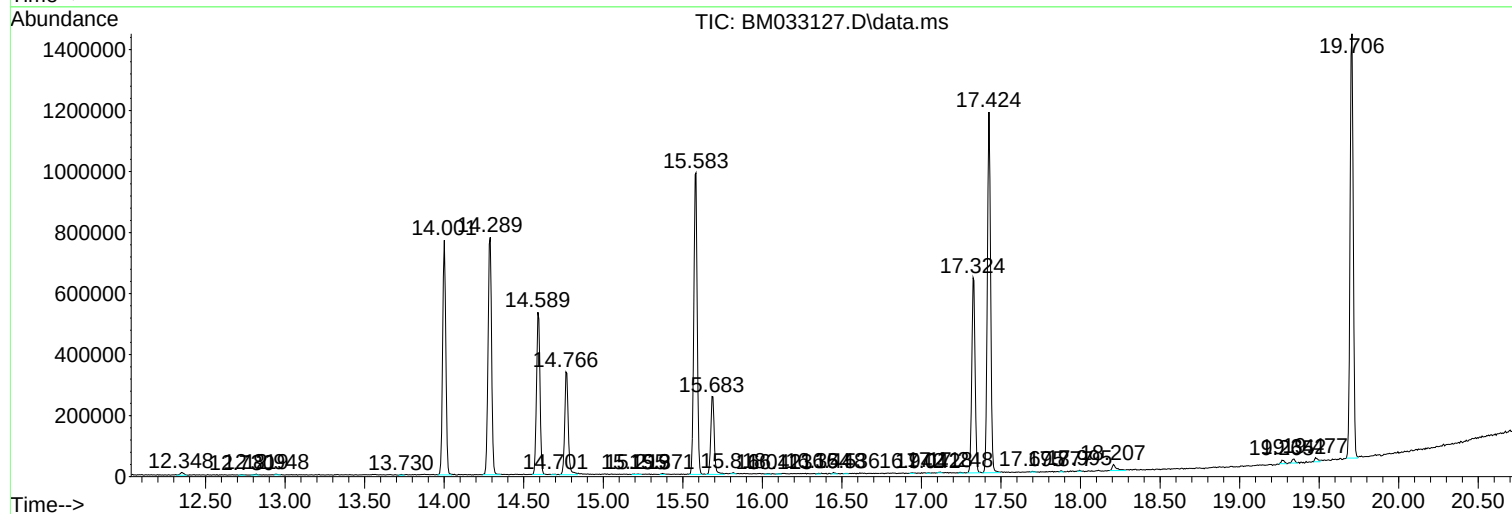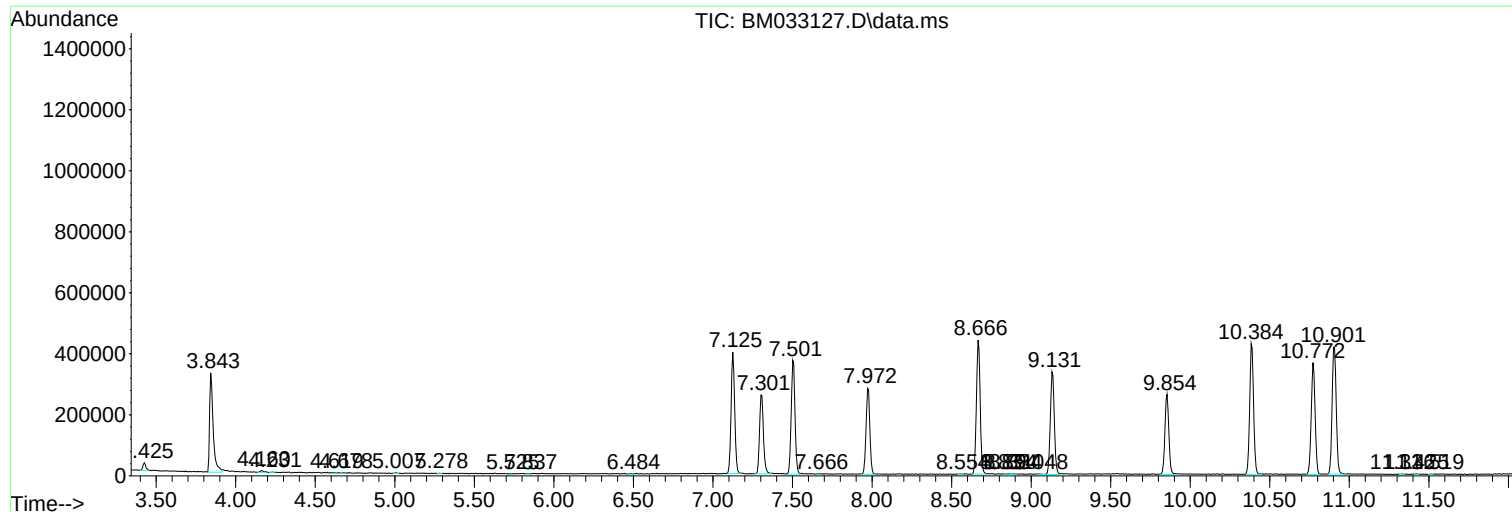

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033127.D
Acq On : 17 Nov 2021 19:47
Operator : CG/JU
Sample : PB140791BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK791

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033127.D
Acq On : 17 Nov 2021 19:47
Operator : CG/JU
Sample : PB140791BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK791

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc