

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033133.D
 Acq On : 17 Nov 2021 23:24
 Operator : CG/JU
 Sample : M4618-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG1Z3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033133.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.390	4	9	13	rBV	70448	106471	4.23%	0.427%
2	3.426	13	15	23	rVB	24251	30102	1.20%	0.121%
3	3.849	83	87	99	rBV	80567	138867	5.52%	0.557%
4	4.073	120	125	129	rVB2	10571	17166	0.68%	0.069%
5	4.161	137	140	146	rVB3	9420	11760	0.47%	0.047%
6	4.484	193	195	199	rVB3	2246	2699	0.11%	0.011%
7	4.690	225	230	239	rVB	42067	67012	2.66%	0.269%
8	5.096	297	299	305	rVB5	3360	4732	0.19%	0.019%
9	6.084	464	467	469	rBV3	2346	2631	0.10%	0.011%
10	6.819	590	592	595	rBV4	2441	2944	0.12%	0.012%
11	7.125	636	644	652	rBV	103818	179640	7.14%	0.720%
12	7.302	666	674	690	rBV	318062	515064	20.47%	2.065%
13	7.502	698	708	717	rBV	334361	545868	21.70%	2.189%
14	7.584	719	722	726	rVB4	2157	3302	0.13%	0.013%
15	7.972	782	788	795	rBV	424514	674026	26.79%	2.703%
16	8.366	850	855	856	rBV5	1832	2593	0.10%	0.010%
17	8.666	900	906	914	rBV2	267610	438422	17.43%	1.758%
18	9.131	978	985	993	rBV	403416	670548	26.65%	2.689%
19	9.531	1048	1053	1060	rBV6	3946	8631	0.34%	0.035%
20	9.849	1100	1107	1116	rVB	292936	498574	19.82%	1.999%
21	10.072	1141	1145	1147	rBV3	2138	2610	0.10%	0.010%
22	10.384	1191	1198	1207	rBV	469358	781966	31.08%	3.135%
23	10.555	1221	1227	1236	rBV3	12166	23898	0.95%	0.096%
24	10.772	1257	1264	1273	rBV	540659	933985	37.12%	3.745%
25	10.902	1279	1286	1298	rBV	416487	723148	28.74%	2.900%
26	11.496	1382	1387	1389	rBV5	1545	2701	0.11%	0.011%
27	11.543	1392	1395	1399	rVB4	2706	4037	0.16%	0.016%
28	12.019	1474	1476	1480	rVB3	2725	3391	0.13%	0.014%
29	12.260	1514	1517	1521	rBV6	2465	3600	0.14%	0.014%
30	12.349	1528	1532	1541	rVB2	10367	16589	0.66%	0.067%
31	13.207	1675	1678	1684	rVV7	1909	3784	0.15%	0.015%
32	13.413	1710	1713	1718	rVB3	4171	4641	0.18%	0.019%
33	13.484	1722	1725	1729	rVB5	1824	2759	0.11%	0.011%
34	13.554	1732	1737	1741	rVV6	6992	10943	0.43%	0.044%
35	13.860	1785	1789	1791	rBV4	3363	4457	0.18%	0.018%
36	13.995	1805	1812	1821	rBV	902460	1288273	51.20%	5.165%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033133.D
 Acq On : 17 Nov 2021 23:24
 Operator : CG/JU
 Sample : M4618-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG1Z3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Title : SVOA CALIBRATION

37	14.072	1821	1825	1828	rVB5	2142	3743	0.15%	0.015%
38	14.231	1846	1852	1855	rBV6	2698	4485	0.18%	0.018%
39	14.284	1855	1861	1872	rVV	1003747	1450420	57.65%	5.816%
40	14.478	1892	1894	1901	rVB6	2375	3181	0.13%	0.013%
41	14.537	1901	1904	1906	rBV4	2518	2910	0.12%	0.012%
42	14.590	1906	1913	1920	rVV	811629	1222563	48.59%	4.902%
43	14.766	1937	1943	1949	rBV	86038	132007	5.25%	0.529%
44	14.995	1979	1982	1986	rVB4	3306	4038	0.16%	0.016%
45	15.095	1997	1999	2002	rBV2	2656	2572	0.10%	0.010%
46	15.378	2041	2047	2051	rVV9	2778	4894	0.19%	0.020%
47	15.578	2073	2081	2092	rVB	1280397	1859313	73.90%	7.455%
48	15.684	2092	2099	2107	rBV	351846	500785	19.90%	2.008%
49	15.825	2118	2123	2126	rBV5	6891	10470	0.42%	0.042%
50	15.978	2145	2149	2150	rBV4	2869	3857	0.15%	0.015%
51	15.995	2150	2152	2155	rVB4	3024	3463	0.14%	0.014%
52	16.248	2192	2195	2196	rBV3	3397	3094	0.12%	0.012%
53	16.313	2200	2206	2210	rVB5	8952	14308	0.57%	0.057%
54	16.448	2225	2229	2231	rBV4	3762	5704	0.23%	0.023%
55	16.625	2256	2259	2263	rVB6	2780	4256	0.17%	0.017%
56	17.013	2321	2325	2327	rBV5	3330	5206	0.21%	0.021%
57	17.131	2338	2345	2349	rBV6	10665	20804	0.83%	0.083%
58	17.231	2358	2362	2363	rBV4	2685	2972	0.12%	0.012%
59	17.325	2372	2378	2387	rVV	984281	1440569	57.26%	5.776%
60	17.425	2388	2395	2405	rVV	1456594	2154621	85.64%	8.639%
61	17.507	2406	2409	2412	rVV4	15254	20637	0.82%	0.083%
62	17.542	2412	2415	2424	rVB	12310	20493	0.81%	0.082%
63	17.989	2487	2491	2496	rVB8	9541	12705	0.50%	0.051%
64	18.207	2523	2528	2533	rBV	85840	126053	5.01%	0.505%
65	18.501	2576	2578	2580	rBV3	4152	3191	0.13%	0.013%
66	19.272	2705	2709	2714	rBV5	21256	30613	1.22%	0.123%
67	19.342	2717	2721	2727	rBV	20927	30463	1.21%	0.122%
68	19.419	2730	2734	2740	rBV	65832	79863	3.17%	0.320%
69	19.477	2740	2744	2749	rBV3	61551	87400	3.47%	0.350%
70	19.701	2776	2782	2791	rBV	1897726	2505986	99.60%	10.048%
71	21.477	3079	3084	3090	rBV	1205643	1482688	58.93%	5.945%
72	23.671	3451	3457	3469	rVB2	1205436	2516011	100.00%	10.088%
73	23.824	3477	3483	3491	rVB2	753513	1431986	56.91%	5.742%




Sum of corrected areas: 24940158

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033133.D
Acq On : 17 Nov 2021 23:24
Operator : CG/JU
Sample : M4618-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG1Z3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

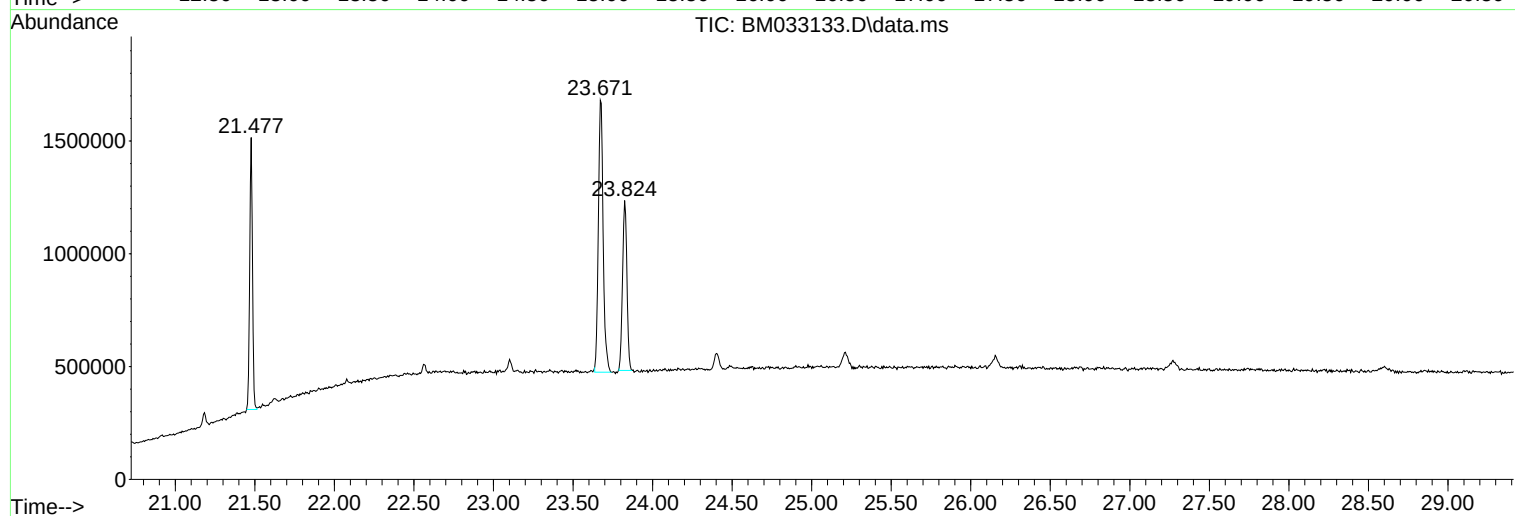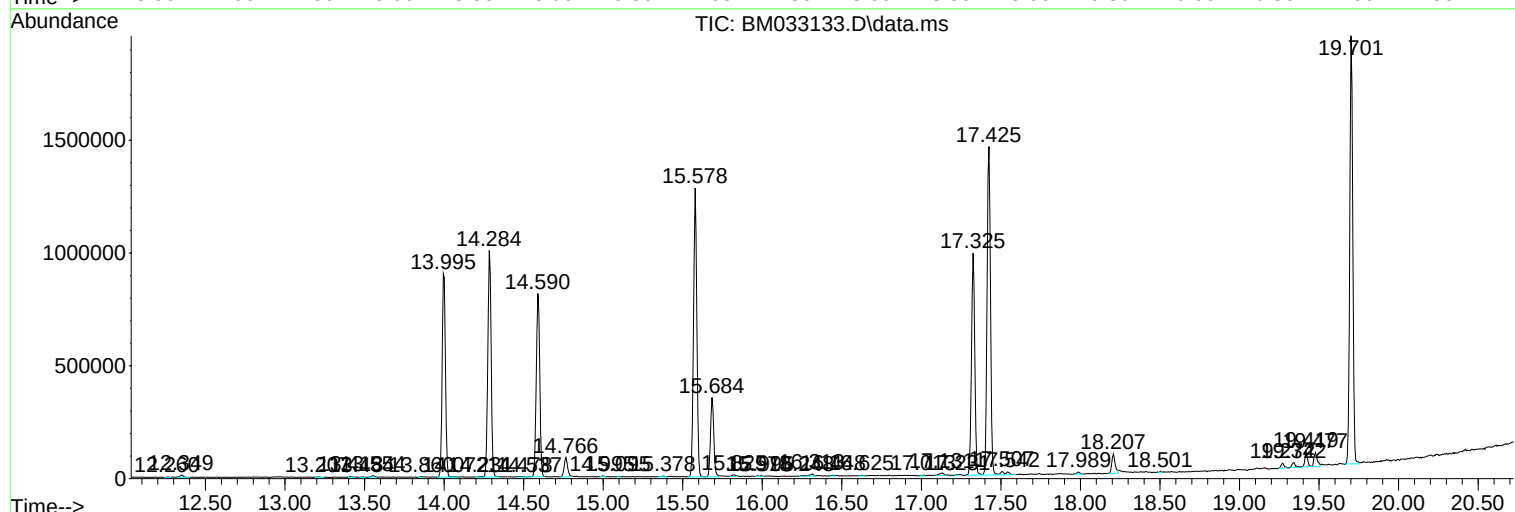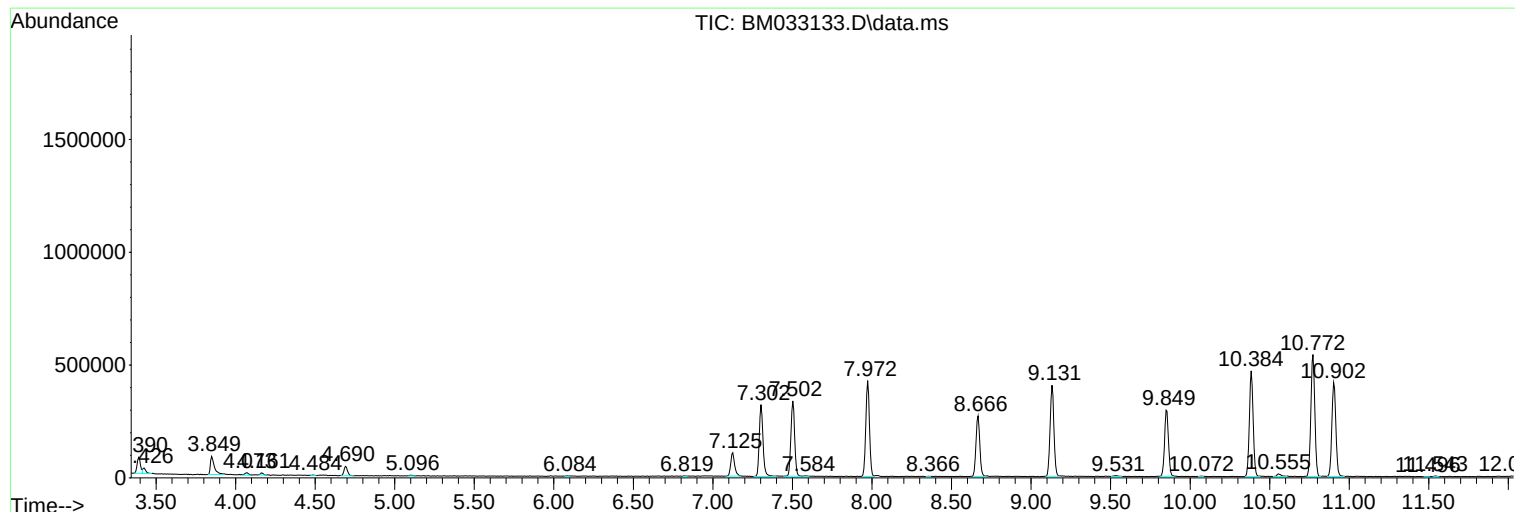

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033133.D
Acq On : 17 Nov 2021 23:24
Operator : CG/JU
Sample : M4618-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG1Z3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033133.D
Acq On : 17 Nov 2021 23:24
Operator : CG/JU
Sample : M4618-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG1Z3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc