

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033143.D
 Acq On : 18 Nov 2021 05:58
 Operator : CG/JU
 Sample : PB140810BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK810

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033143.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.420	10	14	21	rVB	40201	53105	1.93%	0.166%
2	3.802	76	79	82	rBV5	2352	3370	0.12%	0.011%
3	3.837	82	85	102	rBV	497293	773273	28.11%	2.416%
4	4.167	135	141	147	rBV3	7488	13980	0.51%	0.044%
5	5.384	346	348	354	rVB6	1787	3110	0.11%	0.010%
6	5.649	389	393	394	rBV4	2275	2998	0.11%	0.009%
7	6.396	516	520	523	rVB5	1659	2797	0.10%	0.009%
8	6.443	523	528	530	rBV7	2054	2793	0.10%	0.009%
9	7.119	634	643	652	rBV	586779	964126	35.05%	3.013%
10	7.302	666	674	688	rBV	422576	707151	25.71%	2.210%
11	7.502	700	708	716	rBV	574743	936088	34.03%	2.925%
12	7.972	780	788	798	rVB	447457	737323	26.81%	2.304%
13	8.660	898	905	916	rBV	694734	1154186	41.96%	3.606%
14	9.131	977	985	993	rBV	553813	946314	34.40%	2.957%
15	9.849	1098	1107	1118	rBV	461212	751055	27.30%	2.347%
16	10.378	1191	1197	1207	rBV	684190	1189786	43.25%	3.718%
17	10.766	1256	1263	1271	rBV	610767	1044401	37.97%	3.263%
18	10.901	1278	1286	1298	rBV	696262	1206678	43.87%	3.770%
19	12.019	1474	1476	1480	rVB5	2433	3044	0.11%	0.010%
20	12.348	1526	1532	1537	rVB2	14401	25258	0.92%	0.079%
21	12.807	1606	1610	1615	rVB5	1968	2787	0.10%	0.009%
22	13.213	1676	1679	1683	rVB6	2067	3320	0.12%	0.010%
23	13.560	1737	1738	1742	rVB4	3456	2807	0.10%	0.009%
24	13.725	1762	1766	1767	rBV3	2113	3008	0.11%	0.009%
25	13.995	1805	1812	1821	rBV	1250155	1708185	62.10%	5.337%
26	14.284	1854	1861	1868	rBV	1354231	2022772	73.54%	6.320%
27	14.589	1906	1913	1919	rBV	912987	1396584	50.77%	4.364%
28	14.766	1936	1943	1957	rBV	547033	796663	28.96%	2.489%
29	15.001	1980	1983	1986	rBV5	2408	3077	0.11%	0.010%
30	15.578	2074	2081	2089	rBV	1687445	2453578	89.20%	7.666%
31	15.683	2093	2099	2109	rBV	453282	636753	23.15%	1.990%
32	15.813	2118	2121	2126	rVB4	6379	8189	0.30%	0.026%
33	16.442	2226	2228	2231	rVV4	2742	3247	0.12%	0.010%
34	16.495	2234	2237	2239	rBV4	2449	3133	0.11%	0.010%
35	16.730	2275	2277	2281	rBV5	2470	3433	0.12%	0.011%
36	17.119	2339	2343	2345	rVB3	4292	5706	0.21%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033143.D
 Acq On : 18 Nov 2021 05:58
 Operator : CG/JU
 Sample : PB140810BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK810

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Title : SVOA CALIBRATION

37	17.325	2371	2378	2384	rBV	1039445	1558808	56.67%	4.871%
38	17.419	2388	2394	2406	rVV	1698762	2524678	91.78%	7.889%
39	17.566	2416	2419	2420	rBV4	3255	2769	0.10%	0.009%
40	17.695	2438	2441	2443	rBV3	3298	4404	0.16%	0.014%
41	17.877	2468	2472	2476	rBV6	2343	3781	0.14%	0.012%
42	17.977	2486	2489	2495	rVB6	5312	8504	0.31%	0.027%
43	18.201	2523	2527	2533	rBV7	13710	21116	0.77%	0.066%
44	19.271	2704	2709	2712	rBV4	21518	32807	1.19%	0.103%
45	19.336	2717	2720	2726	rVB	22664	29687	1.08%	0.093%
46	19.471	2741	2743	2747	rBV5	8481	9101	0.33%	0.028%
47	19.701	2776	2782	2789	rBV	2007056	2750660	100.00%	8.595%
48	21.477	3079	3084	3089	rBV	1136751	1484811	53.98%	4.639%
49	23.671	3451	3457	3467	rVB	1238308	2571029	93.47%	8.033%
50	23.818	3477	3482	3493	rVB2	697288	1427899	51.91%	4.462%




Sum of corrected areas: 32004132

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033143.D
Acq On : 18 Nov 2021 05:58
Operator : CG/JU
Sample : PB140810BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK810

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

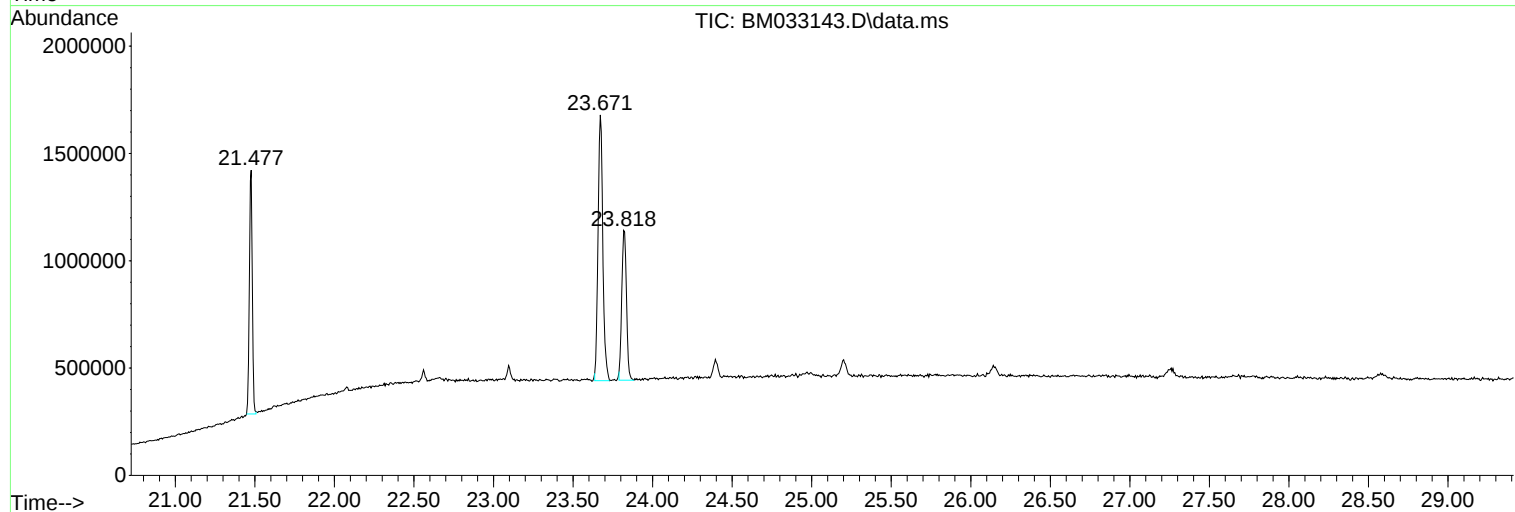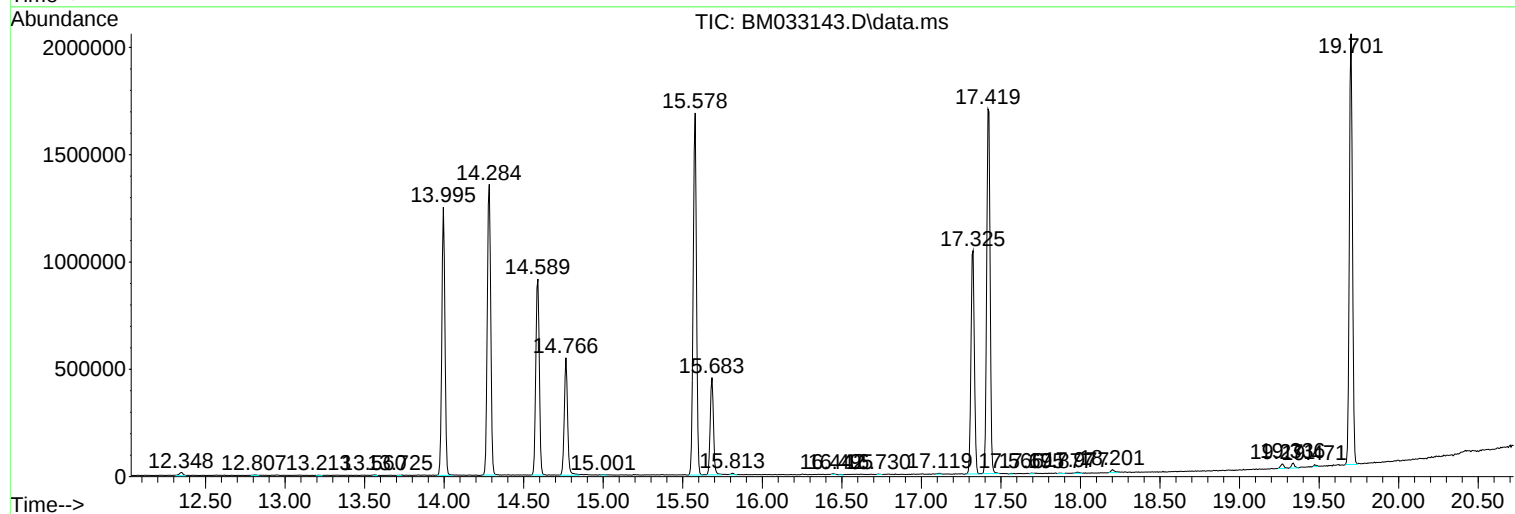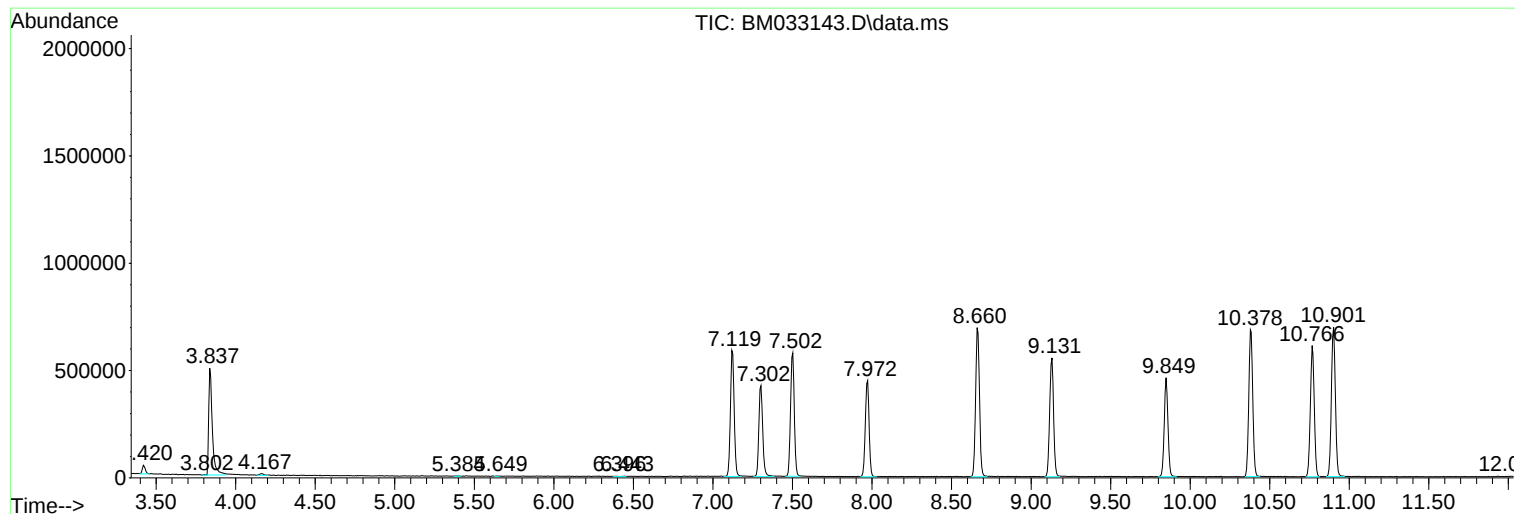

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033143.D
Acq On : 18 Nov 2021 05:58
Operator : CG/JU
Sample : PB140810BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK810

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033143.D
Acq On : 18 Nov 2021 05:58
Operator : CG/JU
Sample : PB140810BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK810

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc