

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033144.D
 Acq On : 18 Nov 2021 06:34
 Operator : CG/JU
 Sample : PB140814BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK814

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033144.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.419	11	14	23	rVB	35926	49113	1.98%	0.175%
2	3.837	81	85	101	rBV	440932	684934	27.59%	2.441%
3	4.161	136	140	146	rVB6	7791	13229	0.53%	0.047%
4	5.866	425	430	432	rBV3	1867	2648	0.11%	0.009%
5	7.119	636	643	654	rBV	529661	849648	34.23%	3.028%
6	7.302	667	674	684	rBV	368493	611435	24.63%	2.179%
7	7.496	700	707	719	rBV	499184	830306	33.45%	2.959%
8	7.972	780	788	796	rBV	373104	618680	24.93%	2.205%
9	8.660	898	905	916	rVV	604050	998923	40.24%	3.560%
10	9.131	976	985	992	rBV	484575	824368	33.21%	2.938%
11	9.848	1100	1107	1116	rBV	390680	650249	26.20%	2.318%
12	10.325	1183	1188	1190	rBV4	1754	2656	0.11%	0.009%
13	10.378	1190	1197	1207	rVV	600266	1031132	41.54%	3.675%
14	10.766	1255	1263	1272	rBV	503580	868110	34.97%	3.094%
15	10.901	1277	1286	1296	rBV	599099	1042215	41.99%	3.715%
16	11.542	1392	1395	1400	rBV5	1698	2626	0.11%	0.009%
17	12.348	1525	1532	1538	rVB3	11386	18128	0.73%	0.065%
18	13.313	1690	1696	1698	rBV4	1311	2515	0.10%	0.009%
19	13.995	1806	1812	1824	rBV	1061788	1480345	59.64%	5.276%
20	14.283	1853	1861	1868	rBV	1145767	1714887	69.09%	6.112%
21	14.589	1906	1913	1920	rBV	744362	1136566	45.79%	4.051%
22	14.766	1937	1943	1954	rBV	498932	705321	28.42%	2.514%
23	14.836	1954	1955	1960	rVB5	2532	3003	0.12%	0.011%
24	14.995	1980	1982	1986	rBV3	2354	2651	0.11%	0.009%
25	15.366	2039	2045	2046	rBV3	2099	3073	0.12%	0.011%
26	15.448	2056	2059	2060	rBV3	2183	2949	0.12%	0.011%
27	15.577	2074	2081	2090	rBV	1418396	2116134	85.25%	7.542%
28	15.683	2093	2099	2111	rVV	397082	559976	22.56%	1.996%
29	15.813	2117	2121	2126	rVB6	6197	9858	0.40%	0.035%
30	16.148	2176	2178	2181	rVB4	2393	2503	0.10%	0.009%
31	16.242	2192	2194	2196	rBV3	2257	2592	0.10%	0.009%
32	16.442	2223	2228	2234	rVB7	2793	4658	0.19%	0.017%
33	17.036	2328	2329	2333	rBV3	2594	2544	0.10%	0.009%
34	17.107	2338	2341	2346	rVB5	3055	5295	0.21%	0.019%
35	17.324	2371	2378	2386	rVV	888790	1298629	52.32%	4.629%
36	17.419	2388	2394	2407	rVV	1555067	2223866	89.59%	7.926%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033144.D
 Acq On : 18 Nov 2021 06:34
 Operator : CG/JU
 Sample : PB140814BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK814

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Title : SVOA CALIBRATION

37	17.501	2407	2408	2412	rVB4	3352	2895	0.12%	0.010%
38	18.001	2486	2493	2495	rBV8	3711	8236	0.33%	0.029%
39	18.201	2523	2527	2532	rBV6	13946	22327	0.90%	0.080%
40	19.001	2661	2663	2664	rBV2	3883	2698	0.11%	0.010%
41	19.271	2705	2709	2714	rVB4	17428	24066	0.97%	0.086%
42	19.336	2716	2720	2726	rVB	17692	27412	1.10%	0.098%
43	19.471	2741	2743	2748	rBV6	7668	8920	0.36%	0.032%
44	19.701	2776	2782	2788	rBV	1876209	2482136	100.00%	8.847%
45	21.477	3079	3084	3090	rBV	1002085	1318862	53.13%	4.701%
46	23.671	3451	3457	3470	rVB2	1218776	2473521	99.65%	8.816%
47	23.824	3477	3483	3492	rVB2	651270	1310128	52.78%	4.670%




Sum of corrected areas: 28056966

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033144.D
Acq On : 18 Nov 2021 06:34
Operator : CG/JU
Sample : PB140814BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK814

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

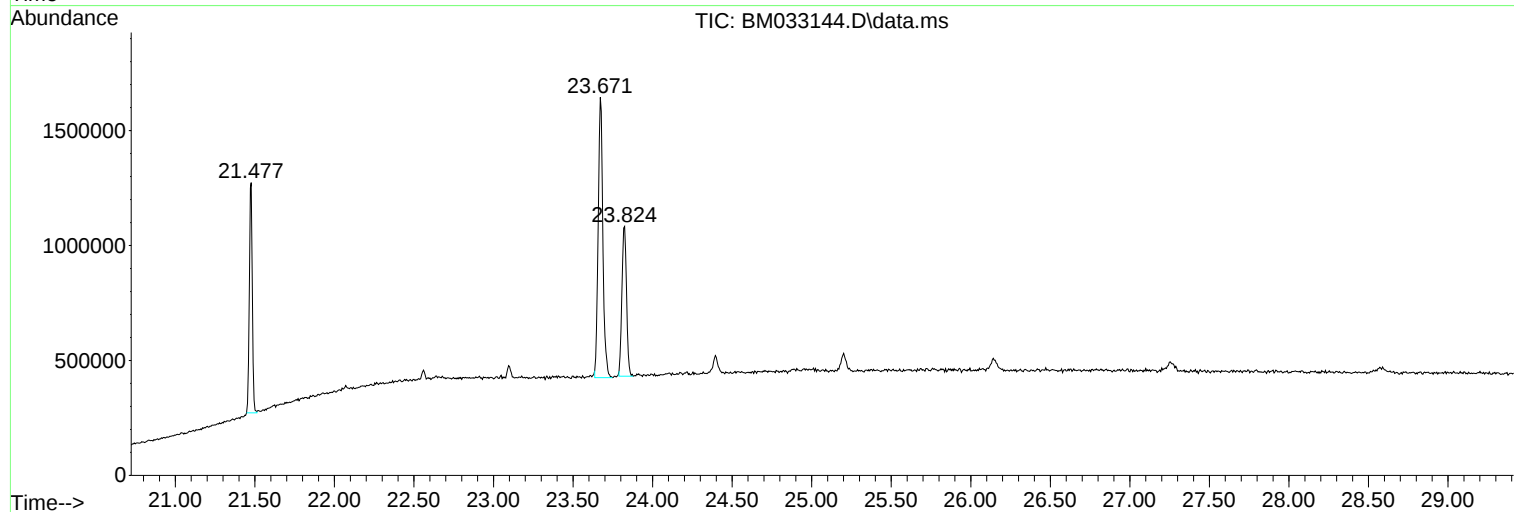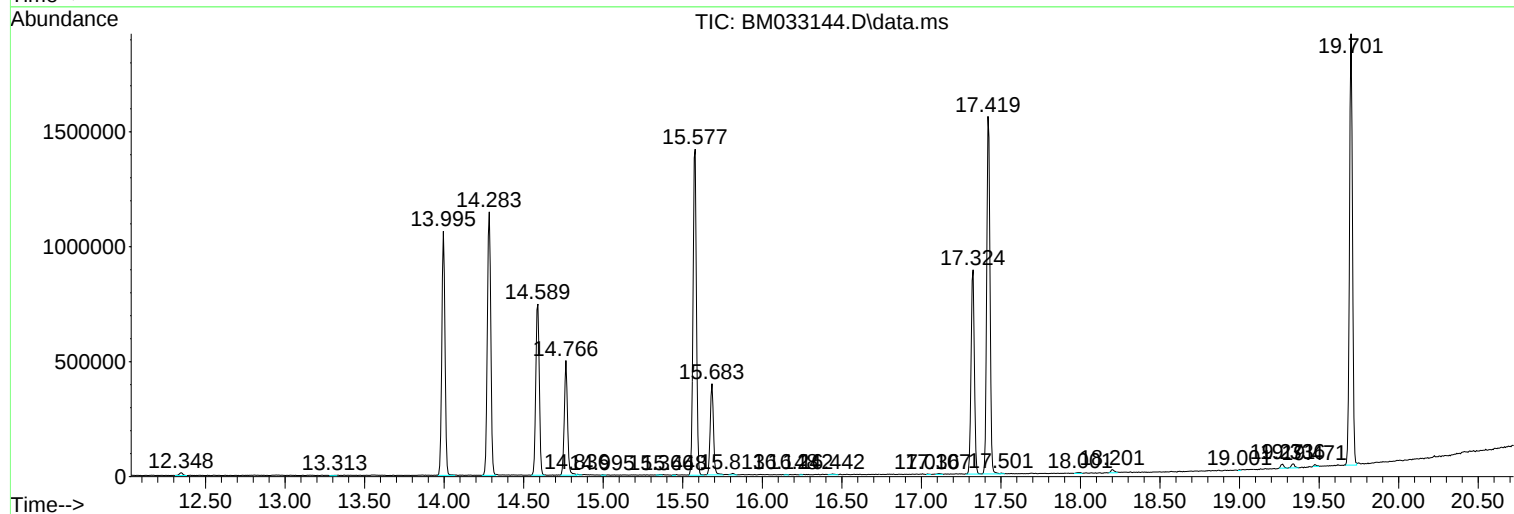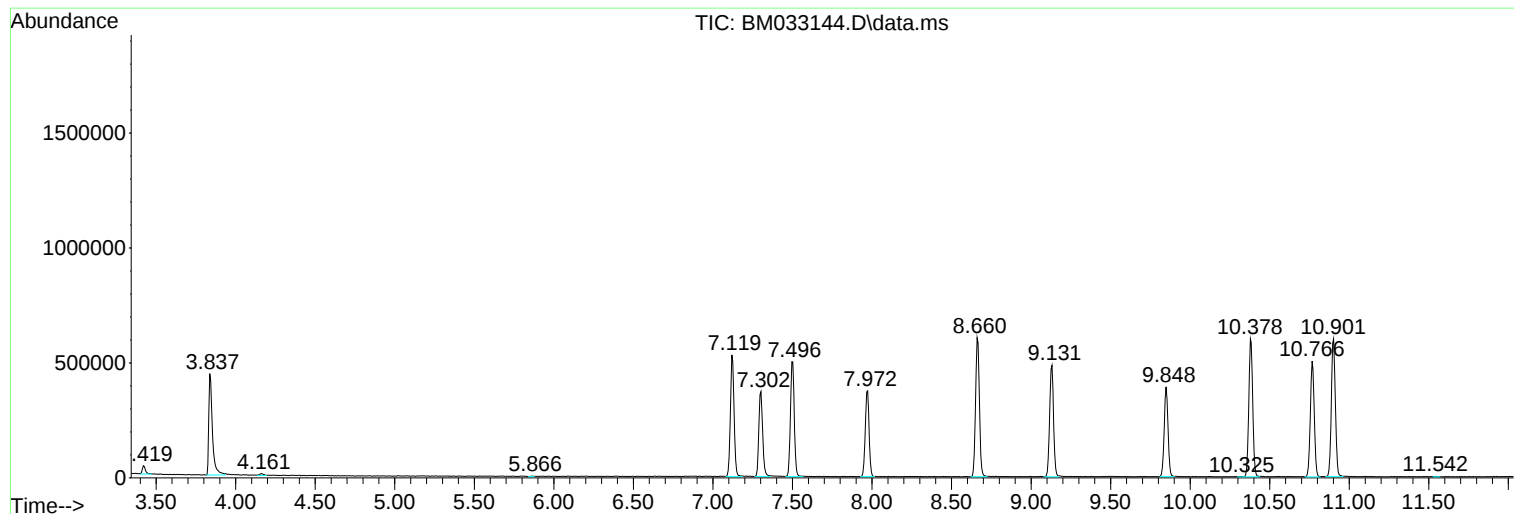

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033144.D
Acq On : 18 Nov 2021 06:34
Operator : CG/JU
Sample : PB140814BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK814

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033144.D
Acq On : 18 Nov 2021 06:34
Operator : CG/JU
Sample : PB140814BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK814

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc