

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033154.D
 Acq On : 18 Nov 2021 14:55
 Operator : CG/JU
 Sample : PB140752BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK752

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033154.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.425	11	15	22	rVB	30882	45298	2.38%	0.179%
2	3.843	82	86	99	rBV	360337	592734	31.11%	2.345%
3	3.972	107	108	111	rVB3	3062	2020	0.11%	0.008%
4	4.125	130	134	136	rBV5	3146	3578	0.19%	0.014%
5	4.166	136	141	146	rVB2	8890	15877	0.83%	0.063%
6	4.596	210	214	216	rBV5	1781	2396	0.13%	0.009%
7	4.701	229	232	233	rBV3	2091	2223	0.12%	0.009%
8	4.766	241	243	245	rVB2	2838	1997	0.10%	0.008%
9	5.107	298	301	302	rVB3	2013	2024	0.11%	0.008%
10	5.131	302	305	306	rBV3	1758	2186	0.11%	0.009%
11	5.225	316	321	322	rBV5	1990	2119	0.11%	0.008%
12	5.243	322	324	327	rBV4	1748	2252	0.12%	0.009%
13	5.601	381	385	389	rBV5	2020	2810	0.15%	0.011%
14	5.666	394	396	399	rVV4	2084	2529	0.13%	0.010%
15	5.725	403	406	408	rBV2	1942	2580	0.14%	0.010%
16	5.748	408	410	414	rVB4	1720	2114	0.11%	0.008%
17	5.984	448	450	452	rVB3	2256	2276	0.12%	0.009%
18	6.013	452	455	456	rBV2	2126	1937	0.10%	0.008%
19	6.301	502	504	510	rVB5	1460	2500	0.13%	0.010%
20	6.442	526	528	533	rVB4	1894	2331	0.12%	0.009%
21	6.490	533	536	538	rBV3	2230	2162	0.11%	0.009%
22	6.619	554	558	561	rVB5	2195	2685	0.14%	0.011%
23	7.119	637	643	656	rVB	467995	750582	39.40%	2.970%
24	7.295	667	673	683	rBV	319408	542089	28.46%	2.145%
25	7.495	701	707	717	rBV	444309	730388	38.34%	2.890%
26	7.566	717	719	723	rVB4	2054	1985	0.10%	0.008%
27	7.854	766	768	771	rBV4	1359	1973	0.10%	0.008%
28	7.966	780	787	797	rVB	443933	726494	38.14%	2.875%
29	8.401	855	861	865	rVB9	1509	2798	0.15%	0.011%
30	8.660	898	905	915	rVV	545660	901205	47.31%	3.566%
31	8.725	915	916	918	rVB2	3914	2120	0.11%	0.008%
32	9.125	976	984	995	rBV	438522	755122	39.64%	2.988%
33	9.525	1050	1052	1055	rVB3	2372	2549	0.13%	0.010%
34	9.607	1061	1066	1069	rBV6	1720	3065	0.16%	0.012%
35	9.848	1098	1107	1116	rBV	351149	591591	31.05%	2.341%
36	10.378	1190	1197	1205	rBV	525561	903244	47.41%	3.574%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033154.D
 Acq On : 18 Nov 2021 14:55
 Operator : CG/JU
 Sample : PB140752BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK752

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Title : SVOA CALIBRATION

37	10.766	1255	1263	1272	rBV	615774	1047469	54.99%	4.145%
38	10.901	1278	1286	1296	rBV	536435	952017	49.97%	3.767%
39	11.172	1327	1332	1335	rBV4	1015	1916	0.10%	0.008%
40	11.530	1390	1393	1394	rBV3	2433	2588	0.14%	0.010%
41	11.830	1443	1444	1447	rBV4	2039	2142	0.11%	0.008%
42	12.007	1471	1474	1477	rBV4	1632	2044	0.11%	0.008%
43	12.342	1526	1531	1537	rVB2	10439	18320	0.96%	0.072%
44	12.730	1594	1597	1600	rBV4	1961	2057	0.11%	0.008%
45	12.766	1600	1603	1607	rVV4	1669	2307	0.12%	0.009%
46	12.801	1607	1609	1612	rVB3	1914	2150	0.11%	0.009%
47	12.901	1623	1626	1629	rBV5	1837	2406	0.13%	0.010%
48	13.136	1664	1666	1670	rBV4	2021	3140	0.16%	0.012%
49	13.319	1693	1697	1702	rBV6	1892	3225	0.17%	0.013%
50	13.554	1734	1737	1743	rVB6	2876	3748	0.20%	0.015%
51	13.995	1804	1812	1822	rBV	955203	1330632	69.85%	5.265%
52	14.283	1852	1861	1869	rBV	1070429	1588699	83.40%	6.286%
53	14.589	1906	1913	1920	rBV	902532	1406606	73.84%	5.566%
54	14.765	1937	1943	1956	rBV	398590	588244	30.88%	2.328%
55	14.936	1970	1972	1975	rBV4	1611	1921	0.10%	0.008%
56	14.995	1979	1982	1985	rVB5	2570	2656	0.14%	0.011%
57	15.401	2049	2051	2056	rVB4	2078	1955	0.10%	0.008%
58	15.477	2062	2064	2068	rVB5	1611	1980	0.10%	0.008%
59	15.571	2074	2080	2087	rBV	1295605	1901768	99.83%	7.525%
60	15.683	2093	2099	2109	rBV	314562	440154	23.11%	1.742%
61	15.812	2118	2121	2124	rBV3	5226	6814	0.36%	0.027%
62	16.130	2173	2175	2178	rVB4	1832	1990	0.10%	0.008%
63	16.354	2210	2213	2214	rBV3	2489	2039	0.11%	0.008%
64	16.442	2224	2228	2234	rVB8	4429	6345	0.33%	0.025%
65	16.524	2237	2242	2245	rBV6	1384	2254	0.12%	0.009%
66	16.836	2293	2295	2299	rVB4	1503	2000	0.10%	0.008%
67	16.901	2303	2306	2309	rBV4	1501	2403	0.13%	0.010%
68	16.959	2313	2316	2319	rBV5	2579	3799	0.20%	0.015%
69	17.106	2338	2341	2346	rVB2	4943	7372	0.39%	0.029%
70	17.324	2371	2378	2386	rBV	1002884	1478185	77.60%	5.849%
71	17.418	2388	2394	2407	rVB	1319010	1895887	99.52%	7.502%
72	18.201	2523	2527	2532	rBV6	11874	18894	0.99%	0.075%
73	18.595	2592	2594	2596	rBV3	2746	3026	0.16%	0.012%
74	18.971	2656	2658	2659	rBV2	3820	2008	0.11%	0.008%
75	19.265	2705	2708	2714	rVB4	14117	19368	1.02%	0.077%
76	19.330	2717	2719	2723	rVB2	13355	14530	0.76%	0.057%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033154.D
Acq On : 18 Nov 2021 14:55
Operator : CG/JU
Sample : PB140752BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK752

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Title : SVOA CALIBRATION

77	19.700	2776	2782	2791	rBV	1395577	1904989	100.00%	7.538%
78	21.477	3079	3084	3090	rBV	920895	1209905	63.51%	4.788%
79	23.671	3451	3457	3467	rVB2	789553	1612469	84.64%	6.380%
80	23.824	3477	3483	3492	rVB2	583542	1153884	60.57%	4.566%


Sum of corrected areas: 25272138

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033154.D
Acq On : 18 Nov 2021 14:55
Operator : CG/JU
Sample : PB140752BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK752

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

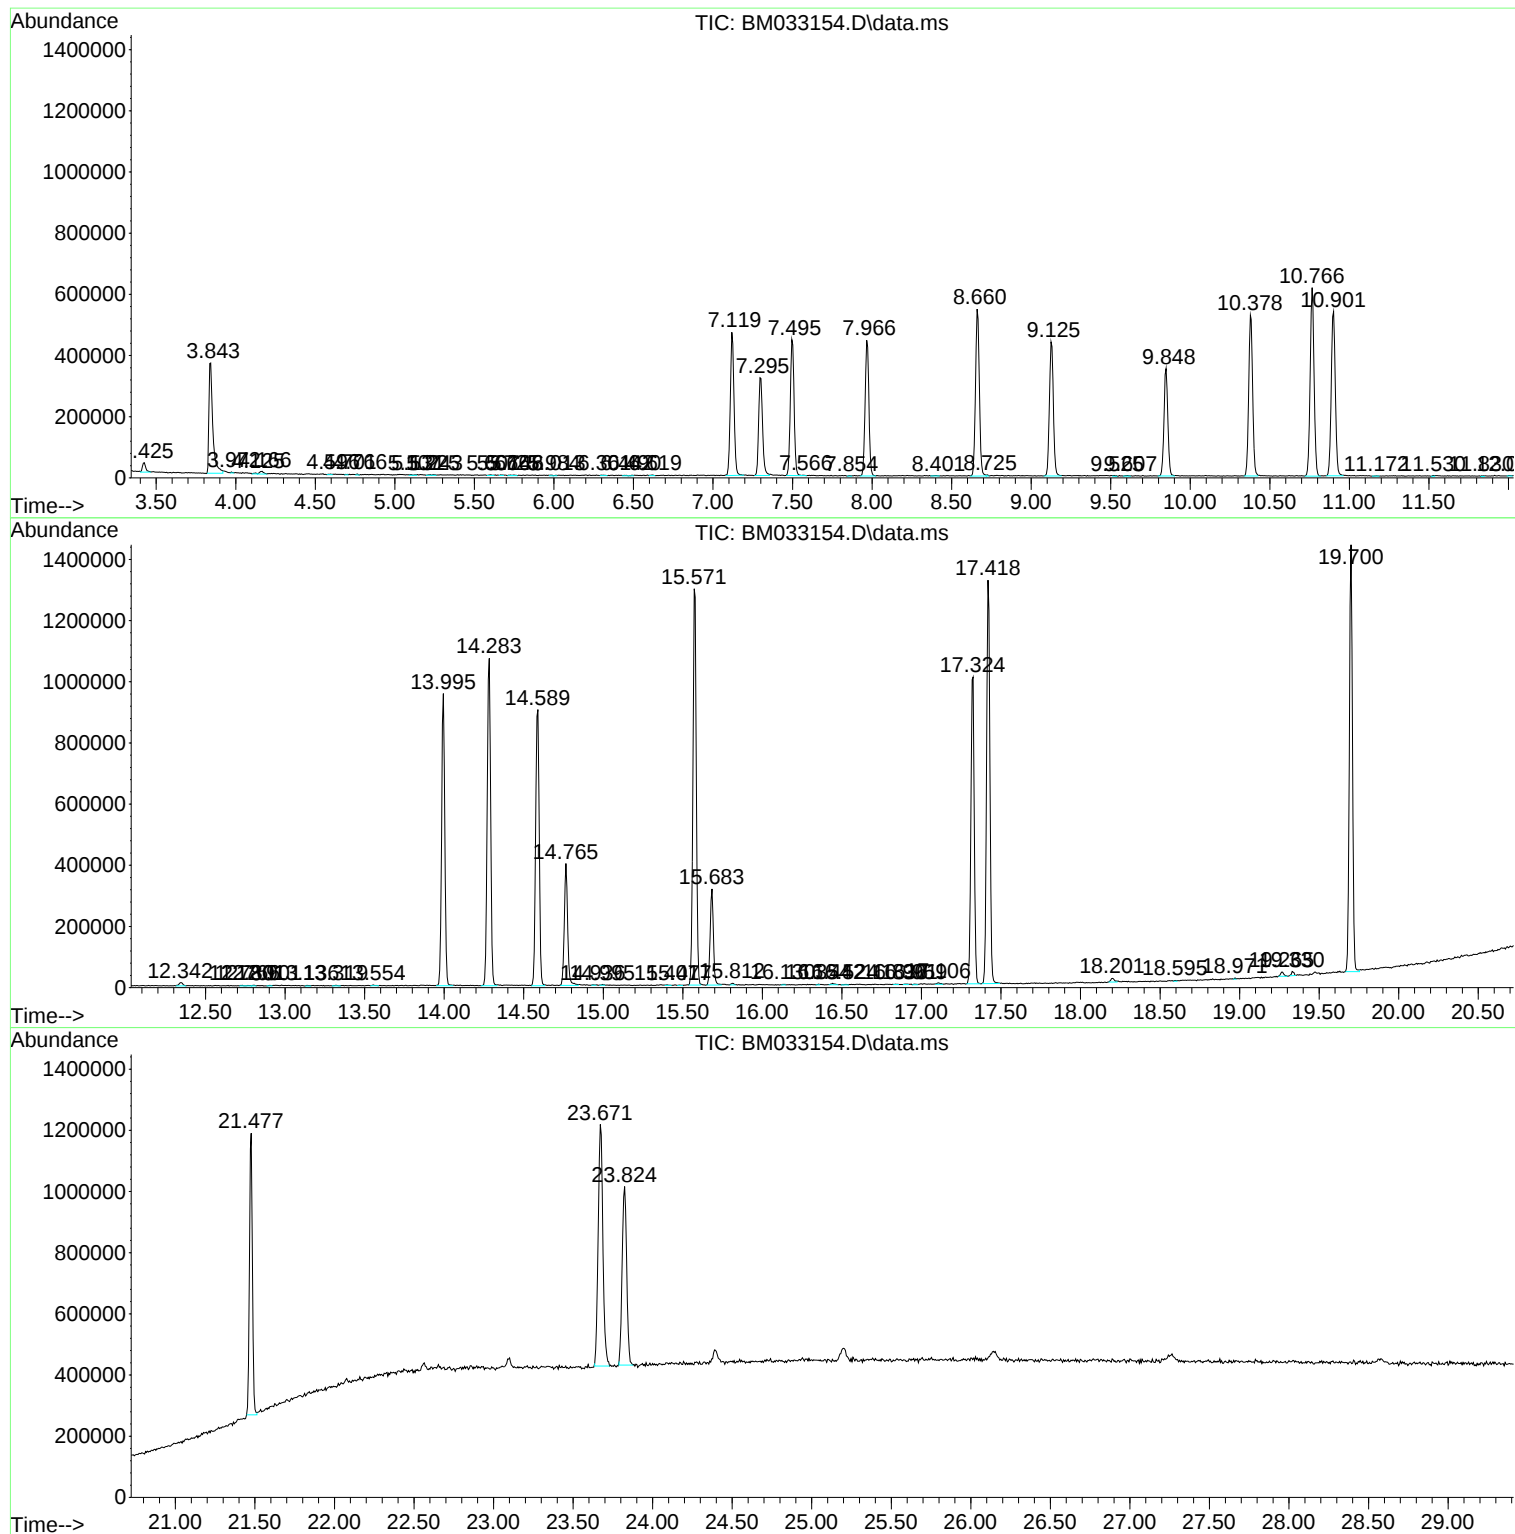

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033154.D
Acq On : 18 Nov 2021 14:55
Operator : CG/JU
Sample : PB140752BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK752

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033154.D
Acq On : 18 Nov 2021 14:55
Operator : CG/JU
Sample : PB140752BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK752

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc