

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033155.D
 Acq On : 18 Nov 2021 15:31
 Operator : CG/JU
 Sample : PB140817BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK817

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033155.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.425	11	15	21	rVB	27986	37636	1.46%	0.135%
2	3.837	82	85	107	rBV	378398	628901	24.33%	2.254%
3	4.154	136	139	144	rBV2	5798	9399	0.36%	0.034%
4	5.578	379	381	386	rBV5	1921	3903	0.15%	0.014%
5	7.119	635	643	651	rBV	492693	782652	30.28%	2.805%
6	7.301	666	674	682	rBV	334733	561405	21.72%	2.012%
7	7.495	700	707	716	rBV	459735	752525	29.11%	2.697%
8	7.654	729	734	736	rBV6	1612	2737	0.11%	0.010%
9	7.966	780	787	797	rVB	376616	621737	24.05%	2.229%
10	8.431	863	866	871	rVB6	2064	2918	0.11%	0.010%
11	8.660	898	905	916	rBV	559122	938804	36.32%	3.365%
12	9.125	977	984	997	rBV	460199	790638	30.59%	2.834%
13	9.313	1012	1016	1019	rVB6	1688	2599	0.10%	0.009%
14	9.848	1099	1107	1116	rBV	383930	633421	24.51%	2.270%
15	10.378	1189	1197	1206	rBV	564314	970504	37.55%	3.479%
16	10.766	1256	1263	1271	rBV	532800	915654	35.42%	3.282%
17	10.901	1279	1286	1295	rBV	574399	1011589	39.14%	3.626%
18	10.960	1295	1296	1299	rVB3	3804	2836	0.11%	0.010%
19	12.348	1526	1532	1539	rVB3	11469	19009	0.74%	0.068%
20	13.324	1694	1698	1701	rBV4	1950	2921	0.11%	0.010%
21	13.566	1734	1739	1741	rBV4	2179	3593	0.14%	0.013%
22	13.789	1776	1777	1782	rVB4	1810	2835	0.11%	0.010%
23	13.995	1805	1812	1818	rBV	1145818	1555650	60.18%	5.576%
24	14.283	1854	1861	1871	rBV	1174294	1757420	67.99%	6.299%
25	14.589	1906	1913	1922	rBV	844632	1303251	50.42%	4.671%
26	14.765	1936	1943	1950	rBV	522907	749884	29.01%	2.688%
27	15.571	2073	2080	2088	rBV	1468375	2218516	85.83%	7.952%
28	15.683	2093	2099	2110	rBV	438666	594234	22.99%	2.130%
29	15.812	2117	2121	2126	rVB6	7167	10054	0.39%	0.036%
30	16.442	2225	2228	2234	rVB6	5144	6201	0.24%	0.022%
31	16.683	2266	2269	2272	rVB5	2971	3334	0.13%	0.012%
32	17.001	2322	2323	2327	rVB3	2380	2759	0.11%	0.010%
33	17.112	2338	2342	2344	rVB4	3536	4252	0.16%	0.015%
34	17.242	2360	2364	2367	rBV5	2176	3360	0.13%	0.012%
35	17.324	2371	2378	2387	rVV	1059731	1540724	59.61%	5.523%
36	17.418	2388	2394	2407	rVV2	1653187	2406907	93.12%	8.627%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033155.D
 Acq On : 18 Nov 2021 15:31
 Operator : CG/JU
 Sample : PB140817BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK817

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Title : SVOA CALIBRATION

37	17.918	2475	2479	2480	rBV4	2171	2659	0.10%	0.010%
38	17.989	2486	2491	2492	rBV4	4000	5366	0.21%	0.019%
39	18.059	2499	2503	2504	rBV2	2208	2627	0.10%	0.009%
40	18.201	2523	2527	2533	rBV6	16026	24761	0.96%	0.089%
41	19.271	2703	2709	2713	rBV4	18500	32175	1.24%	0.115%
42	19.336	2716	2720	2725	rBV	21658	32257	1.25%	0.116%
43	19.700	2776	2782	2790	rBV	1862299	2584845	100.00%	9.265%
44	21.477	3079	3084	3090	rBV	1039081	1325229	51.27%	4.750%
45	23.671	3451	3457	3468	rVB2	973490	1898267	73.44%	6.804%
46	23.824	3477	3483	3491	rVB2	574738	1135282	43.92%	4.069%




Sum of corrected areas: 27898230

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033155.D
Acq On : 18 Nov 2021 15:31
Operator : CG/JU
Sample : PB140817BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK817

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

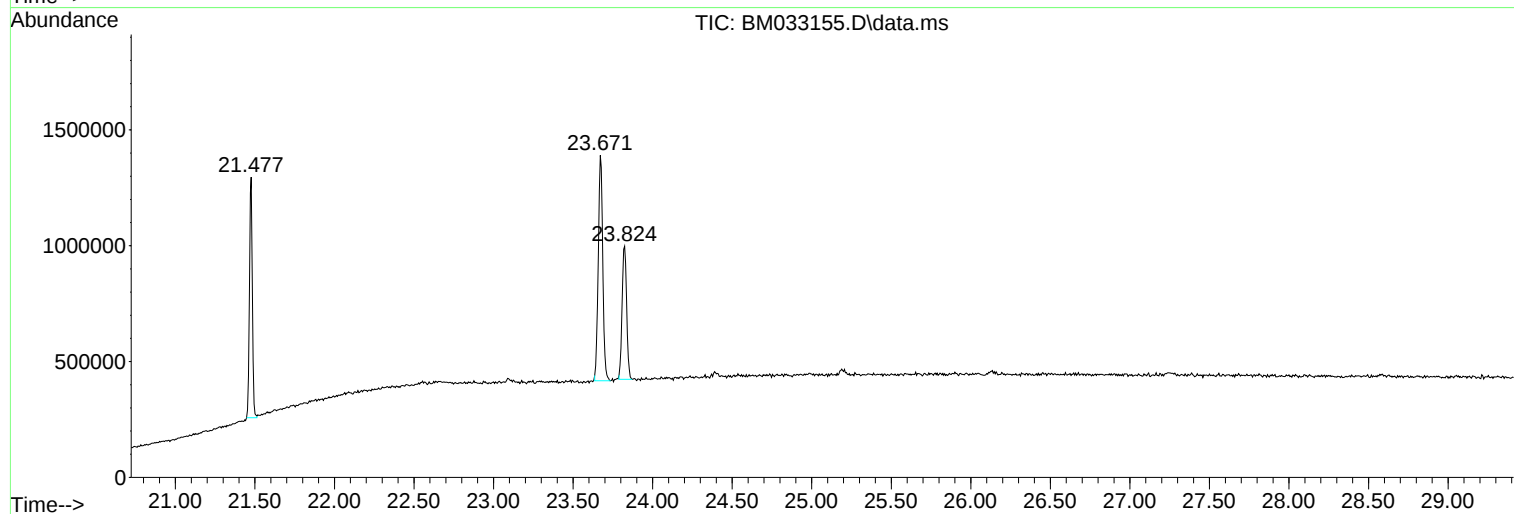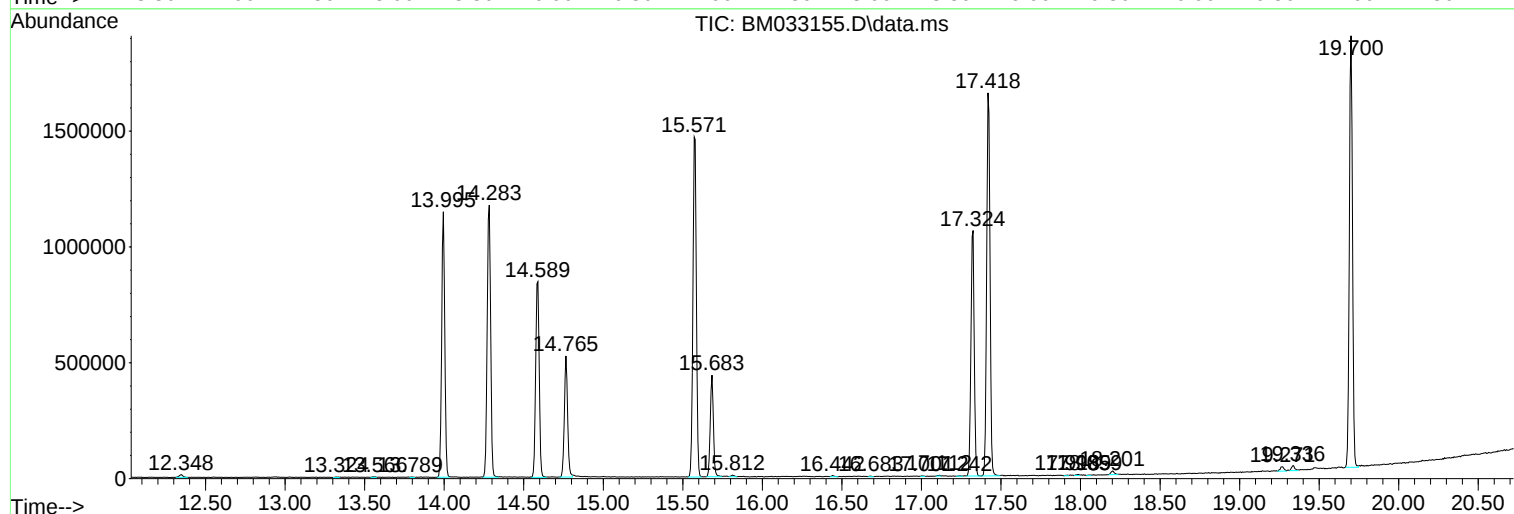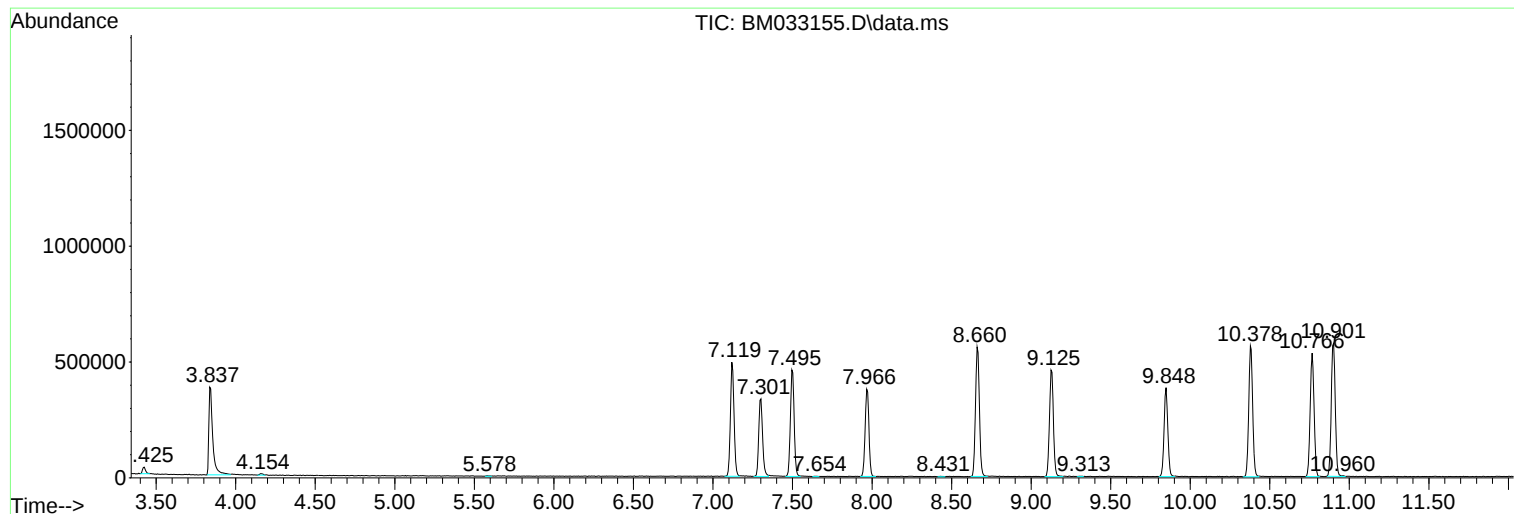

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033155.D
Acq On : 18 Nov 2021 15:31
Operator : CG/JU
Sample : PB140817BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK817

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033155.D
Acq On : 18 Nov 2021 15:31
Operator : CG/JU
Sample : PB140817BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK817

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc