

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033161.D
 Acq On : 18 Nov 2021 19:10
 Operator : CG/JU
 Sample : M4677-16
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AB0

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033161.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.419	11	14	22	rVB2	25397	37749	0.97%	0.117%
2	3.849	83	87	97	rBV	68421	132011	3.38%	0.410%
3	4.060	118	123	129	rBV4	9301	16444	0.42%	0.051%
4	4.160	136	140	145	rVB3	8130	12115	0.31%	0.038%
5	5.290	328	332	335	rVB6	2910	4272	0.11%	0.013%
6	7.119	637	643	655	rVB	93711	167355	4.28%	0.519%
7	7.295	666	673	687	rBV	323899	552504	14.13%	1.714%
8	7.495	698	707	718	rVV	338932	549559	14.06%	1.705%
9	7.584	718	722	727	rVB5	2391	4656	0.12%	0.014%
10	7.966	780	787	795	rBV	396395	634228	16.22%	1.968%
11	8.660	899	905	913	rBV2	275109	450203	11.52%	1.397%
12	9.066	969	974	978	rBV2	8261	14599	0.37%	0.045%
13	9.125	978	984	994	rVB	463928	780874	19.97%	2.423%
14	9.519	1047	1051	1058	rVB3	4766	8828	0.23%	0.027%
15	9.848	1097	1107	1117	rBV	340570	593226	15.17%	1.841%
16	10.378	1190	1197	1208	rBV	526174	871967	22.30%	2.706%
17	10.548	1222	1226	1234	rBV3	13541	25393	0.65%	0.079%
18	10.766	1253	1263	1271	rBV	551332	953057	24.38%	2.957%
19	10.895	1278	1285	1301	rVB	503390	885856	22.66%	2.749%
20	11.536	1388	1394	1397	rBV5	3443	5417	0.14%	0.017%
21	12.342	1526	1531	1538	rVB3	10342	19031	0.49%	0.059%
22	13.995	1805	1812	1818	rBV	1224676	1686017	43.12%	5.232%
23	14.183	1839	1844	1848	rBV4	2218	4235	0.11%	0.013%
24	14.277	1854	1860	1868	rBV	1194067	1790456	45.80%	5.556%
25	14.583	1903	1912	1920	rBV	930284	1378284	35.25%	4.277%
26	14.765	1934	1943	1959	rBV	116323	195704	5.01%	0.607%
27	15.001	1976	1983	1986	rBV5	7572	12959	0.33%	0.040%
28	15.571	2071	2080	2091	rBV	1747275	2519386	64.44%	7.818%
29	15.683	2092	2099	2109	rBV	602011	854632	21.86%	2.652%
30	15.812	2116	2121	2127	rVB5	8162	11425	0.29%	0.035%
31	16.354	2209	2213	2217	rBV6	2918	3995	0.10%	0.012%
32	16.442	2224	2228	2233	rVB8	3406	5110	0.13%	0.016%
33	17.107	2338	2341	2344	rVV3	4005	4874	0.12%	0.015%
34	17.230	2358	2362	2367	rBV6	3226	6621	0.17%	0.021%
35	17.324	2371	2378	2384	rVV	1151568	1732051	44.30%	5.375%
36	17.418	2387	2394	2403	rVV2	2219898	3193639	81.68%	9.910%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033161.D
 Acq On : 18 Nov 2021 19:10
 Operator : CG/JU
 Sample : M4677-16
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Title : SVOA CALIBRATION

37	17.495	2405	2407	2412	rVB5	6660	10580	0.27%	0.033%
38	17.695	2436	2441	2445	rBV6	4643	7923	0.20%	0.025%
39	17.983	2485	2490	2494	rBV3	14848	18970	0.49%	0.059%
40	18.201	2522	2527	2534	rBV2	52395	84535	2.16%	0.262%
41	18.283	2537	2541	2545	rVV3	12686	18991	0.49%	0.059%
42	18.583	2589	2592	2594	rBV4	3323	4196	0.11%	0.013%
43	19.101	2677	2680	2682	rBV4	5099	6270	0.16%	0.019%
44	19.265	2704	2708	2712	rBV3	33020	48545	1.24%	0.151%
45	19.336	2715	2720	2726	rVV	33778	56633	1.45%	0.176%
46	19.471	2739	2743	2747	rBV5	26463	40431	1.03%	0.125%
47	19.700	2776	2782	2790	rBV	2781739	3909704	100.00%	12.132%
48	21.177	3029	3033	3038	rBV	131363	167965	4.30%	0.521%
49	21.477	3079	3084	3089	rBV	1523037	2023793	51.76%	6.280%
50	23.677	3451	3458	3468	rVB2	1911946	3834626	98.08%	11.899%
51	23.824	3477	3483	3490	rVB2	962857	1874328	47.94%	5.816%




Sum of corrected areas: 32226222

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033161.D
Acq On : 18 Nov 2021 19:10
Operator : CG/JU
Sample : M4677-16
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AB0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

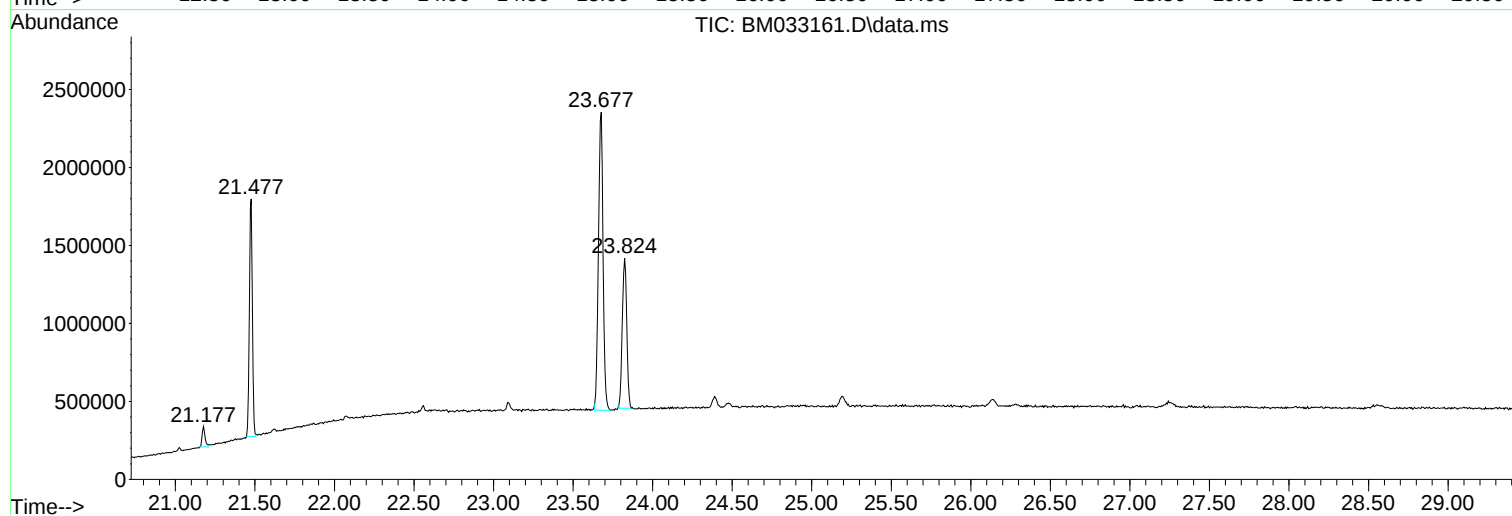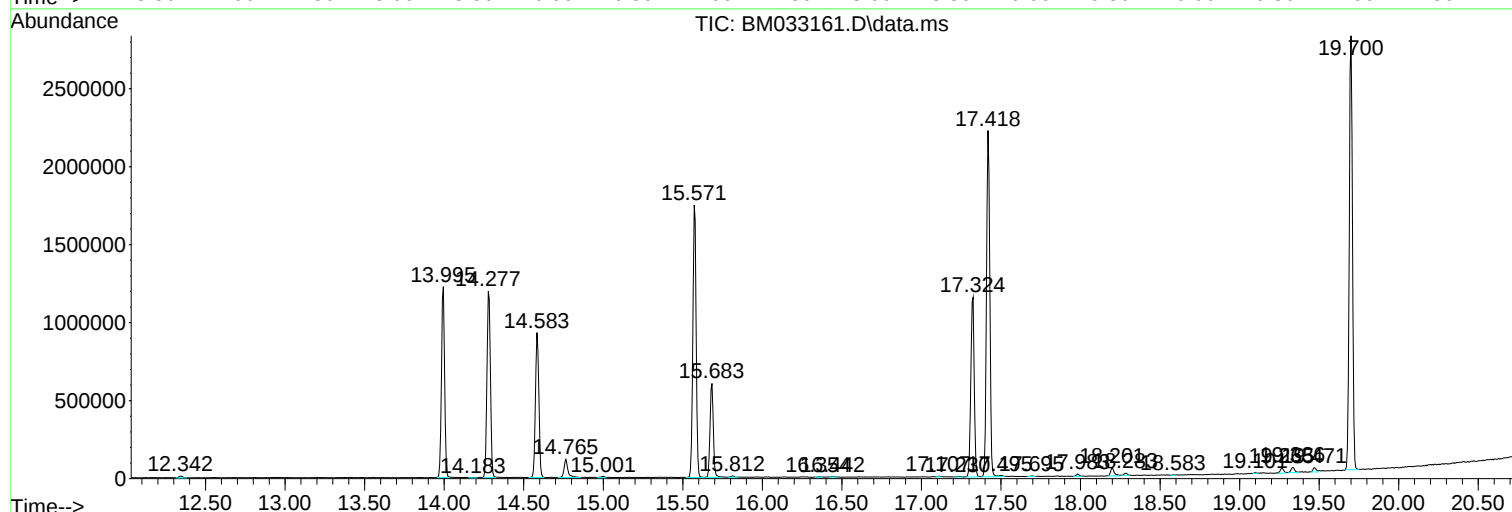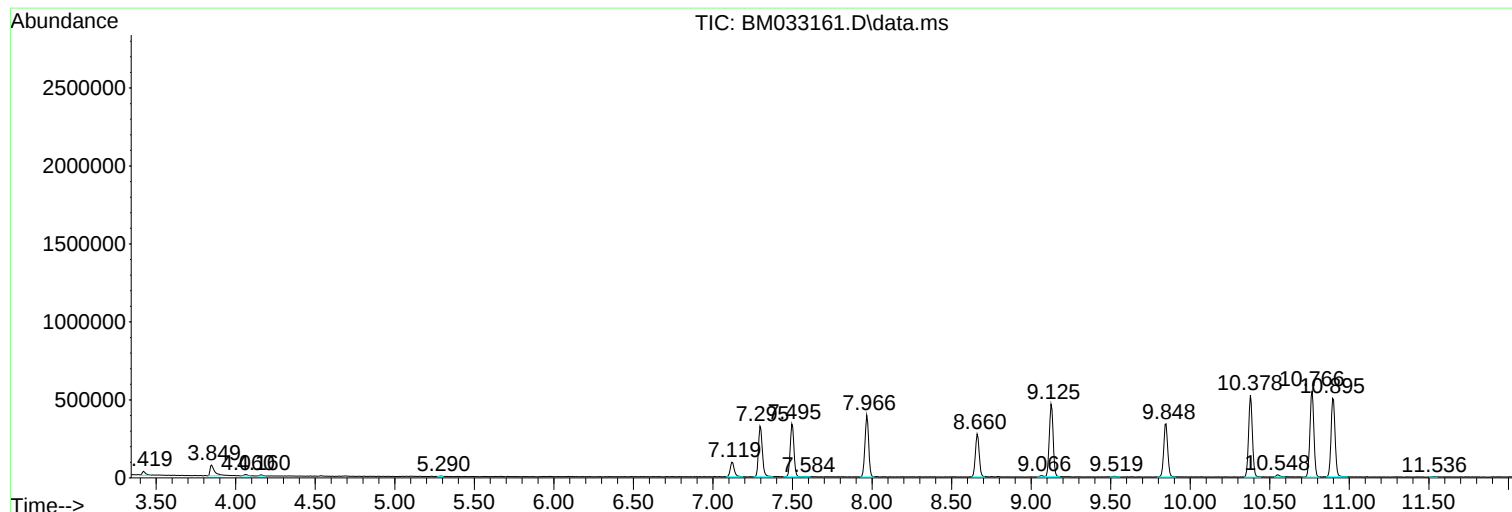

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033161.D
Acq On : 18 Nov 2021 19:10
Operator : CG/JU
Sample : M4677-16
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AB0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033161.D
Acq On : 18 Nov 2021 19:10
Operator : CG/JU
Sample : M4677-16
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AB0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
