

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033166.D
 Acq On : 18 Nov 2021 22:12
 Operator : CG/JU
 Sample : PB147789BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK789

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033166.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.678	54	58	63	rVB3	20355	28185	1.75%	0.369%
2	3.813	79	81	83	rBV3	1978	2084	0.13%	0.027%
3	4.149	135	138	143	rVB2	6839	9457	0.59%	0.124%
4	4.748	238	240	242	rBV3	1920	1715	0.11%	0.022%
5	5.078	294	296	297	rBV2	2462	2107	0.13%	0.028%
6	5.731	403	407	408	rBV3	1837	2490	0.15%	0.033%
7	5.954	443	445	450	rVV5	1853	1854	0.12%	0.024%
8	6.595	551	554	557	rBV5	1433	1739	0.11%	0.023%
9	7.542	712	715	719	rVB5	1466	1921	0.12%	0.025%
10	7.966	779	787	794	rBV	426677	700409	43.59%	9.168%
11	8.042	798	800	803	rVV4	1626	1862	0.12%	0.024%
12	8.078	803	806	808	rVB4	1638	1911	0.12%	0.025%
13	8.413	858	863	864	rBV4	1915	1796	0.11%	0.024%
14	8.507	876	879	886	rBV5	1445	3303	0.21%	0.043%
15	8.707	907	913	914	rBV4	1397	2018	0.13%	0.026%
16	8.725	914	916	921	rVV5	1772	2292	0.14%	0.030%
17	8.795	926	928	932	rVB4	1269	1615	0.10%	0.021%
18	9.683	1072	1079	1080	rVB4	1295	1932	0.12%	0.025%
19	9.948	1120	1124	1126	rBV4	1342	2125	0.13%	0.028%
20	10.025	1134	1137	1140	rBV4	1255	2003	0.12%	0.026%
21	10.760	1254	1262	1271	rBV	520100	916373	57.03%	11.995%
22	10.825	1271	1273	1276	rVB4	1559	1662	0.10%	0.022%
23	11.083	1314	1317	1321	rVB5	1307	2047	0.13%	0.027%
24	11.560	1395	1398	1401	rBV4	1314	1670	0.10%	0.022%
25	11.907	1451	1457	1460	rVB4	1542	2902	0.18%	0.038%
26	11.942	1460	1463	1466	rVB4	2316	2817	0.18%	0.037%
27	11.977	1466	1469	1470	rBV3	2093	2087	0.13%	0.027%
28	11.989	1470	1471	1475	rVB4	1685	1812	0.11%	0.024%
29	12.177	1499	1503	1508	rBV5	1453	2614	0.16%	0.034%
30	12.795	1602	1608	1609	rBV3	2004	2402	0.15%	0.031%
31	13.148	1666	1668	1673	rVB5	1424	2013	0.13%	0.026%
32	13.348	1700	1702	1705	rBV4	1311	1845	0.11%	0.024%
33	14.148	1836	1838	1843	rBV4	1671	2283	0.14%	0.030%
34	14.271	1855	1859	1862	rBV4	1297	2203	0.14%	0.029%
35	14.430	1884	1886	1890	rVB3	1702	2150	0.13%	0.028%
36	14.583	1905	1912	1921	rBV	817671	1204668	74.97%	15.769%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
 Data File : BM033166.D
 Acq On : 18 Nov 2021 22:12
 Operator : CG/JU
 Sample : PB147789BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK789

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
 Title : SVOA CALIBRATION

37	14.848	1954	1957	1959	rBV3	2077	2178	0.14%	0.029%
38	15.207	2015	2018	2019	rBV	1715	1782	0.11%	0.023%
39	15.236	2019	2023	2027	rVB4	1450	3065	0.19%	0.040%
40	15.565	2077	2079	2087	rVB7	1967	2718	0.17%	0.036%
41	15.730	2106	2107	2111	rBV4	1620	1758	0.11%	0.023%
42	16.012	2151	2155	2156	rBV3	1862	2279	0.14%	0.030%
43	16.071	2162	2165	2168	rVB3	1764	2080	0.13%	0.027%
44	16.312	2205	2206	2211	rVB4	2034	1630	0.10%	0.021%
45	16.442	2224	2228	2235	rVB4	3043	5322	0.33%	0.070%
46	16.518	2235	2241	2243	rBV4	1990	2727	0.17%	0.036%
47	16.583	2249	2252	2253	rBV2	1567	1953	0.12%	0.026%
48	16.648	2260	2263	2265	rVB3	1935	1861	0.12%	0.024%
49	16.736	2274	2278	2281	rBV5	2065	2811	0.17%	0.037%
50	16.789	2283	2287	2289	rVB4	2811	3772	0.23%	0.049%
51	17.101	2335	2340	2346	rBV2	3892	8204	0.51%	0.107%
52	17.236	2361	2363	2364	rBV	3202	2112	0.13%	0.028%
53	17.318	2369	2377	2386	rBV	1088271	1555604	96.80%	20.362%
54	17.412	2390	2393	2399	rVB3	3614	5825	0.36%	0.076%
55	17.648	2430	2433	2435	rBV4	2423	2425	0.15%	0.032%
56	17.689	2438	2440	2445	rVV6	2689	3114	0.19%	0.041%
57	17.971	2486	2488	2491	rBV4	1646	1803	0.11%	0.024%
58	18.054	2499	2502	2503	rBV2	2627	2712	0.17%	0.035%
59	18.130	2513	2515	2517	rVB3	2683	2278	0.14%	0.030%
60	18.154	2517	2519	2523	rBV4	2040	3227	0.20%	0.042%
61	18.195	2523	2526	2531	rBV5	9484	13769	0.86%	0.180%
62	18.236	2531	2533	2536	rVV4	1799	2447	0.15%	0.032%
63	18.601	2593	2595	2596	rBV2	2184	1985	0.12%	0.026%
64	18.765	2621	2623	2624	rBV2	5033	3099	0.19%	0.041%
65	18.883	2641	2643	2644	rBV2	3213	2212	0.14%	0.029%
66	18.901	2644	2646	2648	rVV3	3147	2792	0.17%	0.037%
67	21.471	3078	3083	3090	rBV	1241987	1606963	100.00%	21.034%
68	23.818	3476	3482	3491	rVB2	741780	1458794	90.78%	19.095%




Sum of corrected areas: 7639667

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033166.D
Acq On : 18 Nov 2021 22:12
Operator : CG/JU
Sample : PB147789BL
Misc : GCMS CONFIRMATION
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK789

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

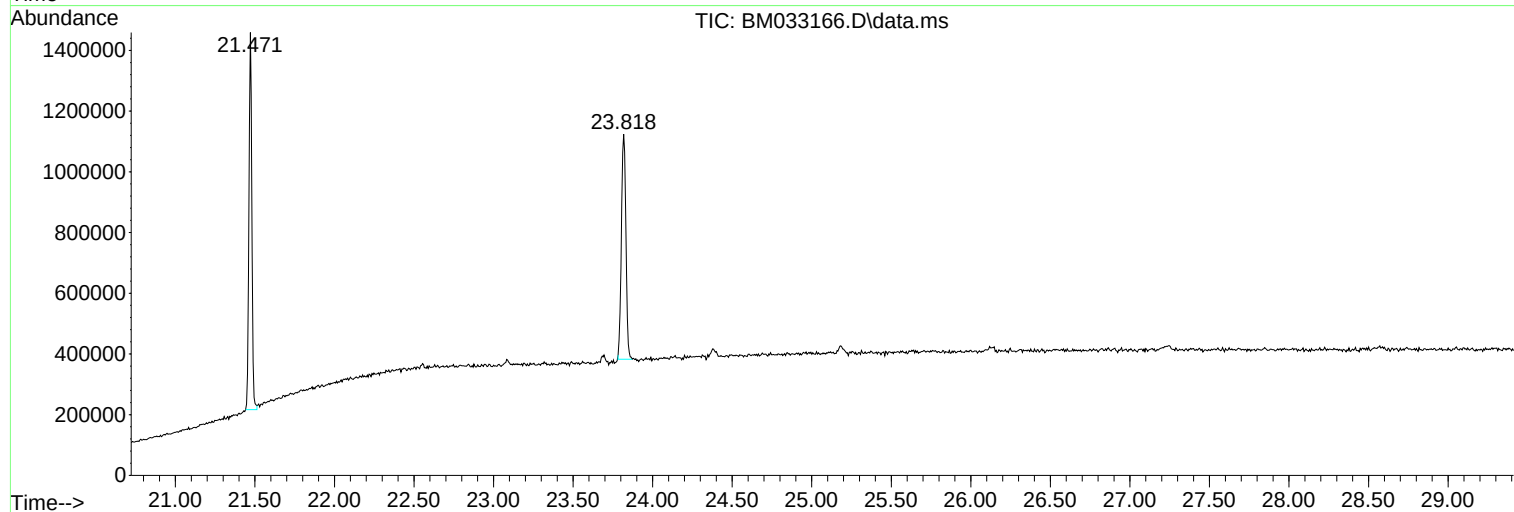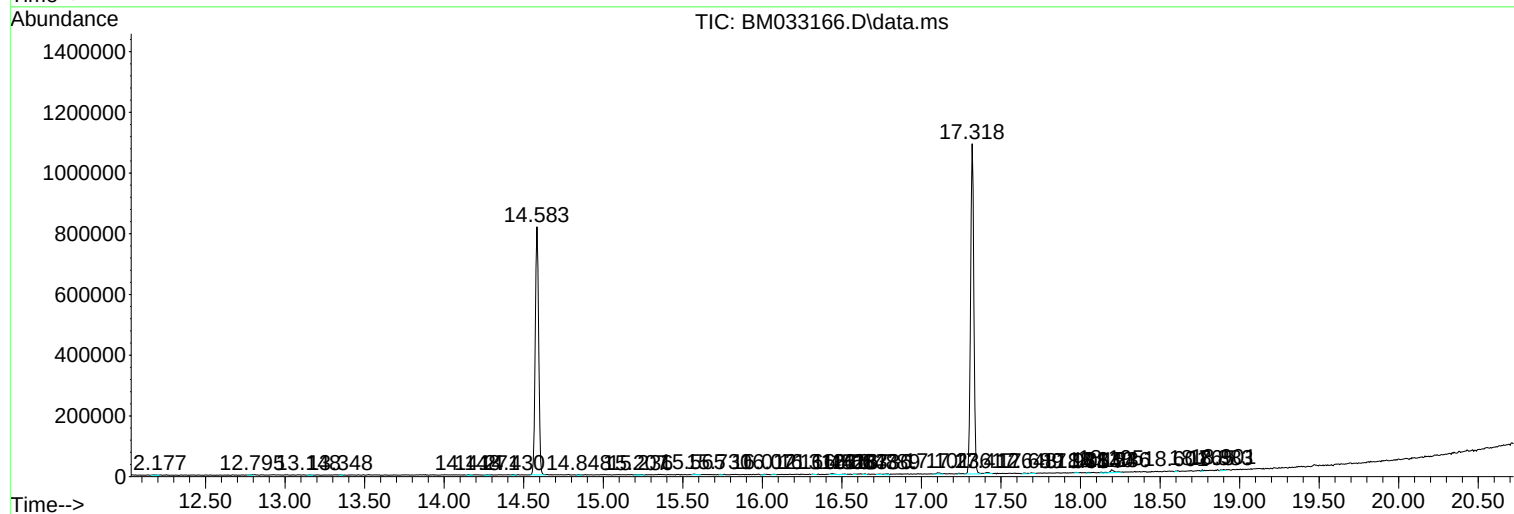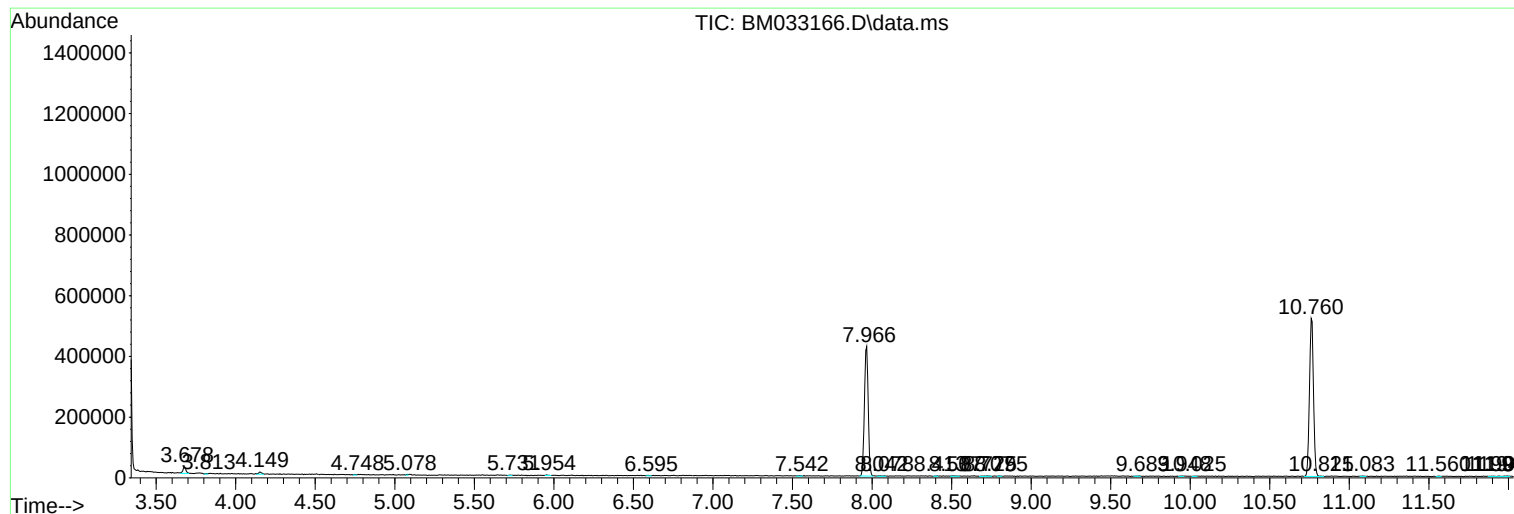

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033166.D
Acq On : 18 Nov 2021 22:12
Operator : CG/JU
Sample : PB147789BL
Misc : GCMS CONFIRMATION
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK789

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111721\
Data File : BM033166.D
Acq On : 18 Nov 2021 22:12
Operator : CG/JU
Sample : PB147789BL
Misc : GCMS CONFIRMATION
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK789

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM111721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc