

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042890.D
 Acq On : 18 Nov 2023 20:21
 Operator : MA/JU
 Sample : 05268-05
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Nov 18 22:10:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 18 22:06:09 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	17726	20.000	ng/ul	0.00
20) Naphthalene-d8	10.628	136	72238	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.469	164	44955	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.227	188	94285	20.000	ng/ul	0.00
79) Chrysene-d12	21.415	240	103332	20.000	ng/ul	0.00
88) Perylene-d12	23.768	264	128508	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0	0.000	ng/uL	
4) Pyridine-d5	3.599	84	70	0.050	ng/ul	0.00
7) Phenol-d5	0.000	99	0	0.000	ng/ul	
9) Bis-(2-Chloroethyl)eth...	0.000	67	0	0.000	ng/ul	
11) 2-Chlorophenol-d4	0.000	132	0	0.000	ng/ul	
15) 4-Methylphenol-d8	0.000	113	0	0.000	ng/ul	
21) Nitrobenzene-d5	0.000	128	0	0.000	ng/ul	
24) 2-Nitrophenol-d4	0.000	143	0	0.000	ng/ul	
28) 2,4-Dichlorophenol-d3	0.000	165	0	0.000	ng/ul	
31) 4-Chloroaniline-d4	0.000	131	0	0.000	ng/ul	
46) Dimethylphthalate-d6	13.916	166	3913	0.920	ng/ul	0.02
49) Acenaphthylene-d8	14.180	160	4493	0.987	ng/ul	0.01
54) 4-Nitrophenol-d4	0.000	143	0	0.000	ng/ul	
60) Fluorene-d10	15.486	176	3744	1.063	ng/ul	0.02
65) 4,6-Dinitro-2-methylph...	0.000	200	0	0.000	ng/ul	
73) Anthracene-d10	17.333	188	5590	1.058	ng/ul	0.00
81) Pyrene-d10	19.633	212	8819	1.303	ng/ul	0.01
92) Benzo(a)pyrene-d12	23.768	264	108112	14.065	ng/ul	0.15
Target Compounds						
					Qvalue	
30) Naphthalene	10.681	128	79933	17.662	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042890.D
Acq On : 18 Nov 2023 20:21
Operator : MA/JU
Sample : 05268-05
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Nov 18 22:10:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 18 22:06:09 2023
Response via : Initial Calibration

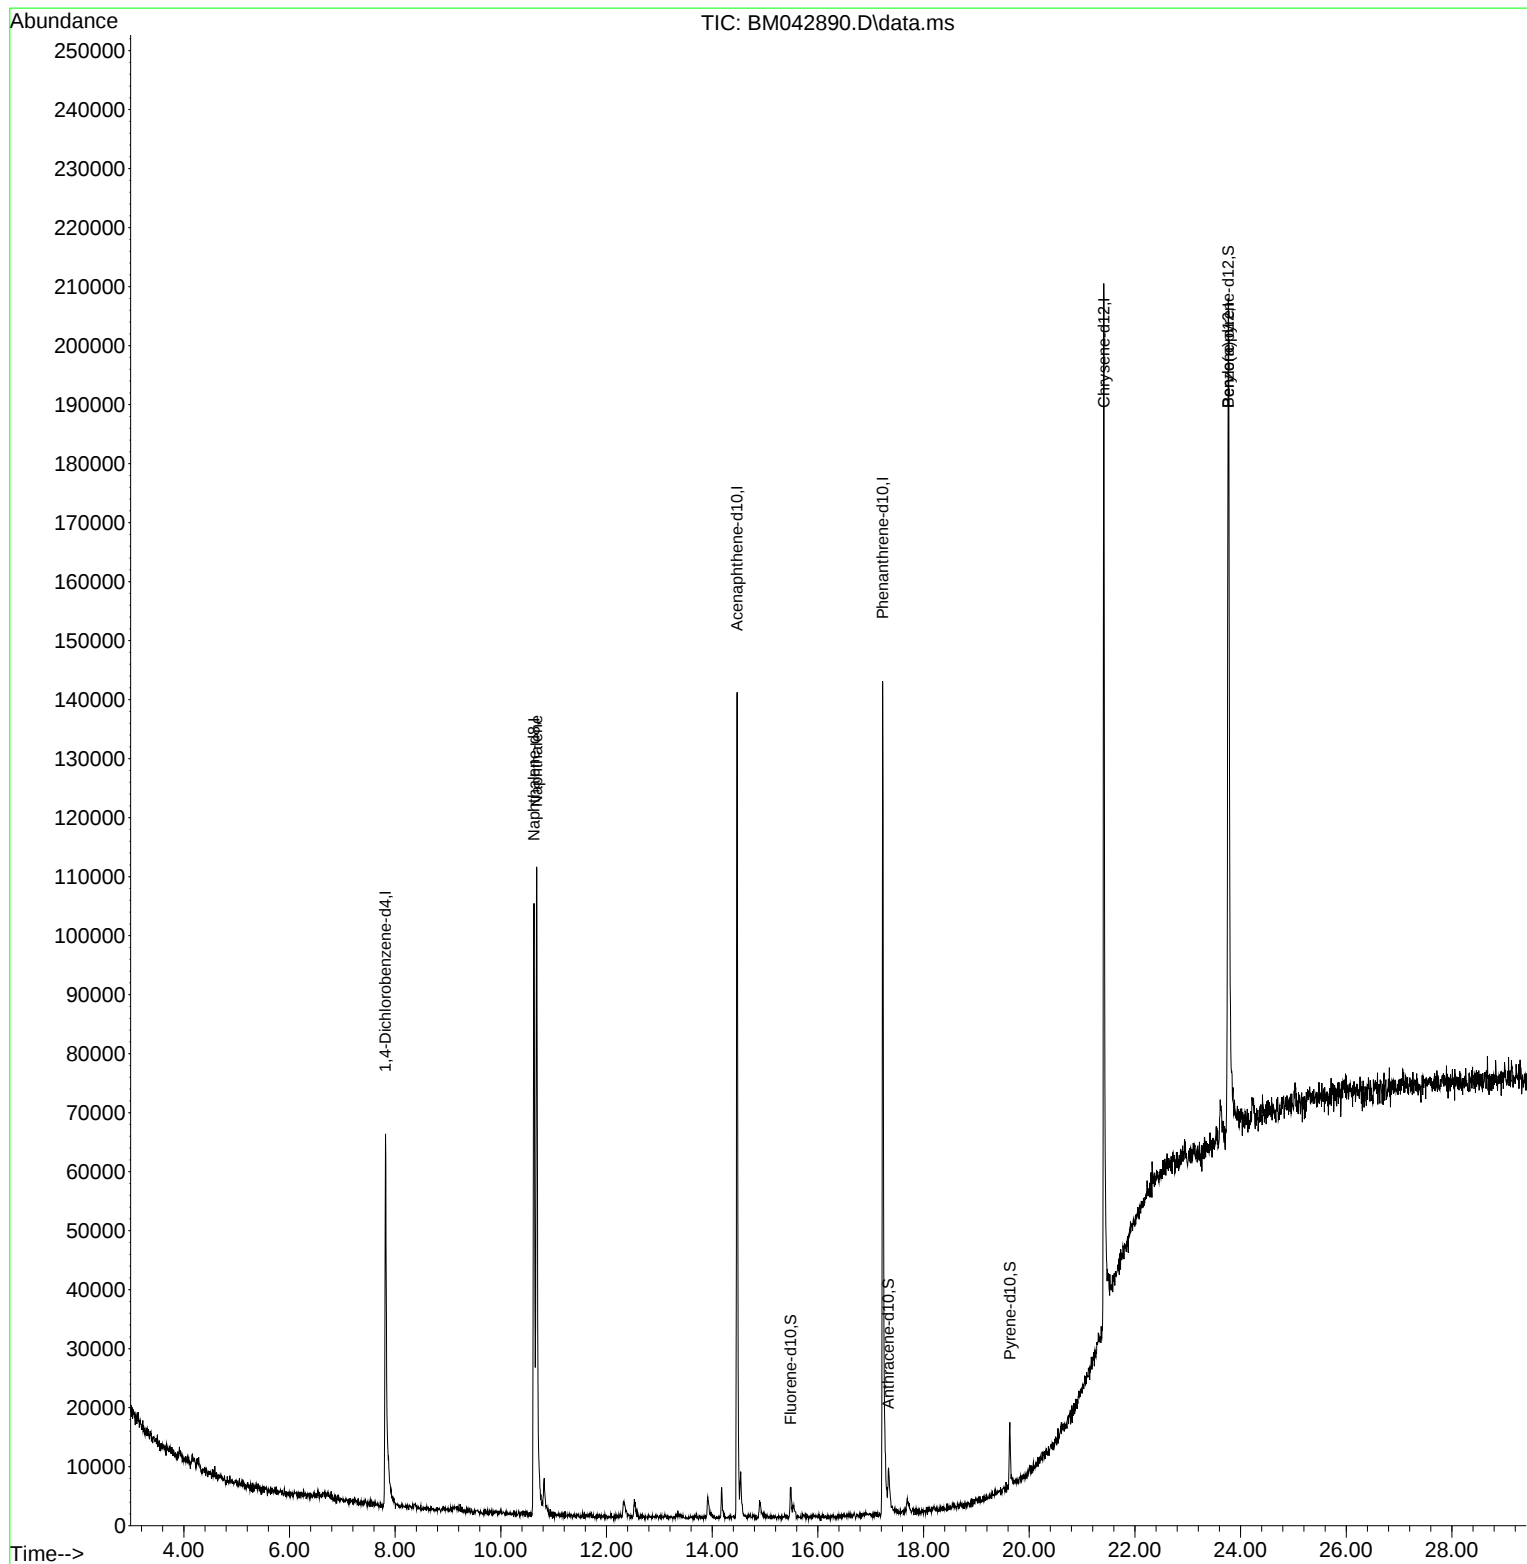

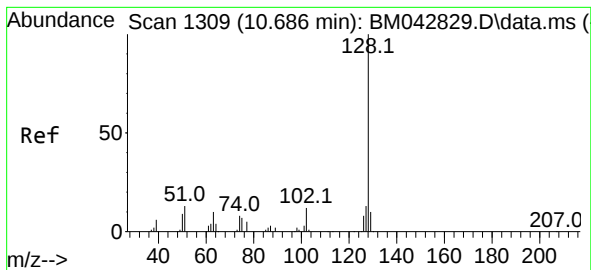

#30
Naphthalene
Concen: 17.662 ng/ul
RT: 10.681 min Scan# 11
Delta R.T. 0.006 min
Lab File: BM042890.D
Acq: 18 Nov 2023 20:21

Instrument :
BNA_M
ClientSampleId :

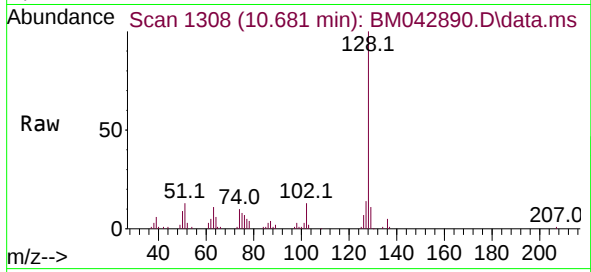

Tgt Ion:128 Resp: 79933
Ion Ratio Lower Upper
128 100
129 11.4 8.6 13.0
127 14.0 10.5 15.7

