

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028726.D
 Acq On : 18 Nov 2023 06:55
 Operator : MA/JU
 Sample : 05369-05
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Nov 18 22:59:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.749	152	2476	0.400	ng/ul	#-0.05
4) Naphthalene-d8	10.479	136	13504	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.325	164	10218	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.09
17) Chrysene-d12	21.301	240	14199	0.400	ng/ul	# 0.00
23) Perylene-d12	23.578	264	16977	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.112	96	35775	13.073	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.129	152	4316	0.212	ng/ul	0.02
18) Fluoranthene-d10	19.113	212	27388	0.599	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.470	202	4137	0.066	ng/ul#	1
26) Benzo(a)pyrene	23.420	252	7379	0.123	ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028726.D
Acq On : 18 Nov 2023 06:55
Operator : MA/JU
Sample : 05369-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Nov 18 22:59:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration




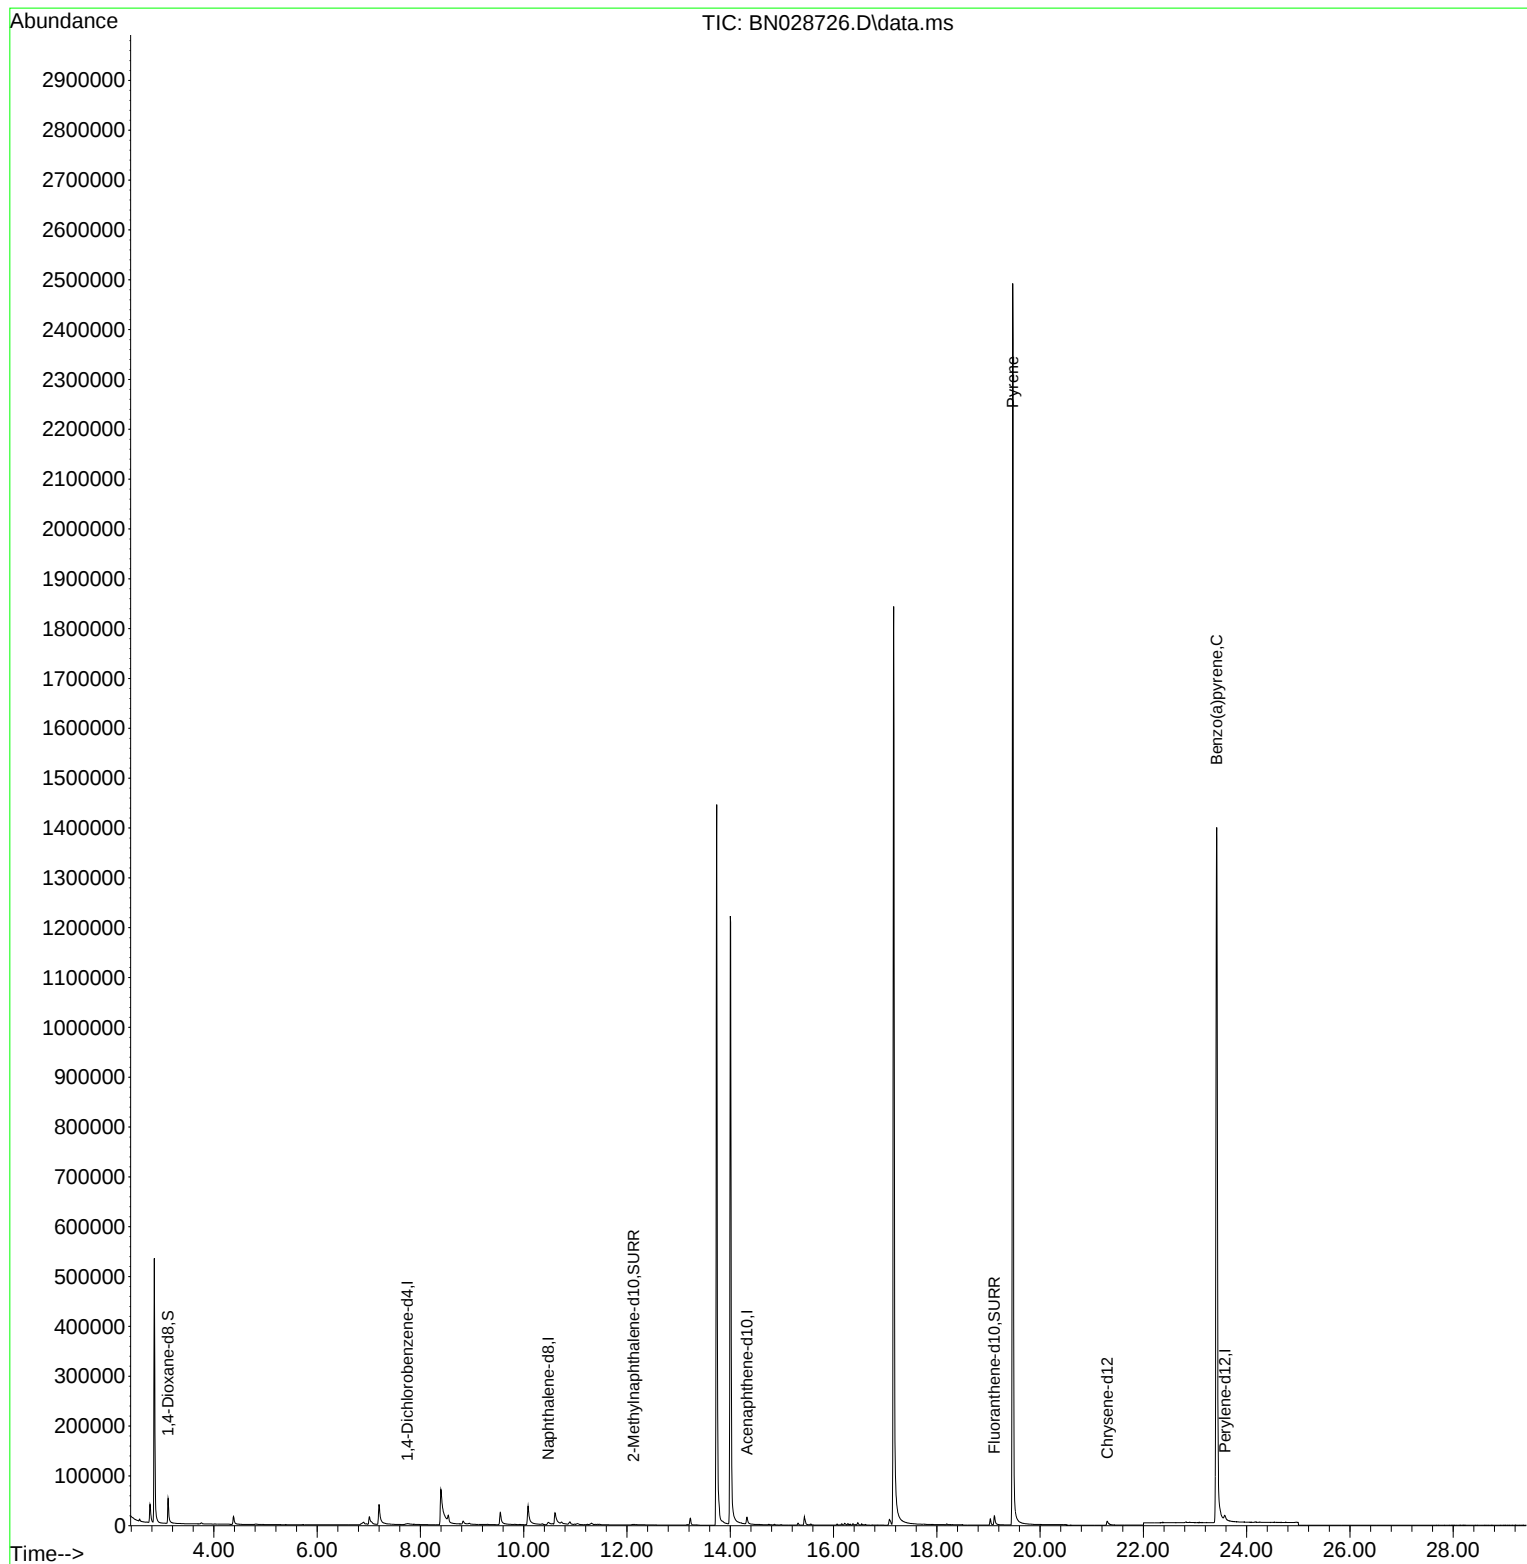


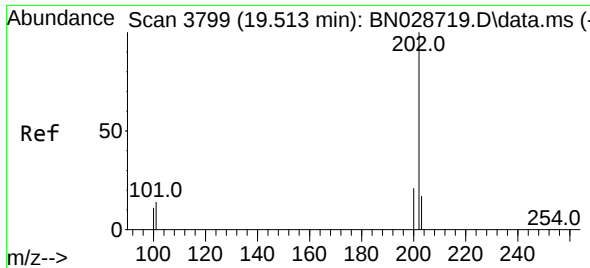

#20
Pyrene
Concen: 0.066 ng/ul
RT: 19.470 min Scan# 31
Delta R.T. -0.042 min
Lab File: BN028726.D
Acq: 18 Nov 2023 06:55

Instrument :
BNA_M
ClientSampleId :

Tgt Ion:202 Resp: 4137
Ion Ratio Lower Upper
202 100
101 153.8 10.3 15.5#
100 1149.7 8.2 12.2#

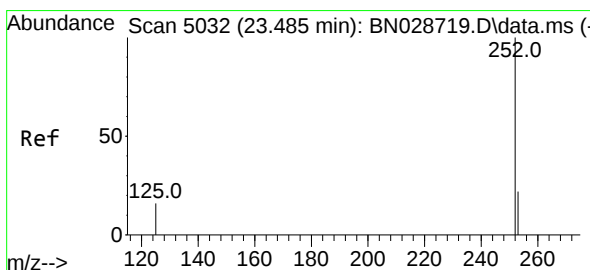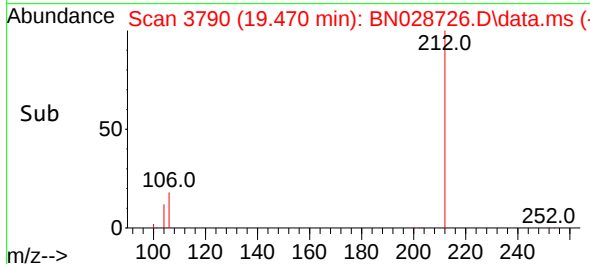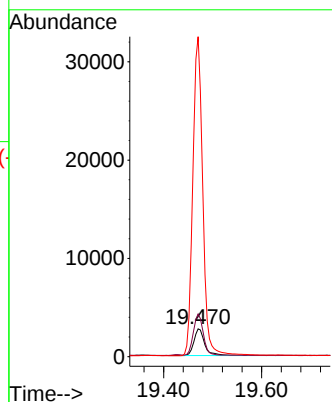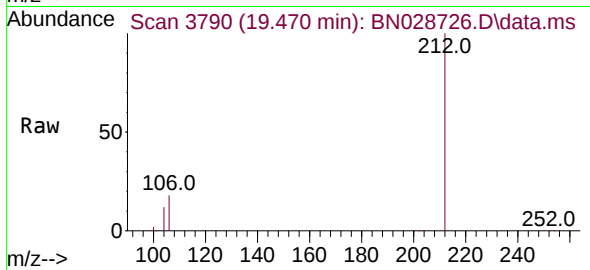

#26
Benzo(a)pyrene
Concen: 0.123 ng/ul
RT: 23.420 min Scan# 5010
Delta R.T. -0.061 min
Lab File: BN028726.D
Acq: 18 Nov 2023 06:55

Tgt Ion:252 Resp: 7379
Ion Ratio Lower Upper
252 100
253 44.7 19.0 28.6#
125 41.1 13.2 19.8#

