

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028735.D
 Acq On : 18 Nov 2023 12:55
 Operator : MA/JU
 Sample : PB157220BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Nov 18 23:02:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.757	152	3416	0.400	ng/ul	#-0.04
4) Naphthalene-d8	10.479	136	17895	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.325	164	13598	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.09
17) Chrysene-d12	21.316	240	14099	0.400	ng/ul	# 0.02
23) Perylene-d12	23.575	264	22239	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.112	96	57278	15.171	ng/ul	0.00
6) 2-Methylnaphthalene-d10	0.000	152	0	0.000	ng/ul	
18) Fluoranthene-d10	19.122	212	23128	0.510	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.470	202	3969	0.064	ng/ul#	1
26) Benzo(a)pyrene	23.417	252	7028	0.089	ng/ul#	56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028735.D
Acq On : 18 Nov 2023 12:55
Operator : MA/JU
Sample : PB157220BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Nov 18 23:02:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration




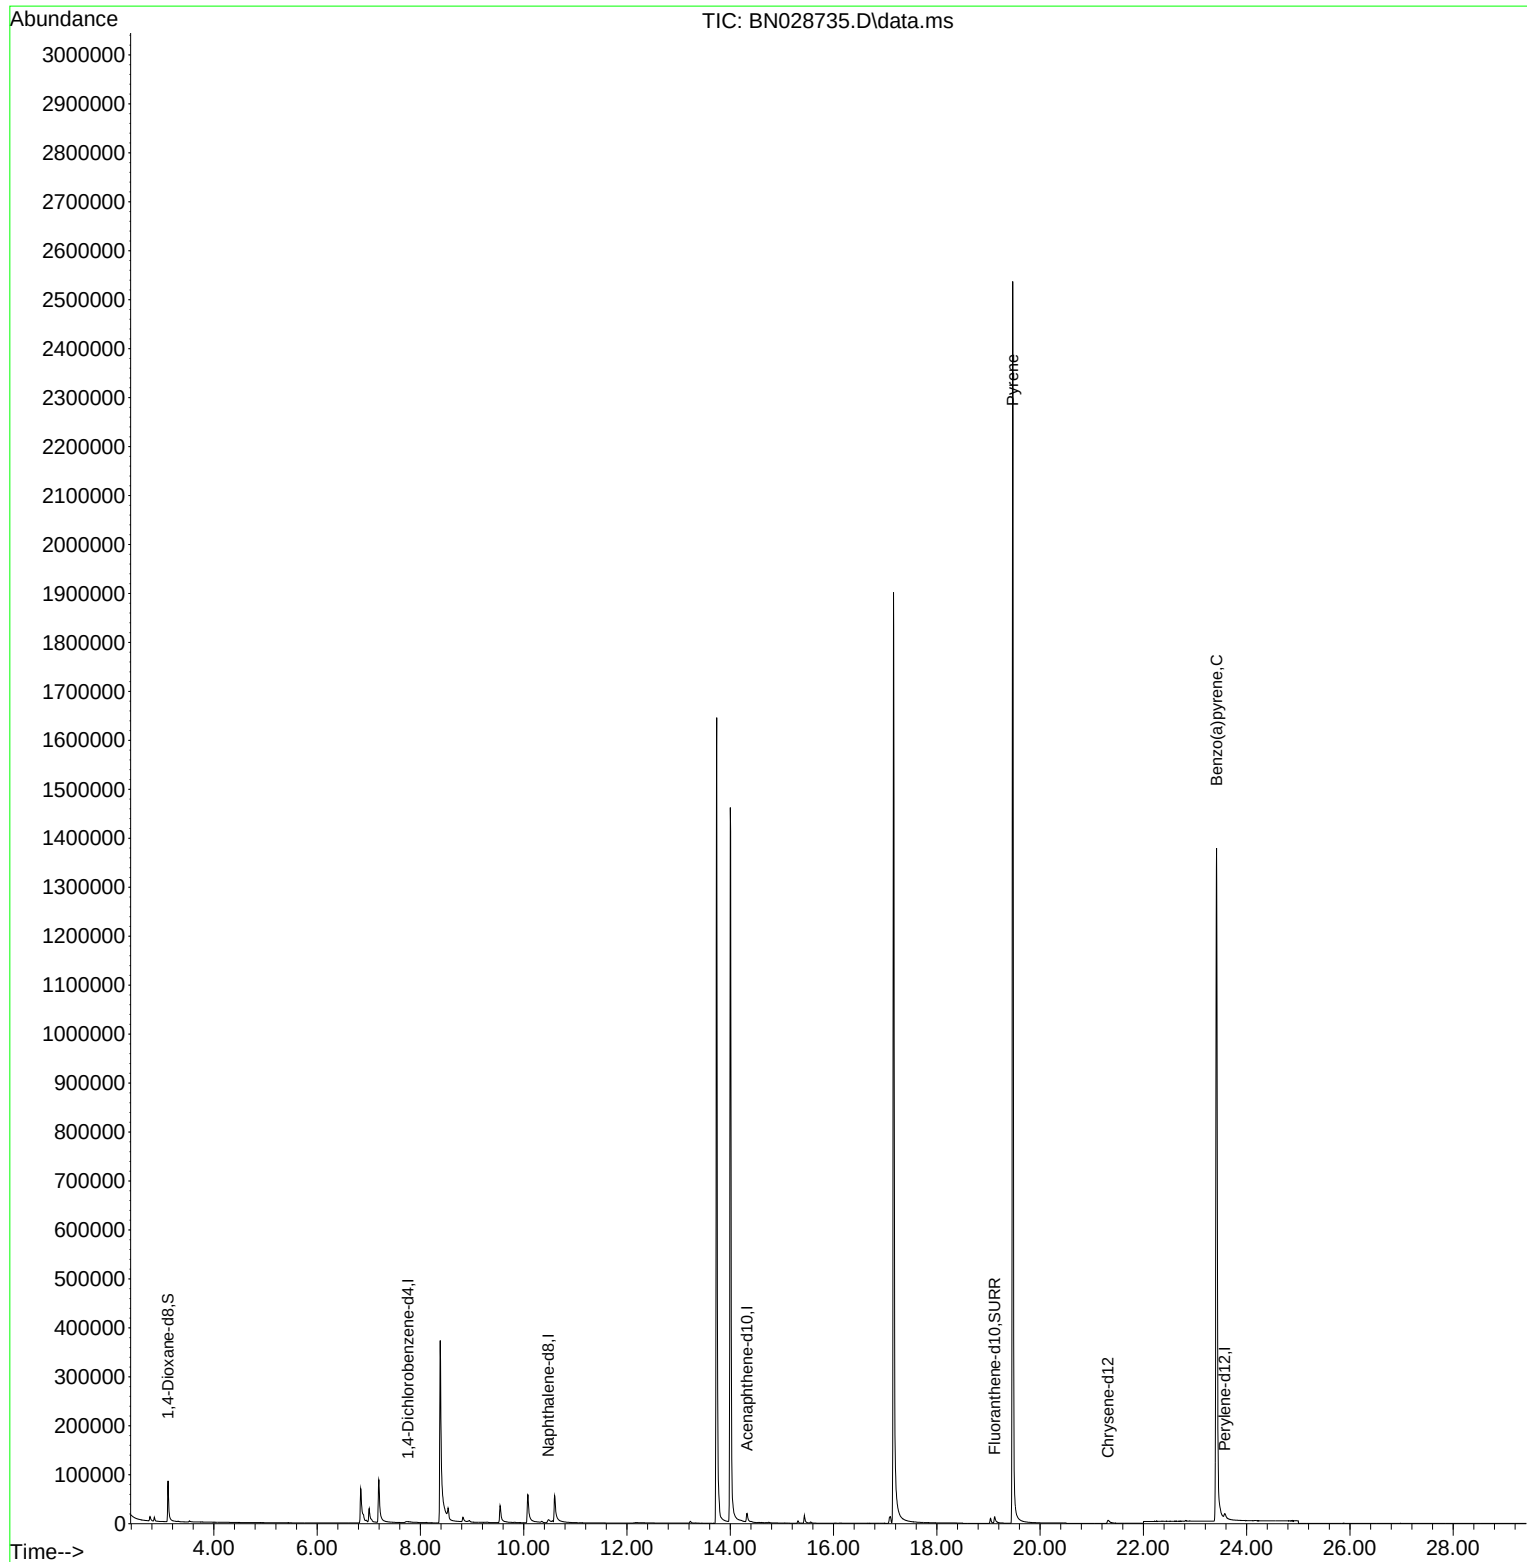


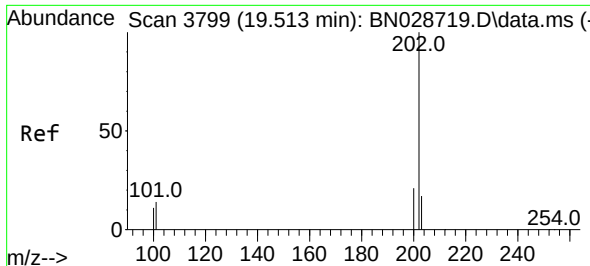

#20
Pyrene
Concen: 0.064 ng/ul
RT: 19.470 min Scan# 31
Delta R.T. -0.042 min
Lab File: BN028735.D
Acq: 18 Nov 2023 12:55

Instrument :
BNA_M
ClientSampleId :

Tgt Ion:202 Resp: 3969
Ion Ratio Lower Upper
202 100
101 163.8 10.3 15.5#
100 1226.0 8.2 12.2#

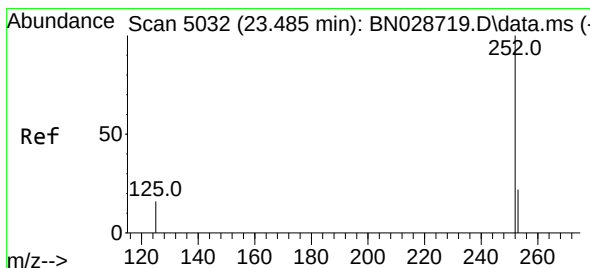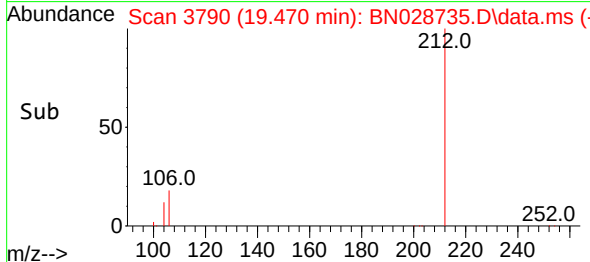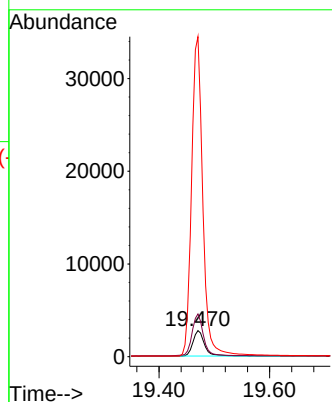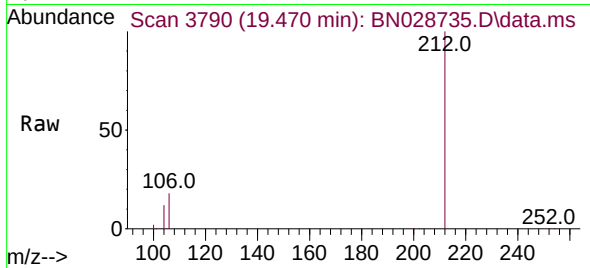

#26
Benzo(a)pyrene
Concen: 0.089 ng/ul
RT: 23.417 min Scan# 5009
Delta R.T. -0.064 min
Lab File: BN028735.D
Acq: 18 Nov 2023 12:55

Tgt Ion:252 Resp: 7028
Ion Ratio Lower Upper
252 100
253 43.4 19.0 28.6#
125 37.6 13.2 19.8#

