

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028736.D
 Acq On : 18 Nov 2023 13:30
 Operator : MA/JU
 Sample : PB157218BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Nov 18 23:02:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.744	152	3933	0.400	ng/ul	#-0.05
4) Naphthalene-d8	10.478	136	20368	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.319	164	15541	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.097	188	30835	0.400	ng/ul	0.00
17) Chrysene-d12	21.314	240	17651	0.400	ng/ul	# 0.02
23) Perylene-d12	23.576	264	26533	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.112	96	55961	12.874	ng/ul	0.00
6) 2-Methylnaphthalene-d10	0.000	152	0	0.000	ng/ul	
18) Fluoranthene-d10	19.120	212	23445	0.413	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.469	202	4032	0.052	ng/ul#	1
26) Benzo(a)pyrene	23.416	252	7324	0.078	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028736.D
Acq On : 18 Nov 2023 13:30
Operator : MA/JU
Sample : PB157218BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Nov 18 23:02:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration




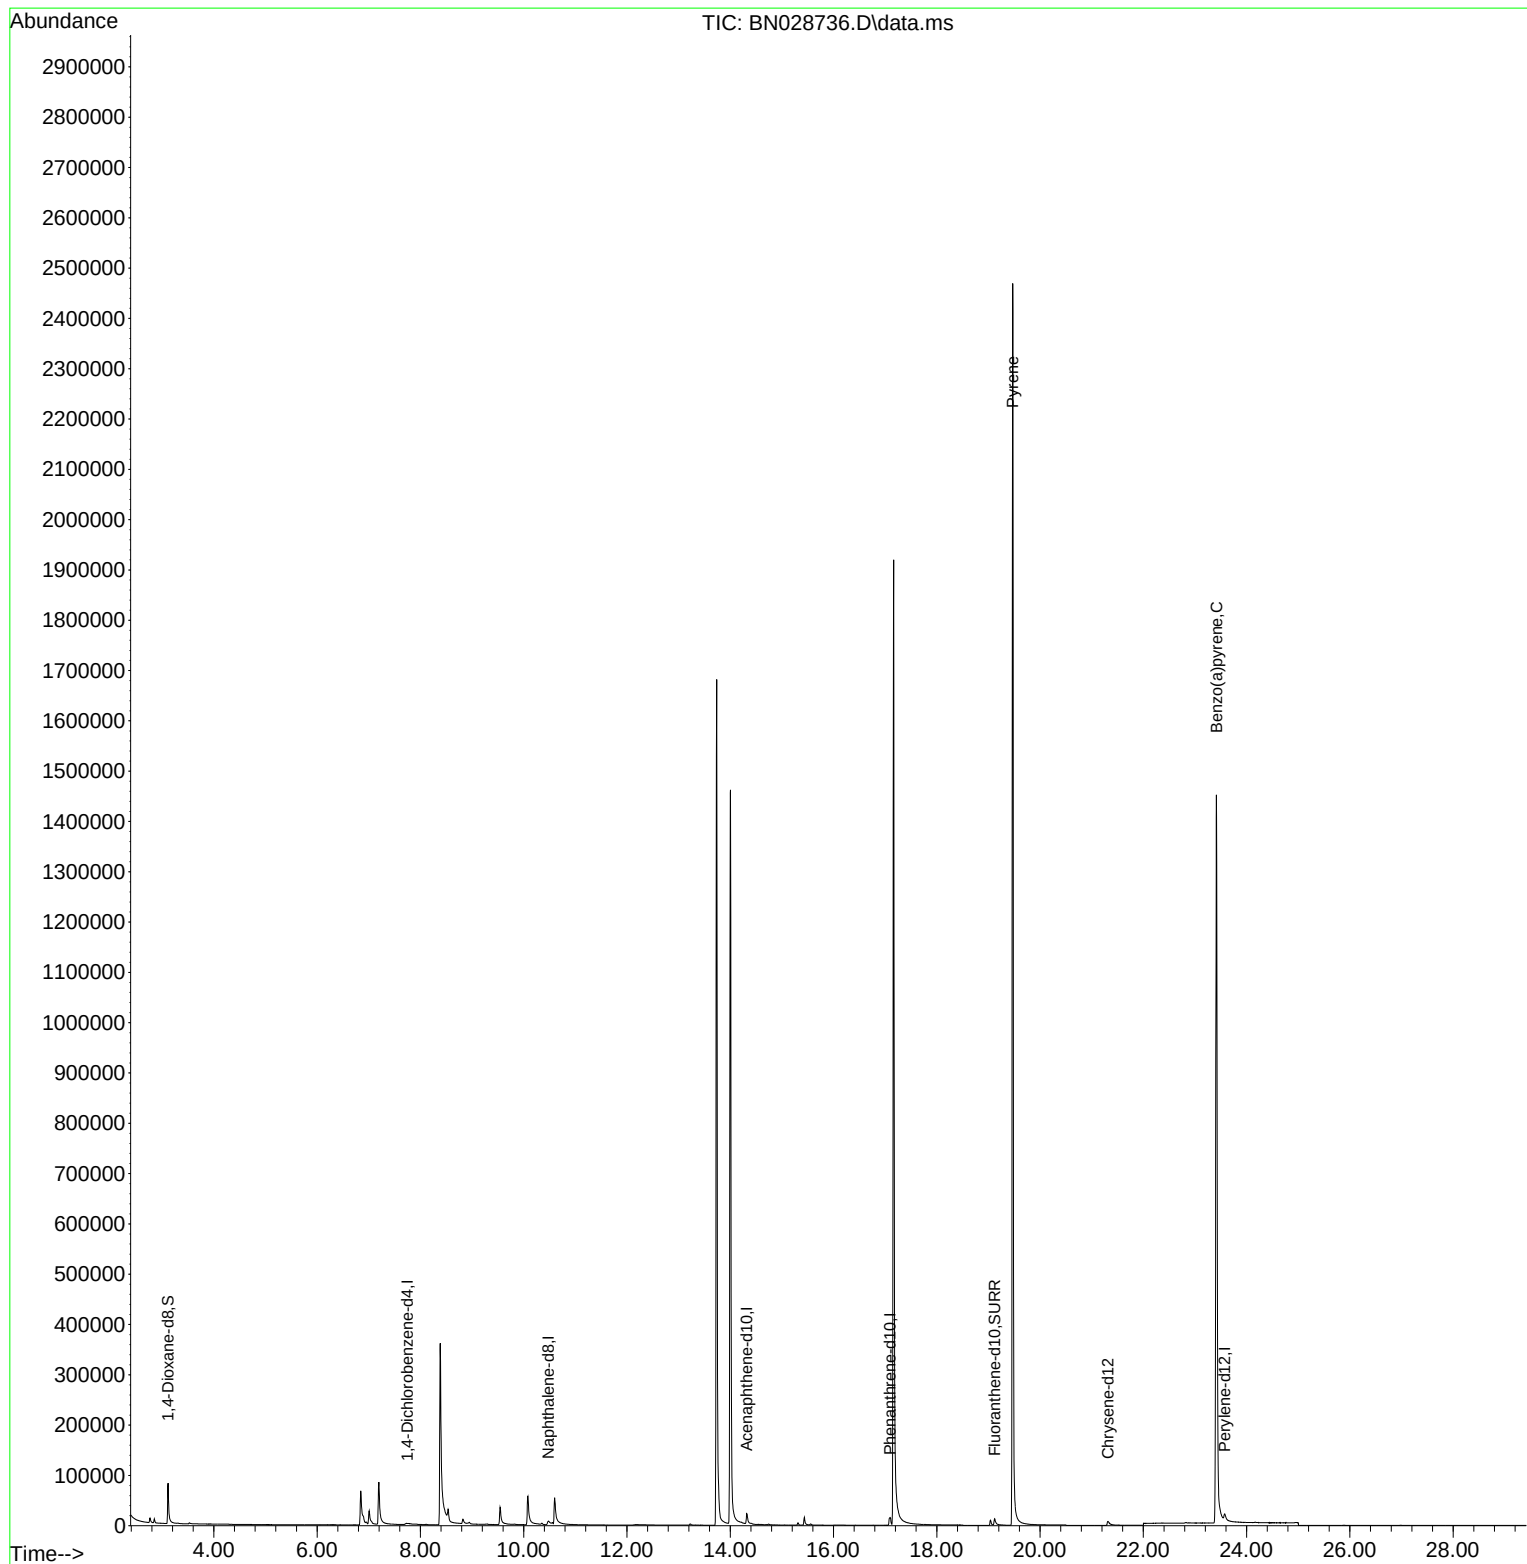


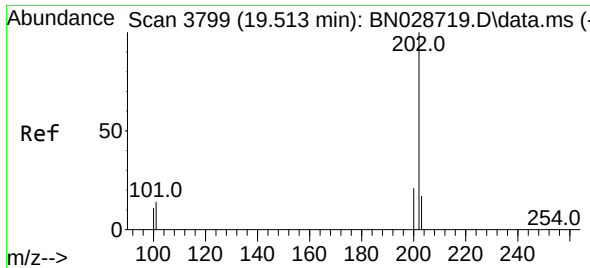

#20
Pyrene
Concen: 0.052 ng/ul
RT: 19.469 min Scan# 31
Delta R.T. -0.043 min
Lab File: BN028736.D
Acq: 18 Nov 2023 13:30

Instrument :
BNA_M
ClientSampleId :

Tgt Ion:202 Resp: 4032
Ion Ratio Lower Upper
202 100
101 164.0 10.3 15.5#
100 1253.7 8.2 12.2#

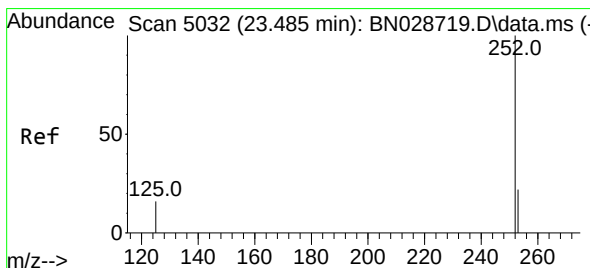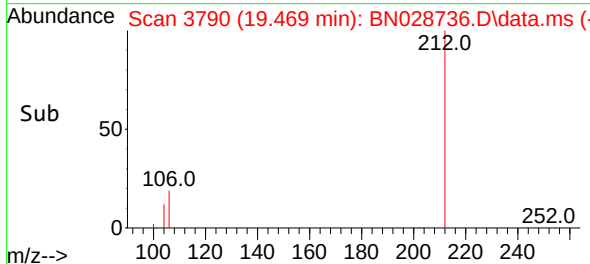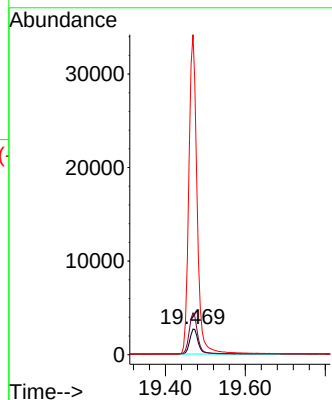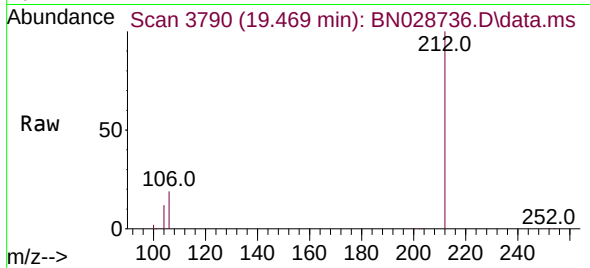

#26
Benzo(a)pyrene
Concen: 0.078 ng/ul
RT: 23.416 min Scan# 5009
Delta R.T. -0.066 min
Lab File: BN028736.D
Acq: 18 Nov 2023 13:30

Tgt Ion:252 Resp: 7324
Ion Ratio Lower Upper
252 100
253 41.8 19.0 28.6#
125 37.4 13.2 19.8#

