

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028738.D
 Acq On : 18 Nov 2023 14:43
 Operator : MA/JU
 Sample : 05369-11
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Nov 18 23:02:38 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.744	152	3256	0.400	ng/ul	#-0.05
4) Naphthalene-d8	10.479	136	16158	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.320	164	12258	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.081	188	23768	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.301	240	14164	0.400	ng/ul	# 0.00
23) Perylene-d12	23.572	264	18705	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.116	96	40576	11.276	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.134	152	4323	0.178	ng/ul	0.02
18) Fluoranthene-d10	19.117	212	26495	0.581	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.470	202	4287	0.069	ng/ul#	1
26) Benzo(a)pyrene	23.417	252	6840	0.103	ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028738.D
Acq On : 18 Nov 2023 14:43
Operator : MA/JU
Sample : 05369-11
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Nov 18 23:02:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration




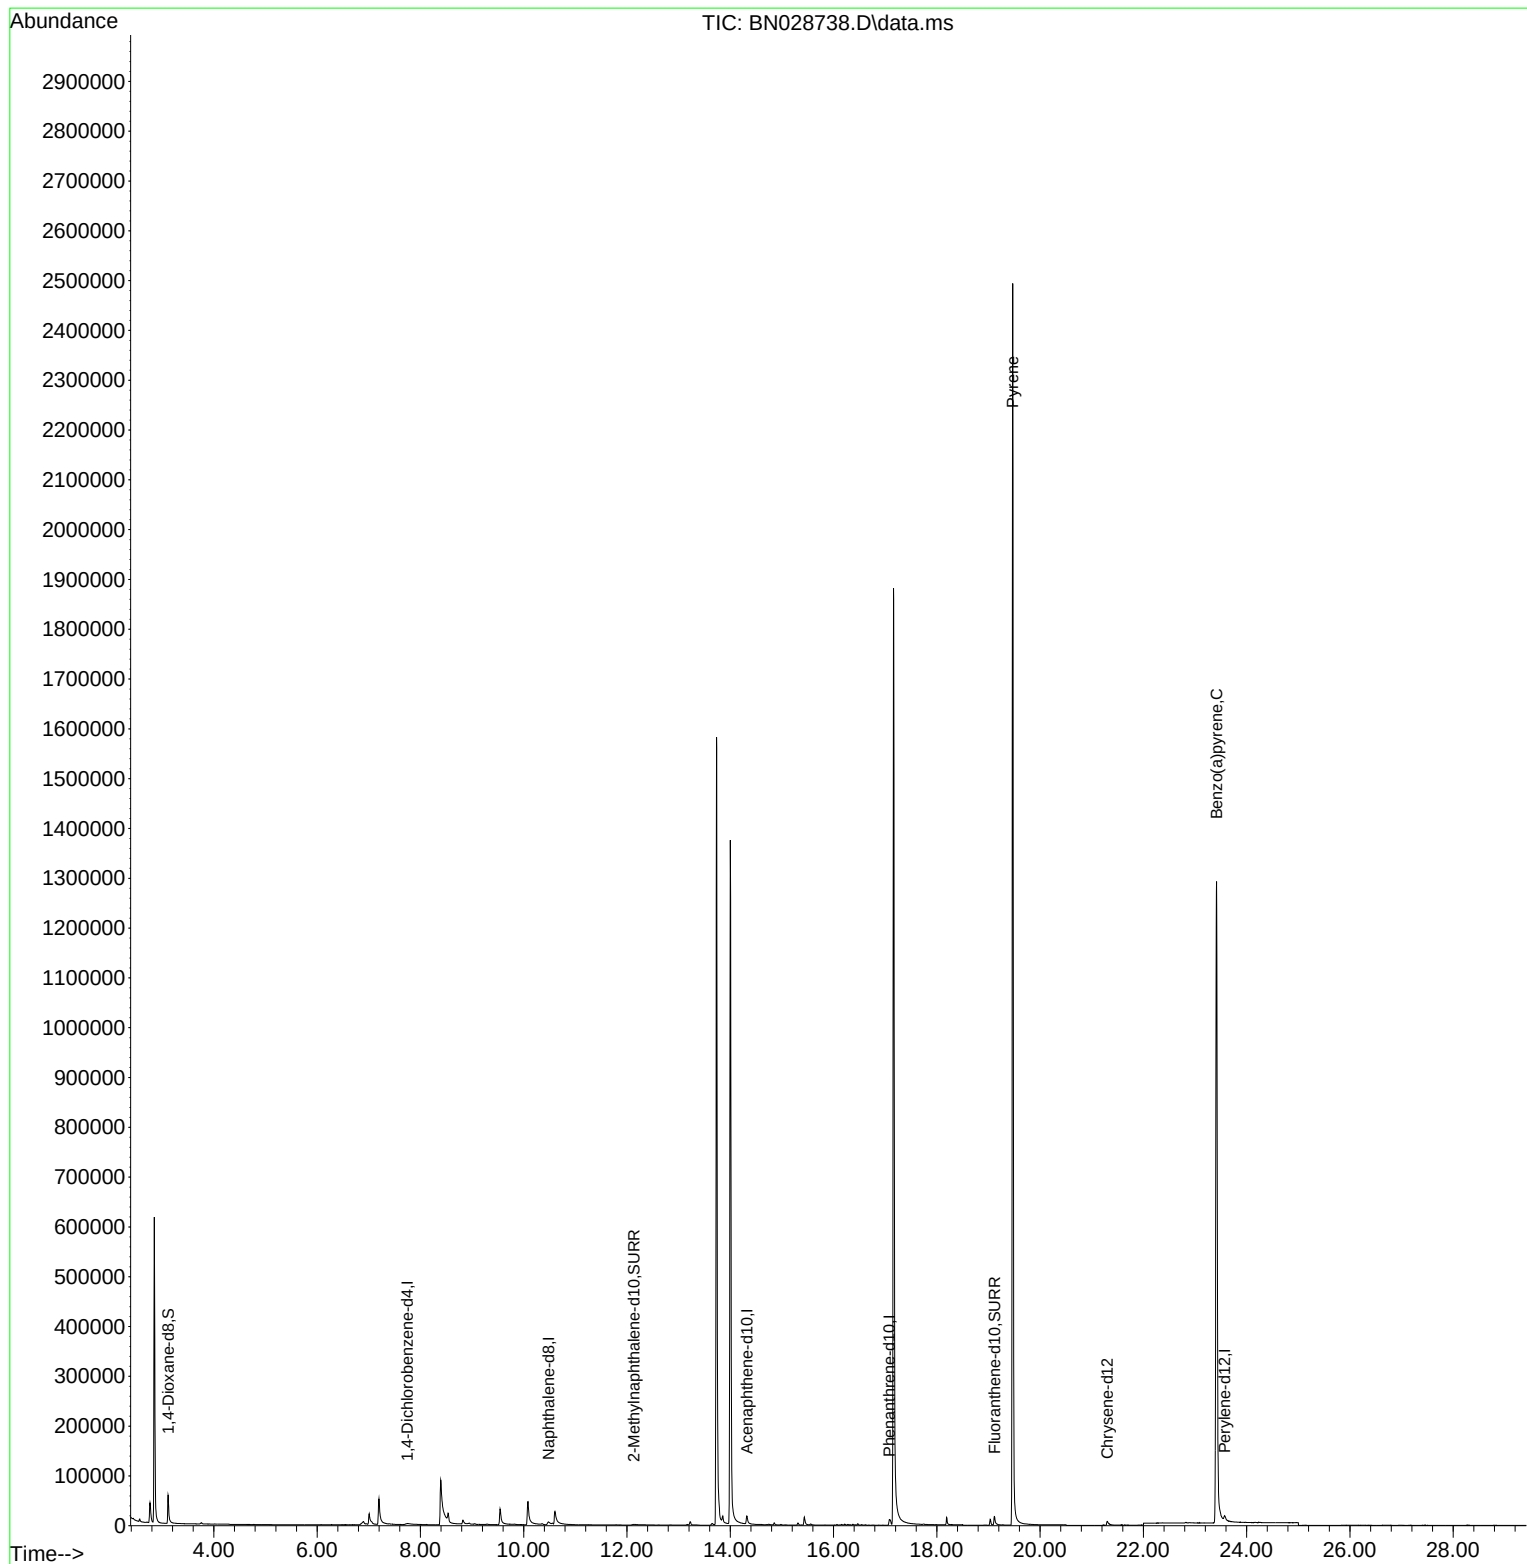


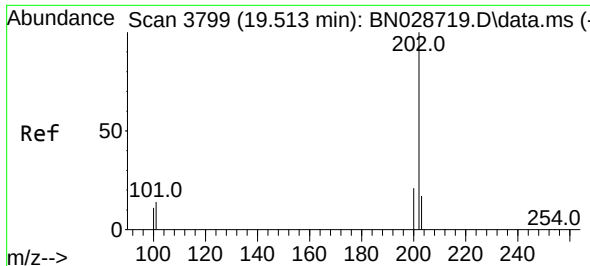

#20
Pyrene
Concen: 0.069 ng/ul
RT: 19.470 min Scan# 31
Delta R.T. -0.042 min
Lab File: BN028738.D
Acq: 18 Nov 2023 14:43

Instrument :
BNA_M
ClientSampleId :

Tgt Ion:202 Resp: 4287
Ion Ratio Lower Upper
202 100
101 153.6 10.3 15.5#
100 1123.6 8.2 12.2#

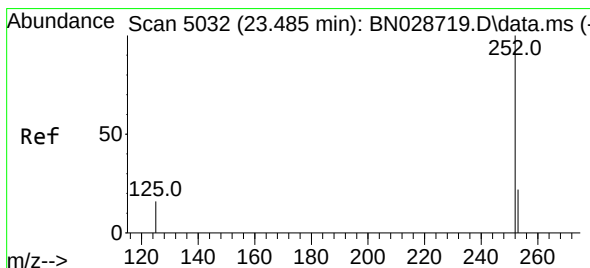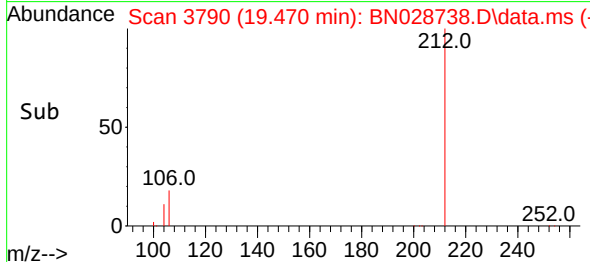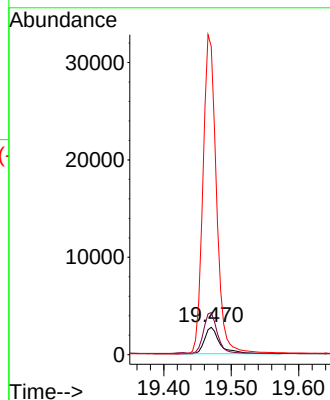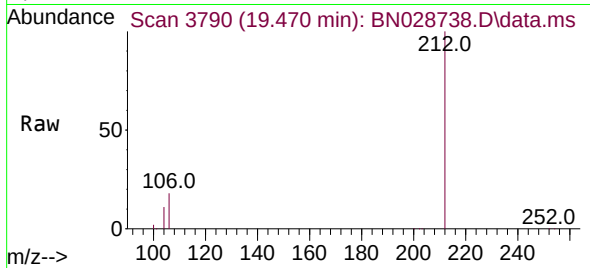

#26
Benzo(a)pyrene
Concen: 0.103 ng/ul
RT: 23.417 min Scan# 5009
Delta R.T. -0.064 min
Lab File: BN028738.D
Acq: 18 Nov 2023 14:43

Tgt Ion:252 Resp: 6840
Ion Ratio Lower Upper
252 100
253 44.4 19.0 28.6#
125 40.7 13.2 19.8#

