

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028742.D
 Acq On : 18 Nov 2023 17:07
 Operator : MA/JU
 Sample : 05369-15
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Nov 18 23:03:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.740	152	3067	0.400	ng/ul	#-0.05
4) Naphthalene-d8	10.473	136	15341	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.320	164	11777	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.09
17) Chrysene-d12	21.304	240	14178	0.400	ng/ul	# 0.00
23) Perylene-d12	23.578	264	18049	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.112	96	44651	13.173	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.134	152	4733	0.205	ng/ul	0.02
18) Fluoranthene-d10	19.117	212	27771	0.609	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.470	202	3980	0.064	ng/ul#	1
26) Benzo(a)pyrene	23.417	252	6969	0.109	ng/ul#	48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028742.D
Acq On : 18 Nov 2023 17:07
Operator : MA/JU
Sample : 05369-15
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Nov 18 23:03:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

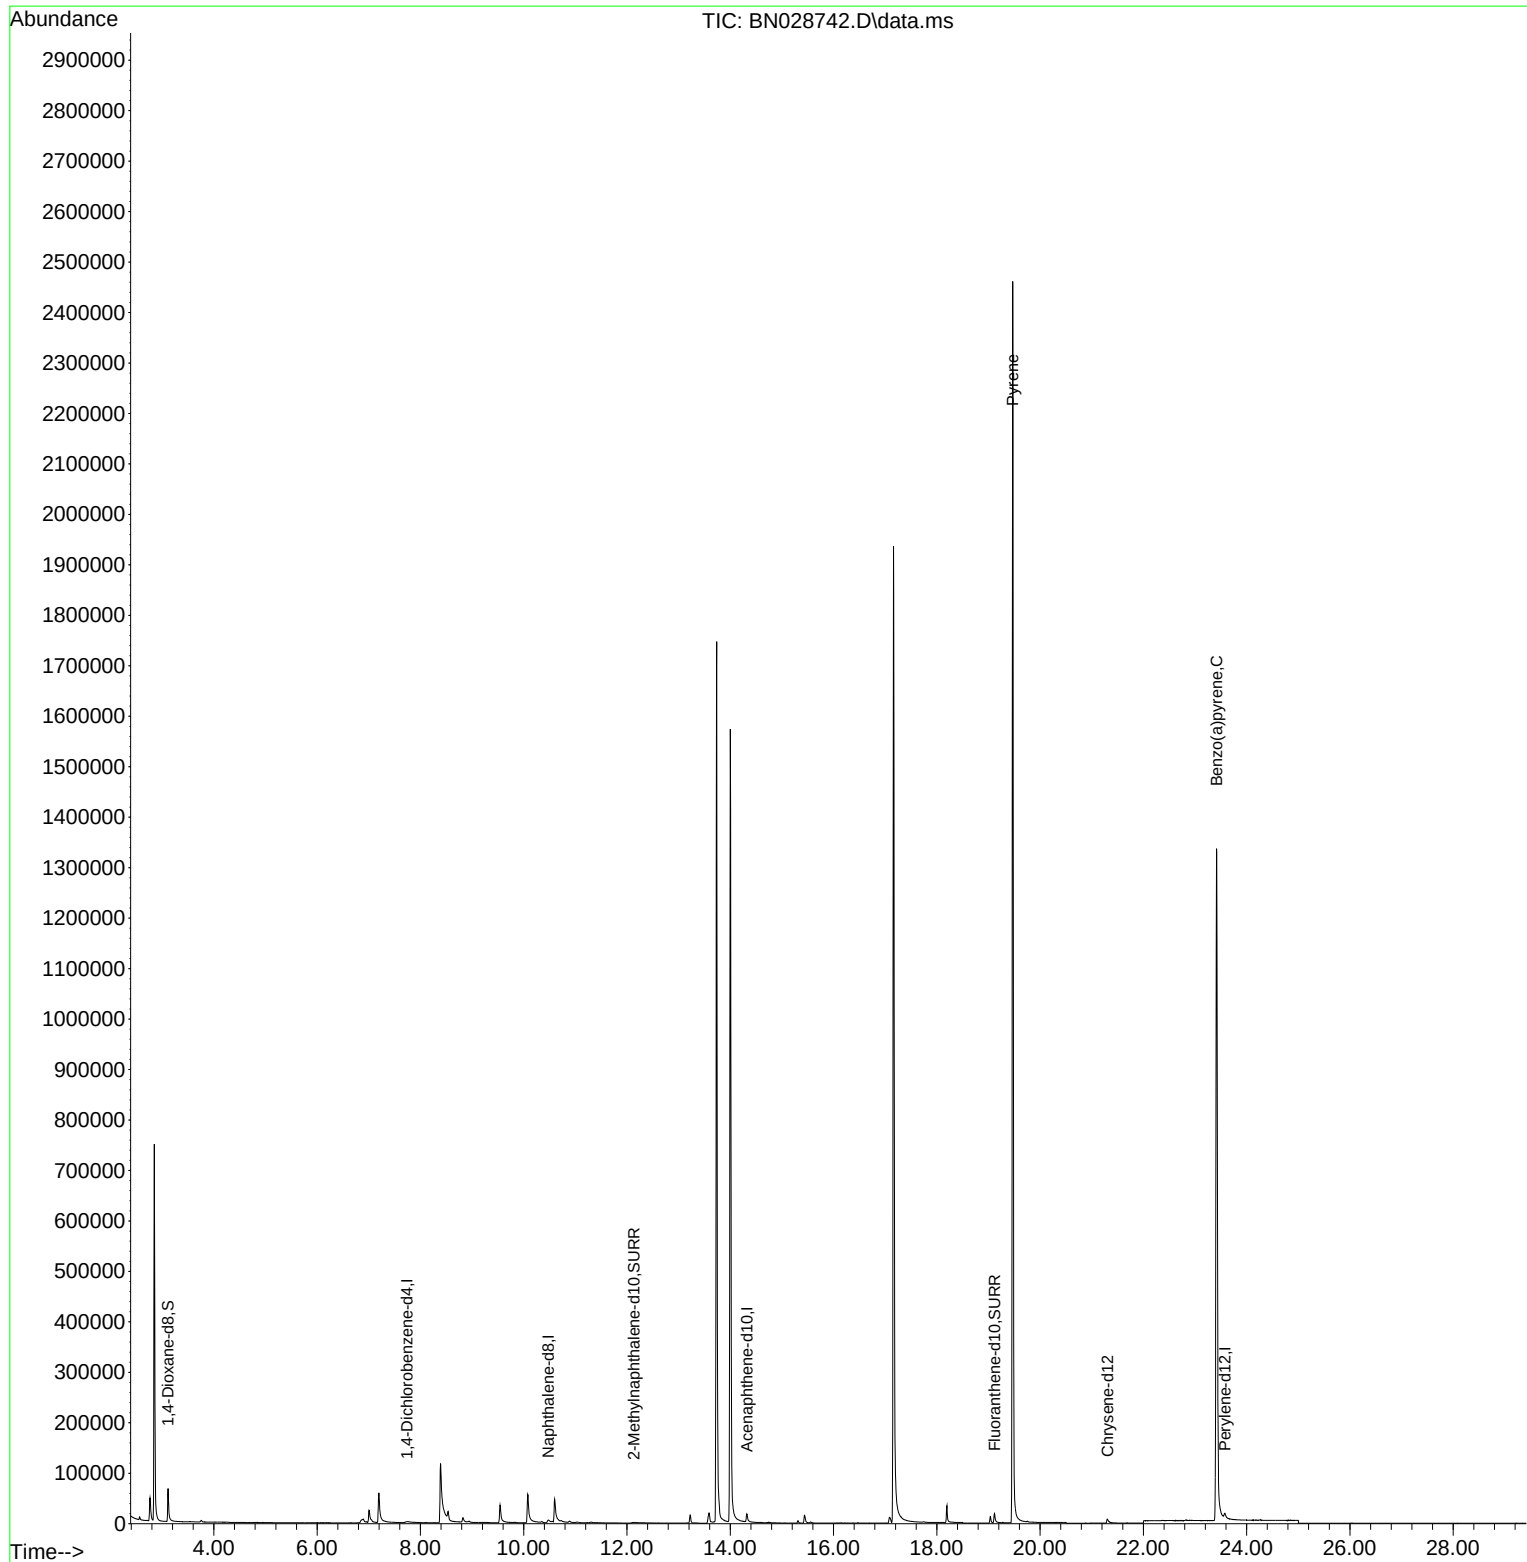

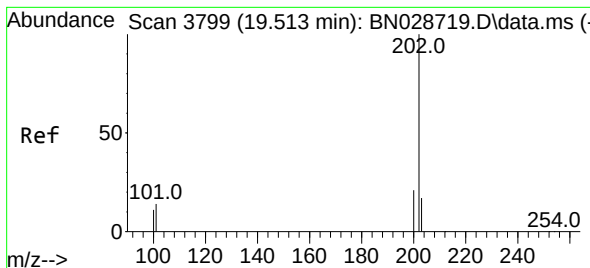

#20

Pyrene

Concen: 0.064 ng/ul

RT: 19.470 min Scan# 31

Delta R.T. -0.042 min

Lab File: BN028742.D

Acq: 18 Nov 2023 17:07





Instrument :

BNA_M

ClientSampleId :

Tgt Ion:202 Resp: 3980

Ion	Ratio	Lower	Upper
202	100		
101	154.5	10.3	15.5#
100	1140.4	8.2	12.2#

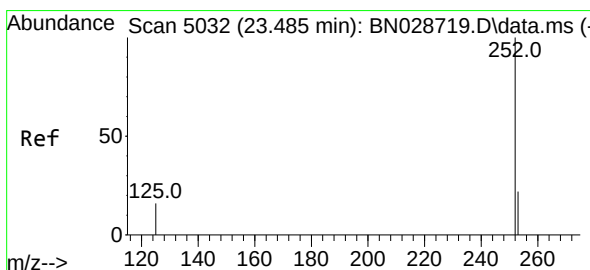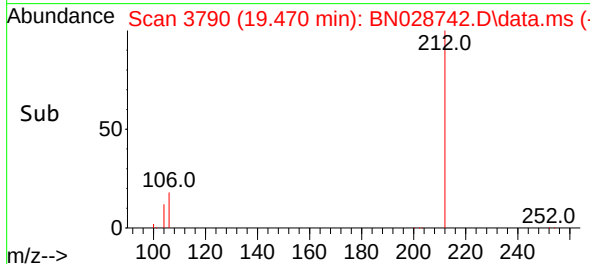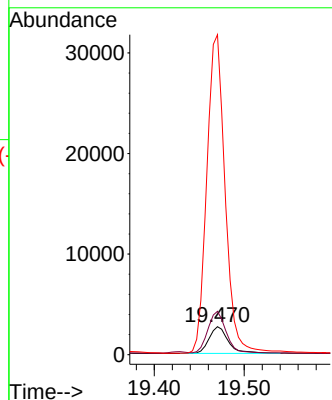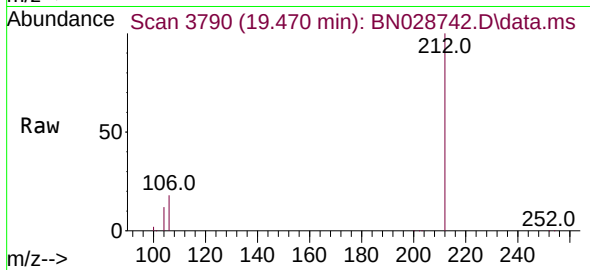

#26

Benzo(a)pyrene

Concen: 0.109 ng/ul

RT: 23.417 min Scan# 5009

Delta R.T. -0.064 min

Lab File: BN028742.D

Acq: 18 Nov 2023 17:07

Tgt Ion:252 Resp: 6969

Ion	Ratio	Lower	Upper
252	100		
253	45.5	19.0	28.6#
125	44.1	13.2	19.8#

