

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028747.D
 Acq On : 18 Nov 2023 20:05
 Operator : MA/JU
 Sample : PB156818BS
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Nov 18 23:04:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.744	152	3551	0.400	ng/ul	#-0.05
4) Naphthalene-d8	10.473	136	18075	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.320	164	13163	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.085	188	25711	0.400	ng/ul	0.00
17) Chrysene-d12	21.310	240	14996	0.400	ng/ul	# 0.01
23) Perylene-d12	23.575	264	20556	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.112	96	44495	11.337	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.151	152	2500	0.092	ng/ul	0.04
18) Fluoranthene-d10	19.117	212	18911	0.392	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.470	202	3086	0.047	ng/ul#	1
26) Benzo(a)pyrene	23.414	252	5295	0.073	ng/ul#	47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028747.D
Acq On : 18 Nov 2023 20:05
Operator : MA/JU
Sample : PB156818BS
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Nov 18 23:04:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

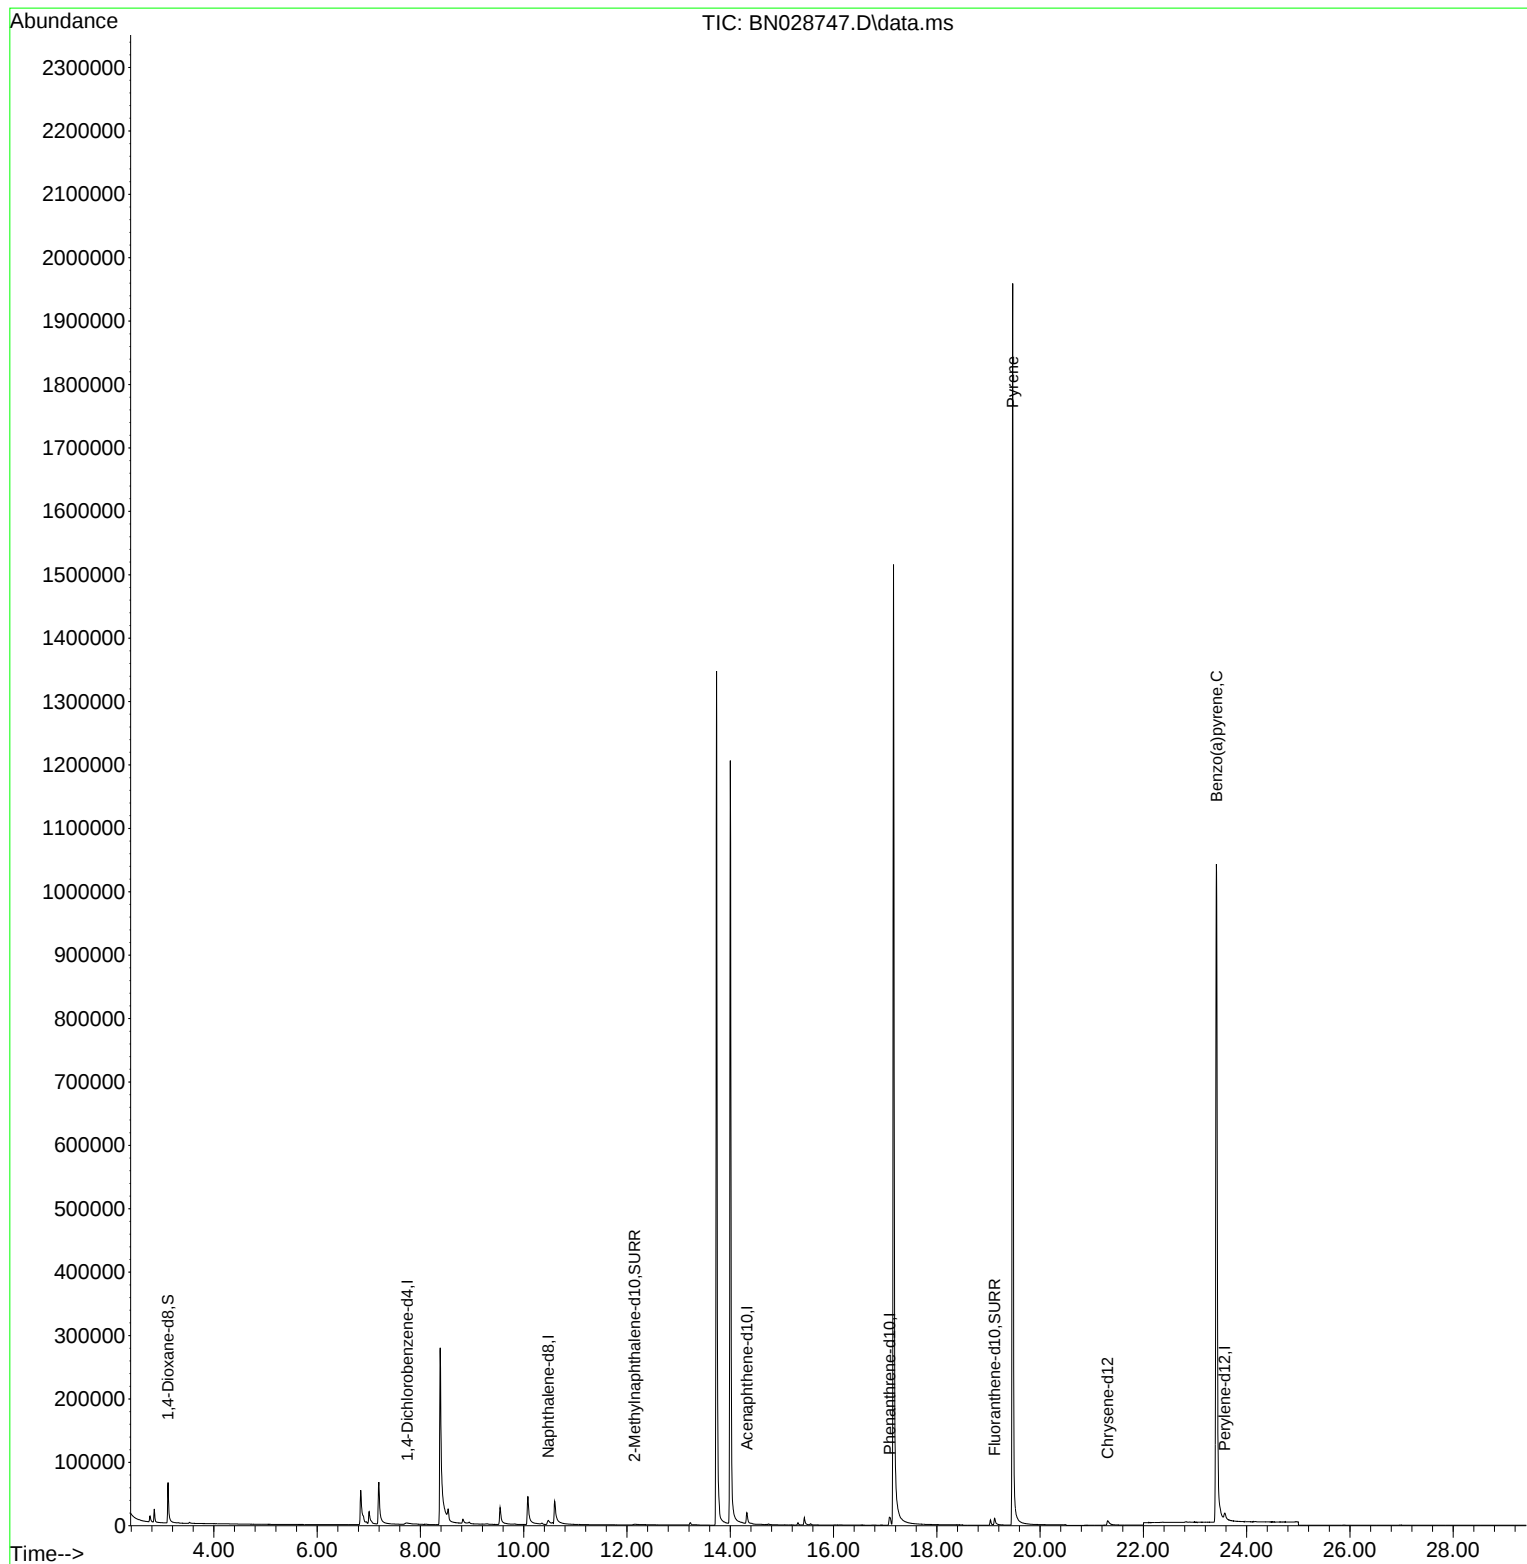



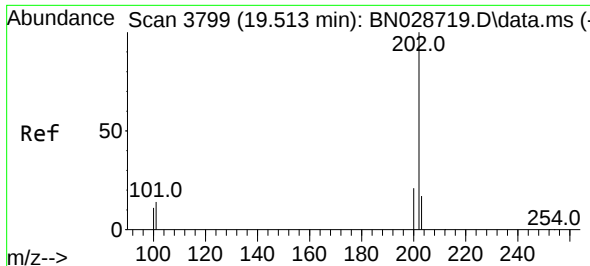


#20
Pyrene
Concen: 0.047 ng/ul
RT: 19.470 min Scan# 31
Delta R.T. -0.042 min
Lab File: BN028747.D
Acq: 18 Nov 2023 20:05

Instrument :
BNA_M
ClientSampleId :

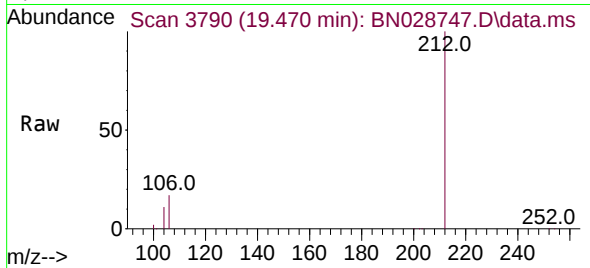

Tgt Ion:202 Resp: 3086
Ion Ratio Lower Upper
202 100
101 152.2 10.3 15.5#
100 1097.3 8.2 12.2#

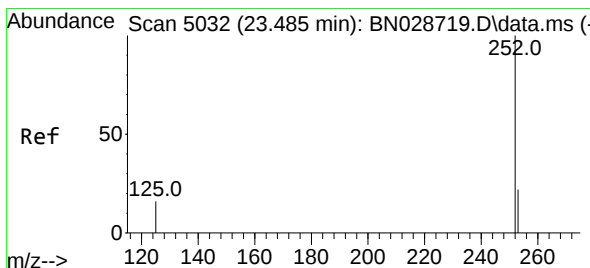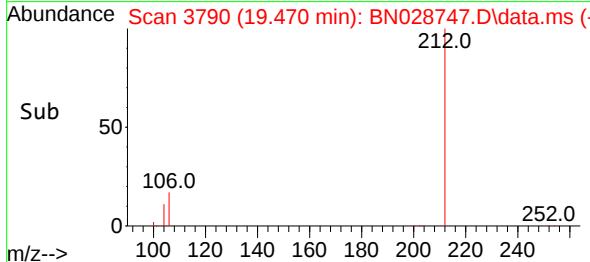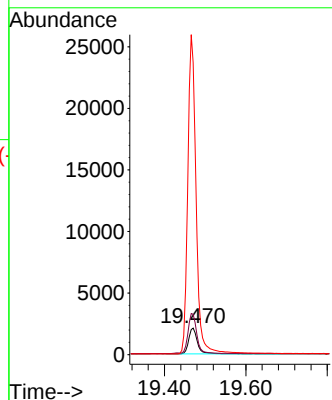

#26
Benzo(a)pyrene
Concen: 0.073 ng/ul
RT: 23.414 min Scan# 5008
Delta R.T. -0.067 min
Lab File: BN028747.D
Acq: 18 Nov 2023 20:05

Tgt Ion:252 Resp: 5295
Ion Ratio Lower Upper
252 100
253 48.0 19.0 28.6#
125 41.9 13.2 19.8#

