




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM111723\  
 Data File : BM042896.D  
 Acq On : 19 Nov 2023 00:35  
 Operator : MA/JU  
 Sample : PB157269BS  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 SLCS269

Manual IntegrationsAPPROVED

Quant Time: Nov 19 03:21:58 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM111323.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Sat Nov 18 22:06:09 2023  
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023  
 Supervised By :mohammad ahmed 11/20/2023

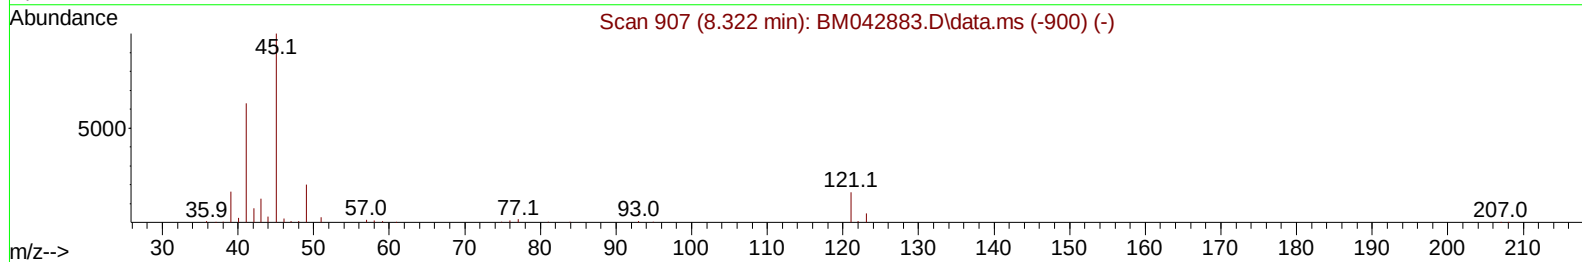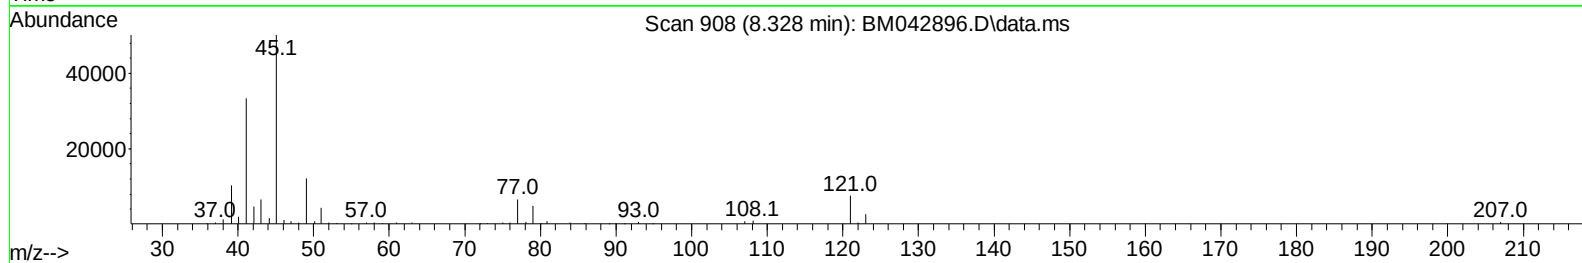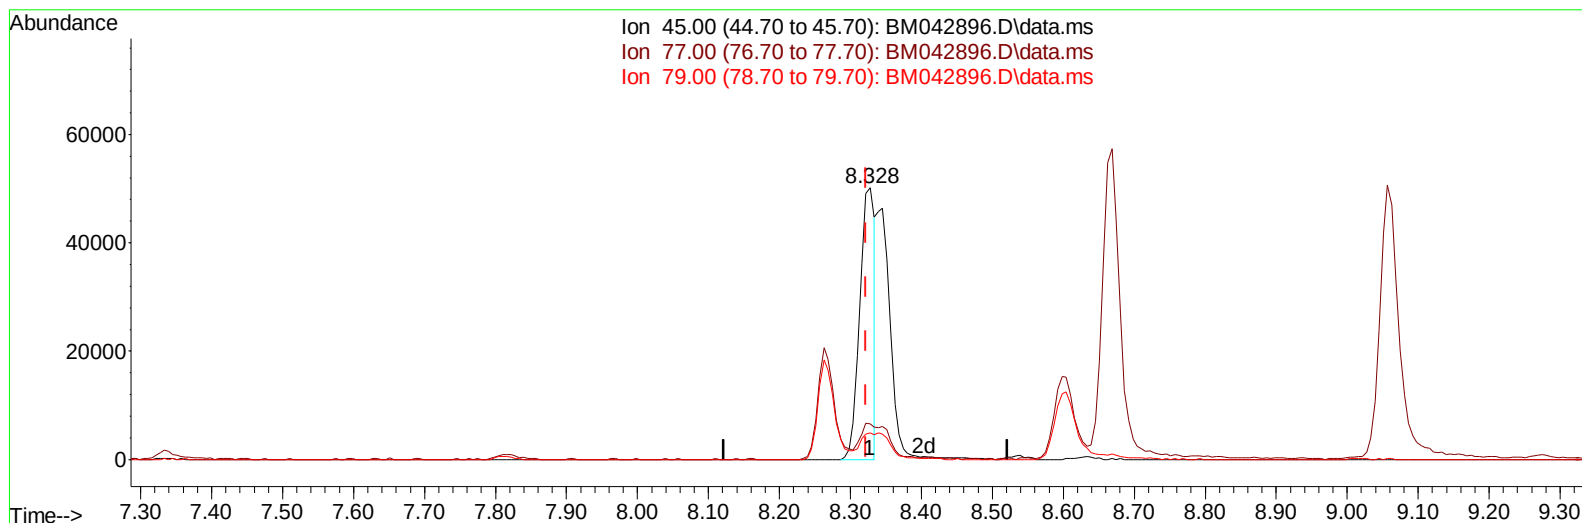

TIC: BM042896.D\data.ms

**(14) 2,2'-oxybis(1-Chloropropane)**

**8.328min (+ 0.006) 20.64 ng/u1**

**response 73512**

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 45.00 | 100.00 | 100.00 |
| 77.00 | 15.20  | 13.20  |
| 79.00 | 10.20  | 9.90   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM111723\  
Data File : BM042896.D  
Acq On : 19 Nov 2023 00:35  
Operator : MA/JU  
Sample : PB157269BS  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SLCS269

Manual IntegrationsAPPROVED

Quant Time: Nov 19 03:21:58 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM111323.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sat Nov 18 22:06:09 2023  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023  
Supervised By :mohammad ahmed 11/20/2023

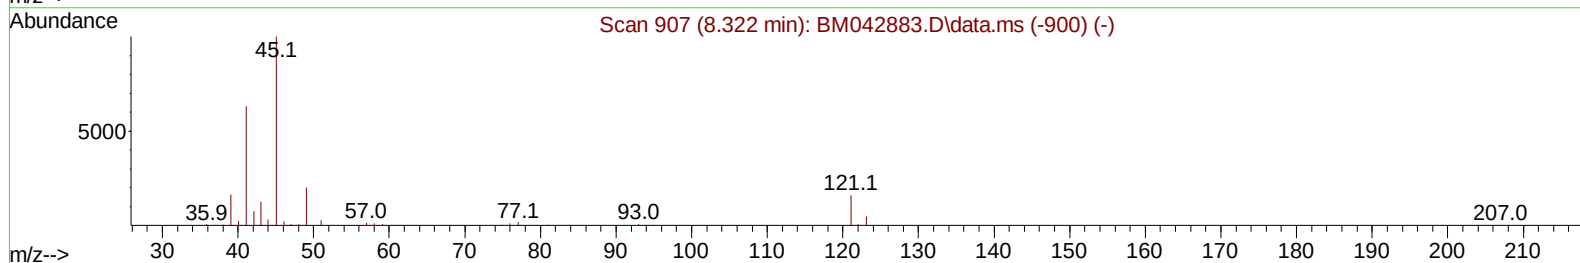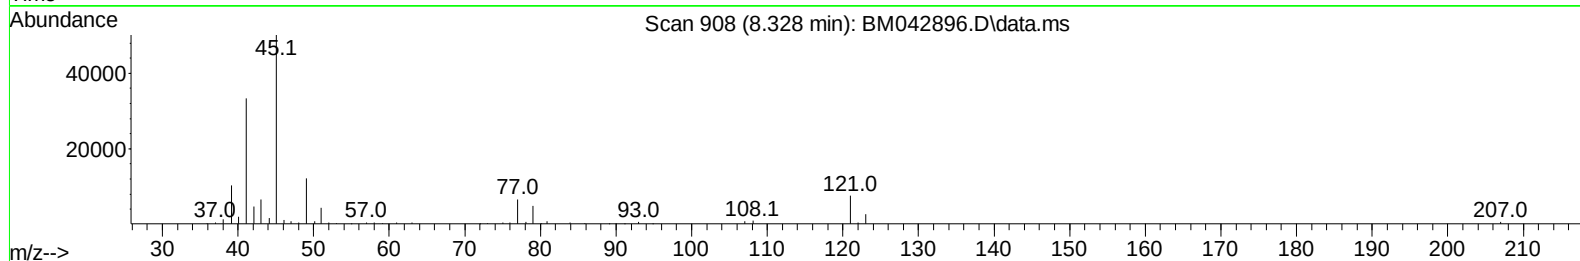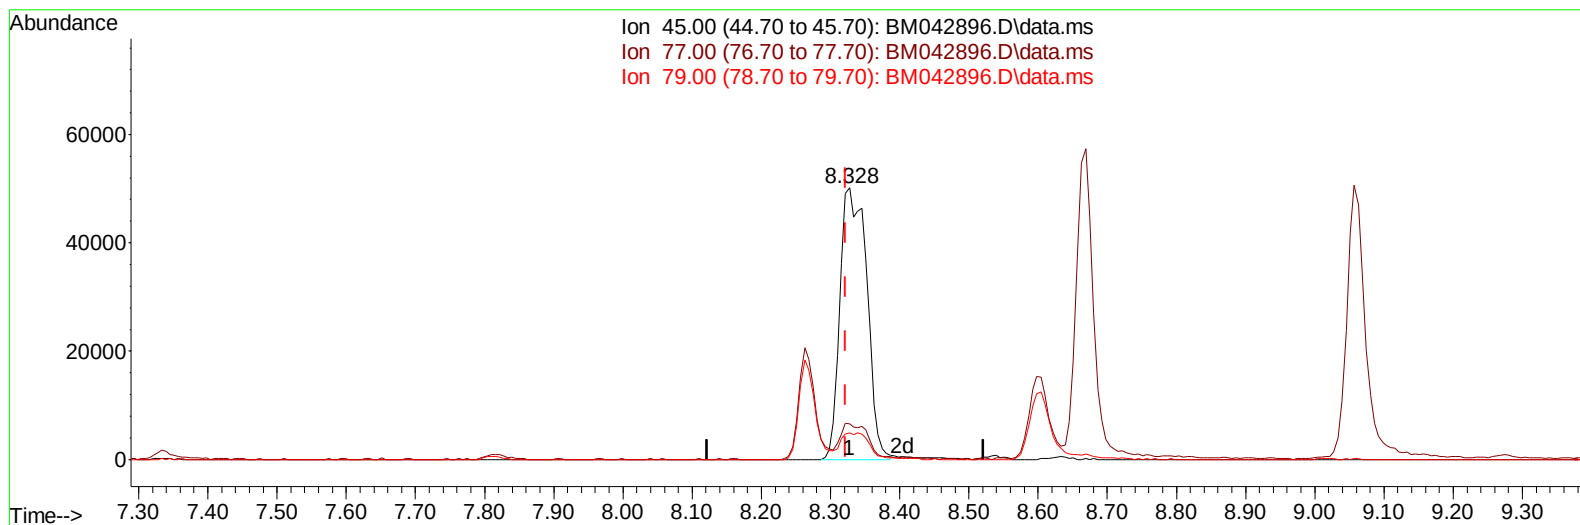

TIC: BM042896.D\data.ms

(14) 2,2'-oxybis(1-Chloropropane)

8.328min (+ 0.006) 37.64 ng/ul m

response 134046

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 45.00 | 100.00 | 100.00 |
| 77.00 | 15.20  | 13.20  |
| 79.00 | 10.20  | 9.90   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM111723\  
 Data File : BM042896.D  
 Acq On : 19 Nov 2023 00:35  
 Operator : MA/JU  
 Sample : PB157269BS  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 SLCS269

Manual IntegrationsAPPROVED

Quant Time: Nov 19 03:21:58 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM111323.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Sat Nov 18 22:06:09 2023  
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023  
 Supervised By :mohammad ahmed 11/20/2023

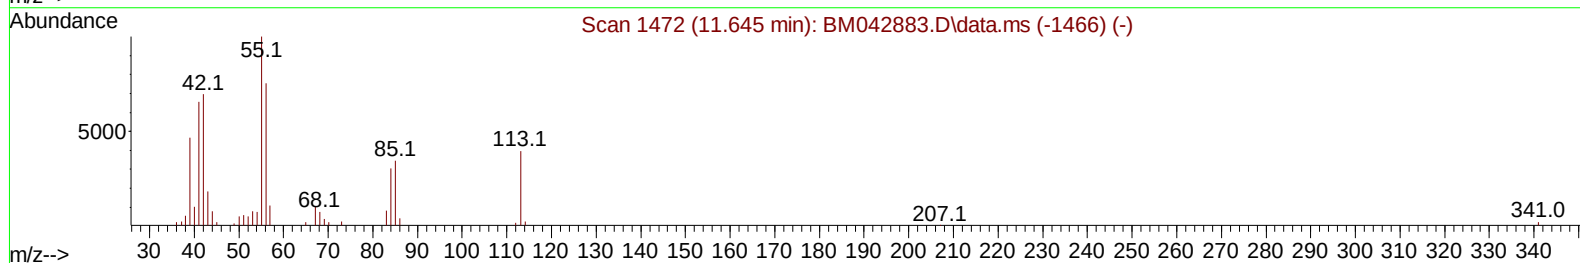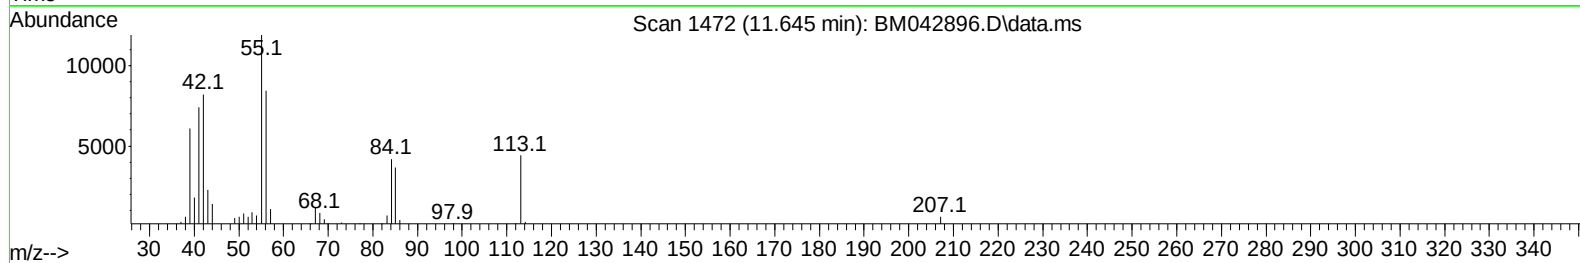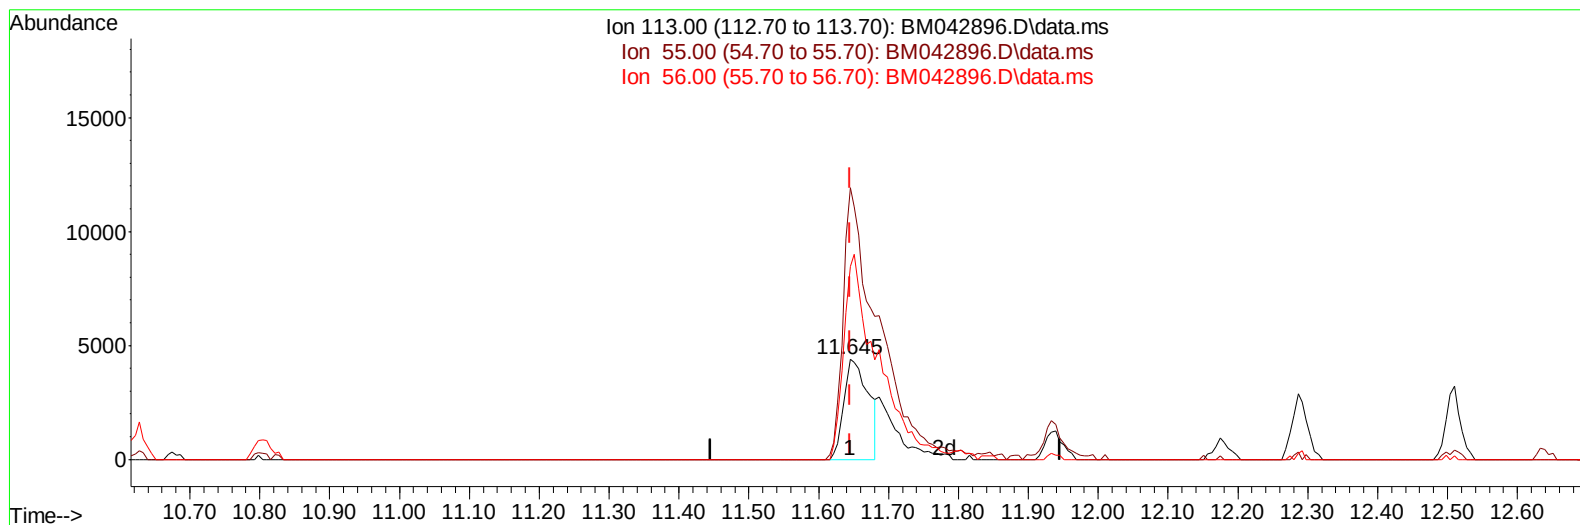

TIC: BM042896.D\data.ms

**(34) Caprolactam**

11.645min (-0.000) 20.97 ng/ul

response 10731

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 113.00 | 100.00 | 100.00 |
| 55.00  | 230.20 | 270.27 |
| 56.00  | 167.90 | 191.99 |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM111723\  
Data File : BM042896.D  
Acq On : 19 Nov 2023 00:35  
Operator : MA/JU  
Sample : PB157269BS  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SLCS269

Manual IntegrationsAPPROVED

Quant Time: Nov 19 03:21:58 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM111323.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sat Nov 18 22:06:09 2023  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023  
Supervised By :mohammad ahmed 11/20/2023

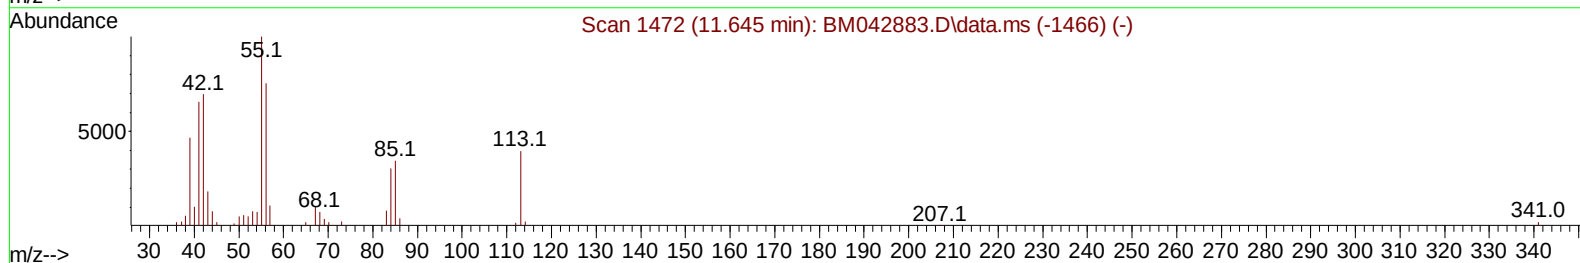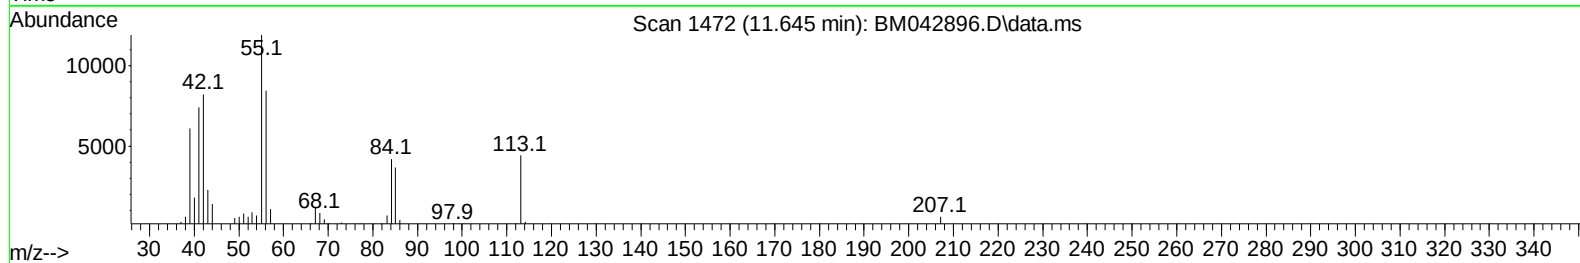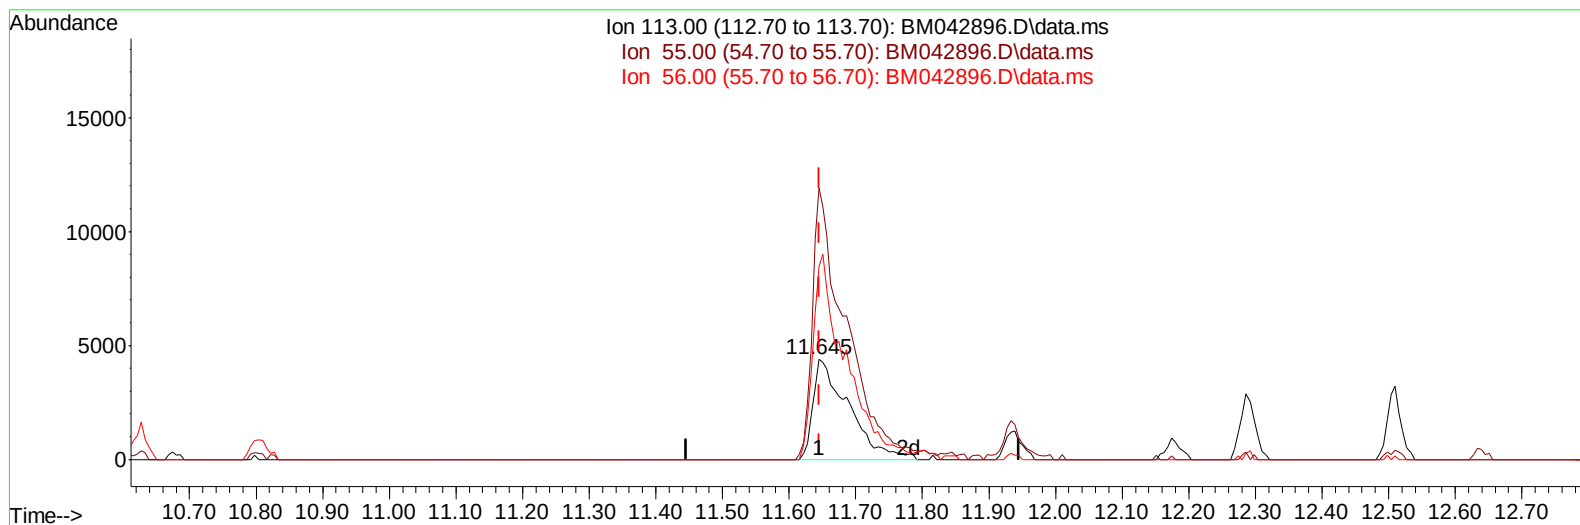

TIC: BM042896.D\data.ms

(34) Caprolactam

11.645min (-0.000) 31.91 ng/ul m

response 16330

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 113.00 | 100.00 | 100.00 |
| 55.00  | 230.20 | 270.27 |
| 56.00  | 167.90 | 191.99 |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM111723\  
 Data File : BM042896.D  
 Acq On : 19 Nov 2023 00:35  
 Operator : MA/JU  
 Sample : PB157269BS  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 SLCS269

Manual IntegrationsAPPROVED

Quant Time: Nov 19 03:21:58 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM111323.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Sat Nov 18 22:06:09 2023  
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023  
 Supervised By :mohammad ahmed 11/20/2023

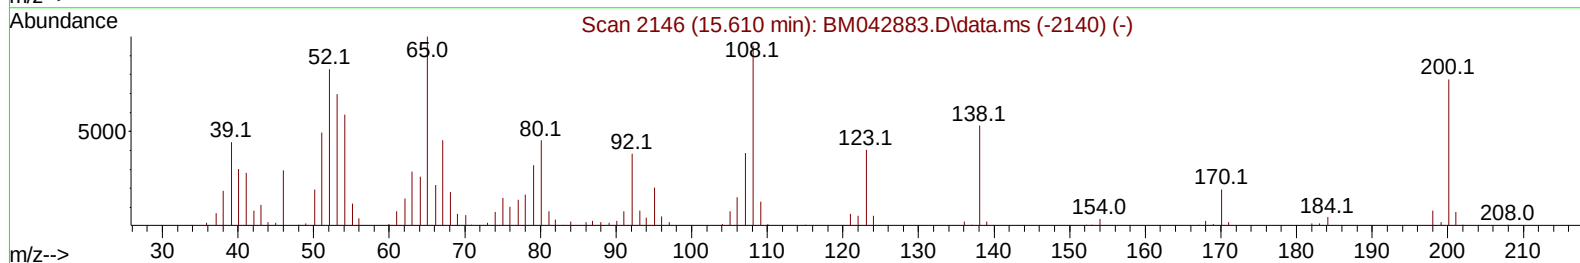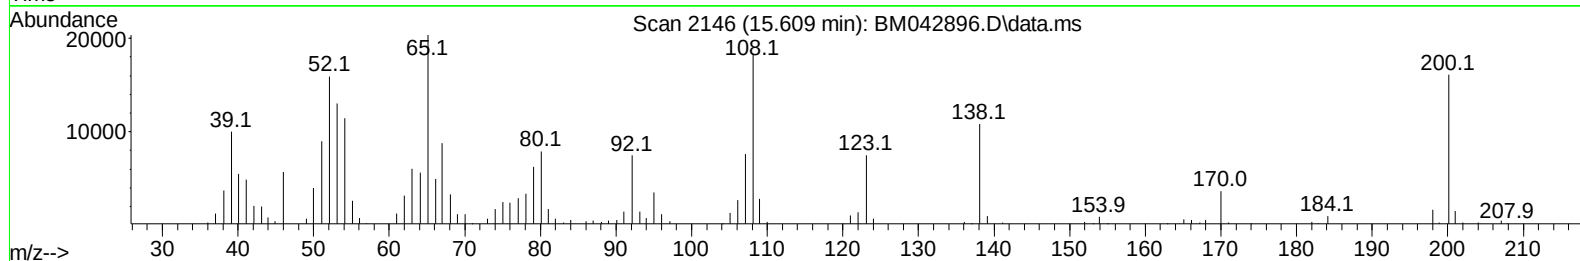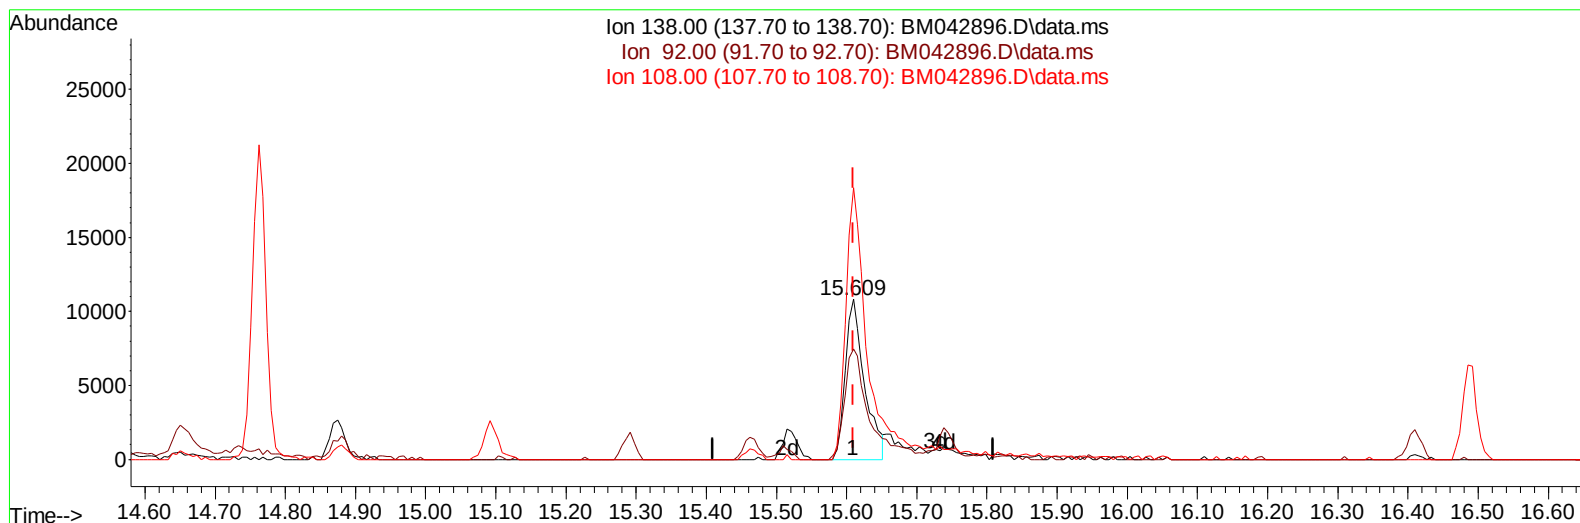

TIC: BM042896.D\data.ms

**(63) 4-Nitroaniline**

**15.609min (-0.000) 26.47 ng/ul**

**response 20713**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 138.00 | 100.00 | 100.00 |
| 92.00  | 59.20  | 69.14  |
| 108.00 | 161.90 | 169.60 |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM111723\  
 Data File : BM042896.D  
 Acq On : 19 Nov 2023 00:35  
 Operator : MA/JU  
 Sample : PB157269BS  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 SLCS269

Manual IntegrationsAPPROVED

Quant Time: Nov 19 03:21:58 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM111323.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Sat Nov 18 22:06:09 2023  
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023  
 Supervised By :mohammad ahmed 11/20/2023

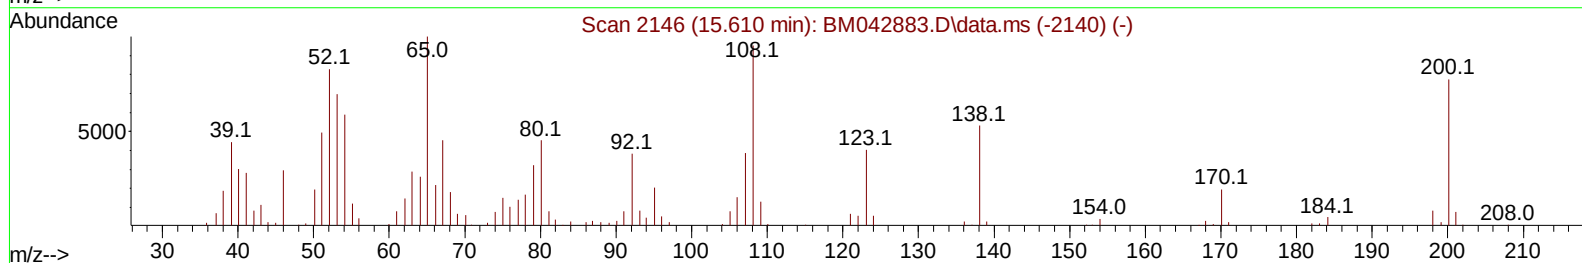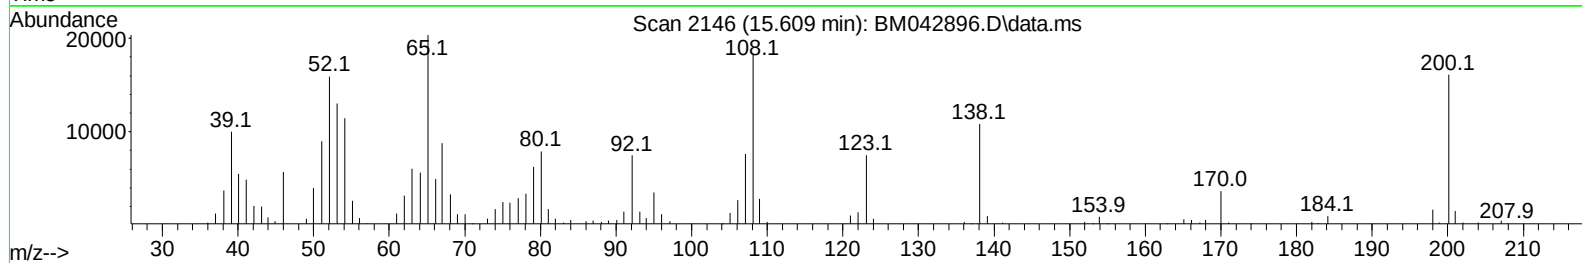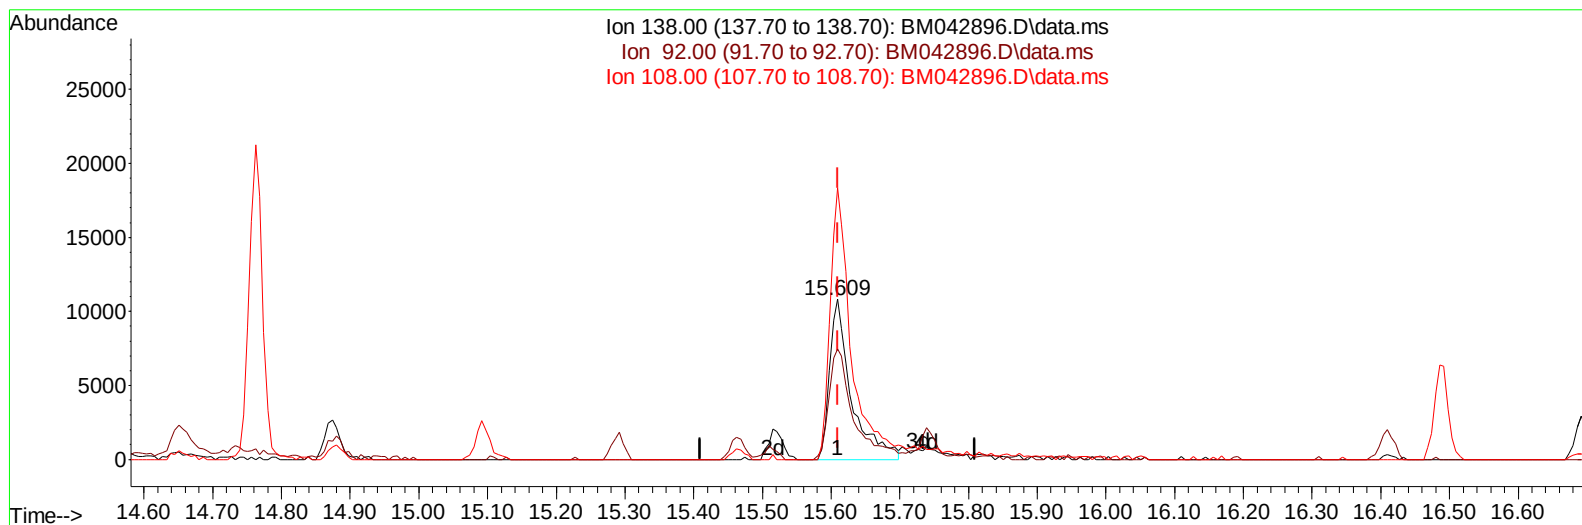

TIC: BM042896.D\data.ms

**(63) 4-Nitroaniline**

**15.609min (-0.000) 30.38 ng/ul m**

**response 23769**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 138.00 | 100.00 | 100.00 |
| 92.00  | 59.20  | 69.14  |
| 108.00 | 161.90 | 169.60 |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM111723\  
 Data File : BM042896.D  
 Acq On : 19 Nov 2023 00:35  
 Operator : MA/JU  
 Sample : PB157269BS  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 SLCS269

Manual IntegrationsAPPROVED

Quant Time: Nov 19 03:21:58 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM111323.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Sat Nov 18 22:06:09 2023  
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023  
 Supervised By :mohammad ahmed 11/20/2023

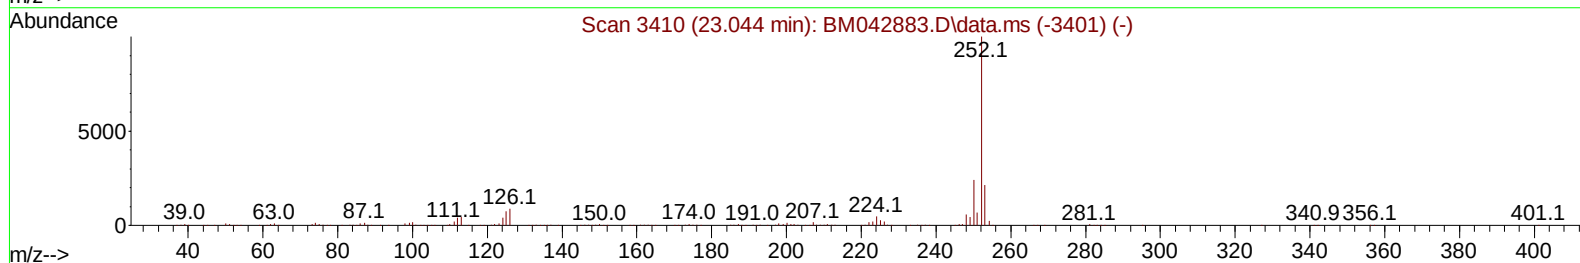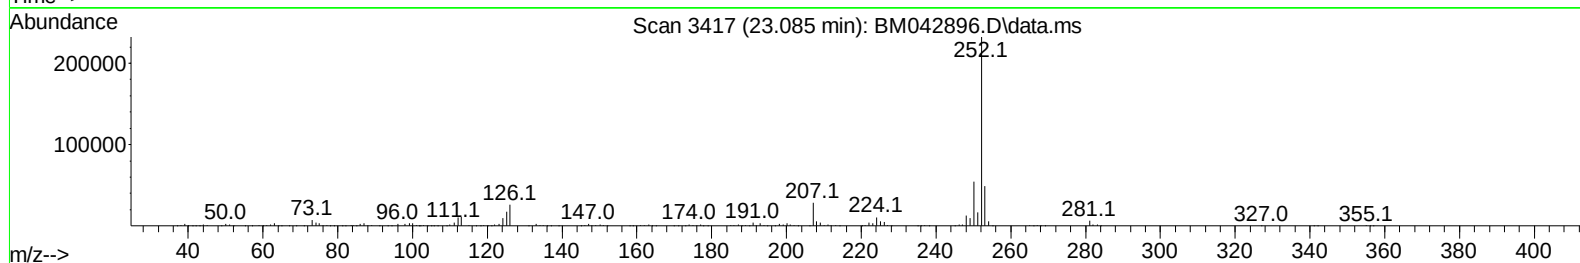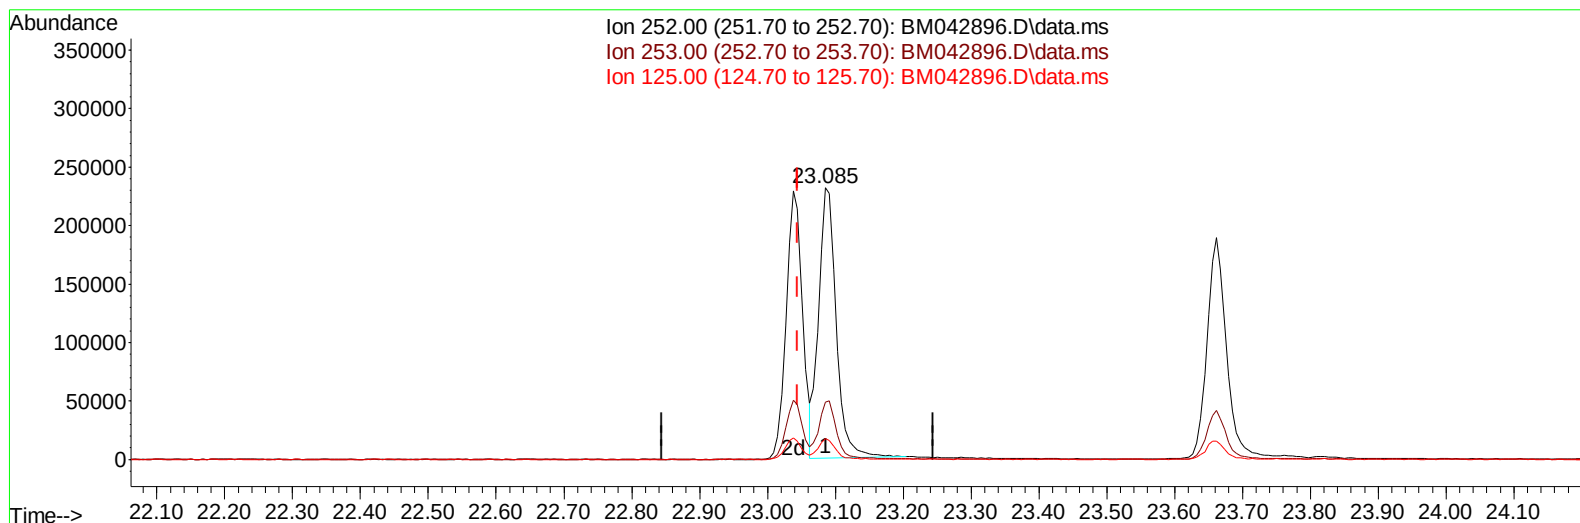

TIC: BM042896.D\data.ms

**(90) Benzo(b)fluoranthene**

**23.085min (+ 0.041) 37.99 ng/ul**

**response 416904**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 21.30  | 21.08  |
| 125.00 | 6.50   | 7.61   |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM111723\  
Data File : BM042896.D  
Acq On : 19 Nov 2023 00:35  
Operator : MA/JU  
Sample : PB157269BS  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SLCS269

Manual IntegrationsAPPROVED

Quant Time: Nov 19 03:21:58 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM111323.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sat Nov 18 22:06:09 2023  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023  
Supervised By :mohammad ahmed 11/20/2023

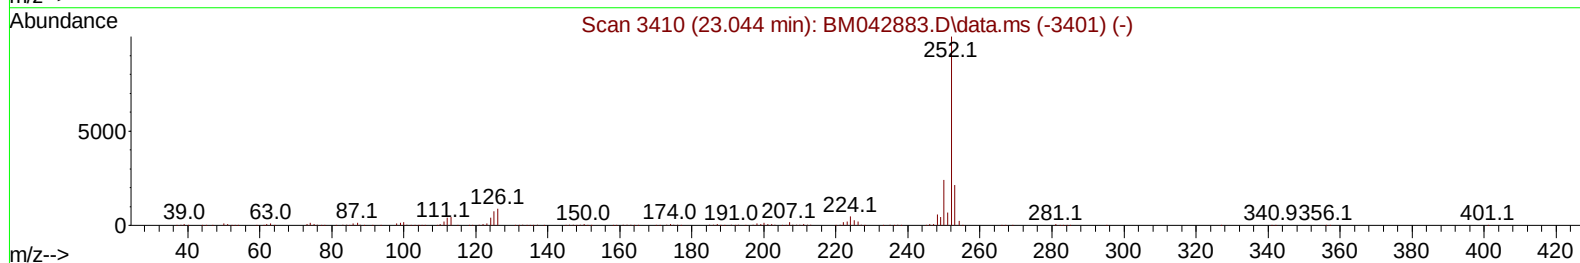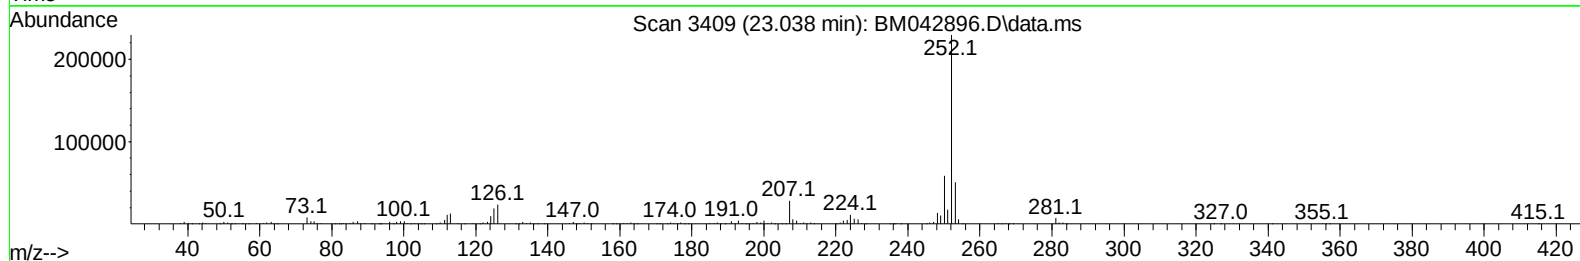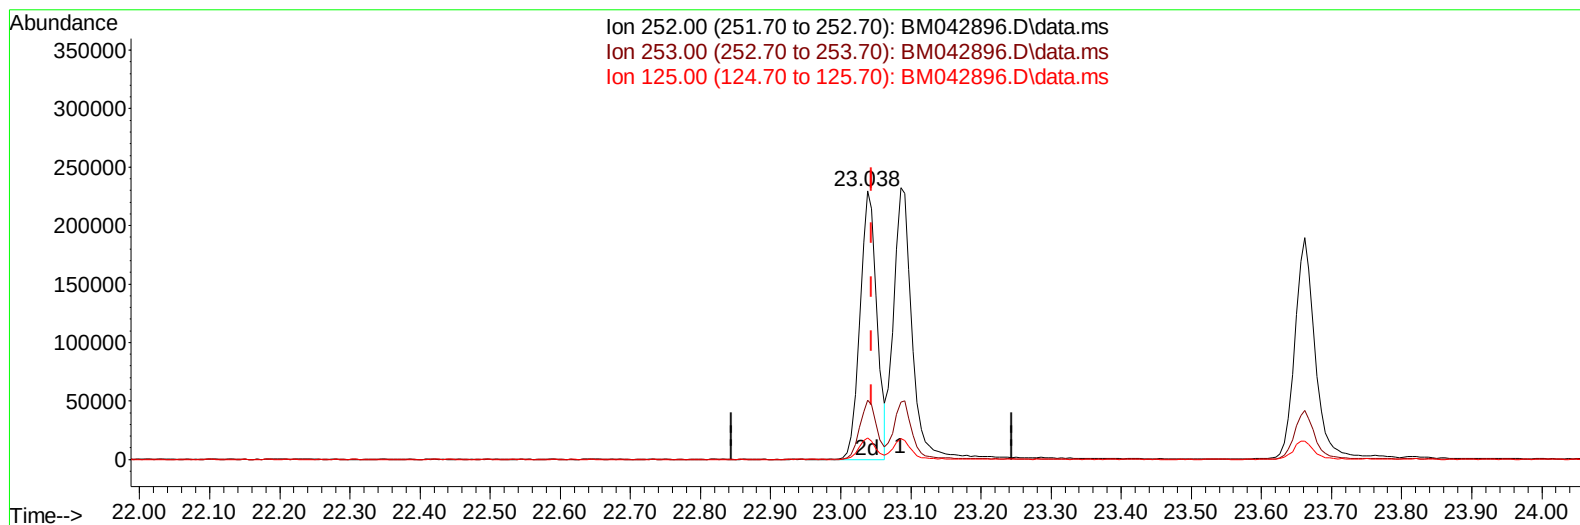

TIC: BM042896.D\data.ms

(90) Benzo(b)fluoranthene

23.038min (-0.006) 35.08 ng/ul m

response 384953

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 21.30  | 22.04  |
| 125.00 | 6.50   | 8.04#  |
| 0.00   | 0.00   | 0.00   |



Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM111723\  
 Data File : BM042896.D  
 Acq On : 19 Nov 2023 00:35  
 Operator : MA/JU  
 Sample : PB157269BS  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 SLCS269

Manual IntegrationsAPPROVED

Quant Time: Nov 19 23:51:42 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM111323.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Sat Nov 18 22:06:09 2023  
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023  
 Supervised By :mohammad ahmed 11/20/2023

| Compound                      | R.T.   | QIon | Response | Conc   | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|--------|--------|----------|
| -----                         |        |      |          |        |        |          |
| Internal Standards            |        |      |          |        |        |          |
| 1) 1,4-Dichlorobenzene-d4     | 7.816  | 152  | 24467    | 20.000 | ng/ul  | 0.00     |
| 20) Naphthalene-d8            | 10.627 | 136  | 95588    | 20.000 | ng/ul  | # 0.00   |
| 38) Acenaphthene-d10          | 14.468 | 164  | 60607    | 20.000 | ng/ul  | 0.00     |
| 64) Phenanthrene-d10          | 17.227 | 188  | 130550   | 20.000 | ng/ul  | 0.00     |
| 79) Chrysene-d12              | 21.409 | 240  | 151002   | 20.000 | ng/ul  | 0.00     |
| 88) Perylene-d12              | 23.768 | 264  | 160815   | 20.000 | ng/ul  | 0.00     |
| System Monitoring Compounds   |        |      |          |        |        |          |
| 3) 1,4-Dioxane-d8             | 3.169  | 96   | 4644     | 5.956  | ng/uL  | 0.00     |
| 4) Pyridine-d5                | 3.610  | 84   | 53254    | 27.456 | ng/ul  | 0.00     |
| 7) Phenol-d5                  | 6.981  | 99   | 73806    | 30.995 | ng/ul  | 0.00     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.163  | 67   | 57014    | 34.074 | ng/ul  | 0.00     |
| 11) 2-Chlorophenol-d4         | 7.333  | 132  | 56229    | 30.602 | ng/ul  | 0.00     |
| 15) 4-Methylphenol-d8         | 8.539  | 113  | 56271    | 30.012 | ng/ul  | 0.00     |
| 21) Nitrobenzene-d5           | 9.016  | 128  | 25996    | 31.019 | ng/ul  | 0.00     |
| 24) 2-Nitrophenol-d4          | 9.727  | 143  | 28582    | 29.154 | ng/ul  | 0.00     |
| 28) 2,4-Dichlorophenol-d3     | 10.251 | 165  | 56396    | 30.937 | ng/ul  | 0.00     |
| 31) 4-Chloroaniline-d4        | 10.804 | 131  | 55325    | 23.903 | ng/ul  | 0.00     |
| 46) Dimethylphthalate-d6      | 13.892 | 166  | 175001   | 30.509 | ng/ul  | 0.00     |
| 49) Acenaphthylene-d8         | 14.168 | 160  | 192145   | 31.308 | ng/ul  | 0.00     |
| 54) 4-Nitrophenol-d4          | 14.721 | 143  | 16109    | 24.857 | ng/ul  | 0.00     |
| 60) Fluorene-d10              | 15.462 | 176  | 146086   | 30.756 | ng/ul  | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 15.615 | 200  | 27643    | 27.954 | ng/ul  | 0.00     |
| 73) Anthracene-d10            | 17.327 | 188  | 228754   | 31.266 | ng/ul  | 0.00     |
| 81) Pyrene-d10                | 19.621 | 212  | 297629   | 30.099 | ng/ul  | 0.00     |
| 92) Benzo(a)pyrene-d12        | 23.615 | 264  | 312118   | 32.447 | ng/ul  | 0.00     |
| Target Compounds              |        |      |          |        |        |          |
|                               |        |      |          |        | Qvalue |          |
| 2) 1,4-Dioxane                | 3.204  | 88   | 10319    | 12.427 | ng/ul# | 84       |
| 5) Pyridine                   | 3.628  | 79   | 69150    | 32.787 | ng/ul  | 98       |
| 6) Benzaldehyde               | 6.981  | 77   | 44388    | 32.489 | ng/ul  | 86       |
| 8) Phenol                     | 7.010  | 94   | 78760    | 33.252 | ng/ul  | 96       |
| 10) Bis(2-Chloroethyl)ether   | 7.257  | 93   | 66119    | 33.794 | ng/ul  | 91       |
| 12) 2-Chlorophenol            | 7.369  | 128  | 59599    | 32.593 | ng/ul# | 88       |
| 13) 2-Methylphenol            | 8.263  | 108  | 55214    | 31.260 | ng/ul  | 95       |
| 14) 2,2'-oxybis(1-Chloropr... | 8.328  | 45   | 134046m  | 37.635 | ng/ul  |          |
| 16) Acetophenone              | 8.669  | 105  | 98118    | 31.122 | ng/ul  | 92       |
| 17) N-Nitroso-di-n-propyla... | 8.633  | 70   | 62262    | 32.442 | ng/ul  | 93       |
| 18) 4-Methylphenol            | 8.598  | 108  | 61796    | 32.180 | ng/ul  | 95       |
| 19) Hexachloroethane          | 8.863  | 117  | 35198    | 34.536 | ng/ul  | 87       |
| 22) Nitrobenzene              | 9.057  | 77   | 91705    | 36.205 | ng/ul  | 95       |
| 23) Isophorone                | 9.563  | 82   | 167334   | 33.169 | ng/ul  | 98       |
| 25) 2-Nitrophenol             | 9.757  | 139  | 31453    | 31.577 | ng/ul  | 87       |
| 26) 2,4-Dimethylphenol        | 9.798  | 107  | 65042    | 30.519 | ng/ul  | 94       |
| 27) Bis(2-Chloroethoxy)met... | 10.057 | 93   | 89633    | 35.160 | ng/ul  | 99       |
| 29) 2,4-Dichlorophenol        | 10.274 | 162  | 56942    | 32.992 | ng/ul  | 95       |
| 30) Naphthalene               | 10.674 | 128  | 193228   | 32.267 | ng/ul  | 98       |
| 32) 4-Chloroaniline           | 10.827 | 127  | 56584    | 25.482 | ng/ul  | 98       |
| 33) Hexachlorobutadiene       | 10.898 | 225  | 51253    | 33.618 | ng/ul  | 96       |
| 34) Caprolactam               | 11.645 | 113  | 16330m   | 31.911 | ng/ul  |          |
| 35) 4-Chloro-3-methylphenol   | 11.933 | 107  | 59685    | 32.273 | ng/ul  | 98       |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM111723\  
 Data File : BM042896.D  
 Acq On : 19 Nov 2023 00:35  
 Operator : MA/JU  
 Sample : PB157269BS  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 SLCS269

Manual IntegrationsAPPROVED

Quant Time: Nov 19 23:51:42 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM111323.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Sat Nov 18 22:06:09 2023  
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023  
 Supervised By :mohammad ahmed 11/20/2023

| Compound                      | R.T.   | QIon | Response | Conc   | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|--------|--------|----------|
| 36) 2-Methylnaphthalene       | 12.286 | 142  | 130362   | 32.480 | ng/ul  | 94       |
| 37) 1-Methylnaphthalene       | 12.510 | 142  | 130083   | 30.826 | ng/ul  | 97       |
| 39) 1,2,4,5-Tetrachloroben... | 12.639 | 216  | 84803    | 35.678 | ng/ul  | 97       |
| 40) Hexachlorocyclopentadiene | 12.580 | 237  | 32981    | 29.308 | ng/ul  | 96       |
| 41) 2,4,6-Trichlorophenol     | 12.904 | 196  | 47847    | 32.955 | ng/ul  | 96       |
| 42) 2,4,5-Trichlorophenol     | 12.980 | 196  | 48129    | 34.330 | ng/ul  | 97       |
| 43) 1,1'-Biphenyl             | 13.304 | 154  | 175058   | 34.635 | ng/ul  | 98       |
| 44) 2-Chloronaphthalene       | 13.351 | 162  | 140955   | 34.666 | ng/ul  | 98       |
| 45) 2-Nitroaniline            | 13.604 | 65   | 49573    | 37.383 | ng/ul  | 92       |
| 47) Dimethylphthalate         | 13.939 | 163  | 184793   | 33.076 | ng/ul  | 98       |
| 48) 2,6-Dinitrotoluene        | 14.092 | 165  | 33559    | 31.973 | ng/ul  | 91       |
| 50) Acenaphthylene            | 14.198 | 152  | 231044   | 33.597 | ng/ul  | 99       |
| 51) 3-Nitroaniline            | 14.439 | 138  | 23988    | 27.949 | ng/ul  | 99       |
| 52) Acenaphthene              | 14.533 | 153  | 156201   | 33.585 | ng/ul  | 99       |
| 53) 2,4-Dinitrophenol         | 14.651 | 184  | 12931    | 24.777 | ng/ul# | 81       |
| 55) 4-Nitrophenol             | 14.739 | 109  | 32303    | 31.676 | ng/ul  | 90       |
| 56) Dibenzofuran              | 14.874 | 168  | 219421   | 33.991 | ng/ul  | 99       |
| 57) 2,4-Dinitrotoluene        | 14.880 | 165  | 51697    | 33.549 | ng/ul  | 97       |
| 58) 2,3,4,6-Tetrachlorophenol | 15.092 | 232  | 46610    | 32.029 | ng/ul# | 97       |
| 59) Diethylphthalate          | 15.292 | 149  | 190119   | 32.452 | ng/ul  | 99       |
| 61) Fluorene                  | 15.521 | 166  | 188243   | 34.347 | ng/ul  | 99       |
| 62) 4-Chlorophenyl-phenyle... | 15.515 | 204  | 101956   | 34.519 | ng/ul  | 96       |
| 63) 4-Nitroaniline            | 15.609 | 138  | 23769m   | 30.377 | ng/ul  |          |
| 66) 4,6-Dinitro-2-methylph... | 15.627 | 198  | 31769    | 31.556 | ng/ul# | 88       |
| 67) N-Nitrosodiphenylamine    | 15.745 | 169  | 142746   | 34.862 | ng/ul  | 98       |
| 68) 4-Bromophenyl-phenylether | 16.409 | 248  | 60329    | 34.717 | ng/ul  | 91       |
| 69) Hexachlorobenzene         | 16.492 | 284  | 71432    | 33.625 | ng/ul  | 96       |
| 70) Atrazine                  | 16.692 | 200  | 37014    | 23.468 | ng/ul  | 95       |
| 71) Pentachlorophenol         | 16.862 | 266  | 36266    | 29.646 | ng/ul  | 92       |
| 72) Phenanthrene              | 17.268 | 178  | 284268   | 34.855 | ng/ul  | 98       |
| 74) Anthracene                | 17.362 | 178  | 284710   | 34.706 | ng/ul  | 99       |
| 75) 1,2,3,4-Tetrachloroben... | 13.257 | 216  | 86330    | 37.398 | ng/uL  | 99       |
| 76) Pentachlorobenzene        | 14.762 | 250  | 88300    | 36.455 | ng/uL  | 98       |
| 77) Carbazole                 | 17.656 | 167  | 215421   | 31.802 | ng/ul  | 99       |
| 78) Di-n-butylphthalate       | 18.168 | 149  | 328714   | 33.186 | ng/ul  | 99       |
| 80) Fluoranthene              | 19.286 | 202  | 354967   | 31.484 | ng/ul  | 99       |
| 82) Pyrene                    | 19.650 | 202  | 381254   | 31.892 | ng/ul  | 100      |
| 83) Butylbenzylphthalate      | 20.533 | 149  | 150552   | 29.485 | ng/ul  | 88       |
| 84) 3,3'-Dichlorobenzidine    | 21.338 | 252  | 98435    | 25.470 | ng/ul  | 99       |
| 85) Benzo(a)anthracene        | 21.391 | 228  | 391410   | 33.020 | ng/ul  | 98       |
| 86) Bis(2-ethylhexyl)phtha... | 21.280 | 149  | 229250   | 29.592 | ng/ul  | 100      |
| 87) Chrysene                  | 21.444 | 228  | 376753   | 32.773 | ng/ul  | 98       |
| 89) Di-n-octyl phthalate      | 22.185 | 149  | 403745   | 31.081 | ng/ul  | 100      |
| 90) Benzo(b)fluoranthene      | 23.038 | 252  | 384953m  | 35.076 | ng/ul  |          |
| 91) Benzo(k)fluoranthene      | 23.085 | 252  | 416904   | 35.686 | ng/ul  | 98       |
| 93) Benzo(a)pyrene            | 23.662 | 252  | 376253   | 35.183 | ng/ul  | 99       |
| 94) Indeno(1,2,3-cd)pyrene    | 26.226 | 276  | 477436   | 35.923 | ng/ul  | 99       |
| 95) Dibenzo(a,h)anthracene    | 26.238 | 278  | 378737   | 34.372 | ng/ul  | 98       |
| 96) Benzo(g,h,i)perylene      | 26.991 | 276  | 374483   | 35.483 | ng/ul  | 98       |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

**Instrument :**

BNA\_M

**ClientSampleId :**

SLCS269

**Manual IntegrationsAPPROVED**

Reviewed By :Yogesh Patel 11/20/2023

Supervised By :mohammad ahmed 11/20/2023

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM111723\  
 Data File : BM042896.D  
 Acq On : 19 Nov 2023 00:35  
 Operator : MA/JU  
 Sample : PB157269BS  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :

BNA\_M

ClientSampleId :

SLCS269

Manual IntegrationsAPPROVED

Quant Time: Nov 19 23:51:42 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM111323.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Sat Nov 18 22:06:09 2023  
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023  
 Supervised By :mohammad ahmed 11/20/2023

