

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042850.D
 Acq On : 17 Nov 2023 18:51
 Operator : MA/JU
 Sample : PB157227BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK227

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042850.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	38	rVB2	12728	16772	1.55%	0.170%
2	3.610	103	106	124	rBV	143428	242793	22.46%	2.466%
3	4.334	227	229	232	rVB2	2126	1835	0.17%	0.019%
4	4.616	273	277	279	rVB4	2452	2563	0.24%	0.026%
5	5.051	349	351	354	rVB3	1563	1507	0.14%	0.015%
6	5.210	377	378	380	rBV2	2038	1294	0.12%	0.013%
7	5.363	402	404	406	rVB3	1636	1161	0.11%	0.012%
8	6.687	626	629	631	rVB3	1285	1309	0.12%	0.013%
9	6.857	656	658	660	rBV3	1605	1256	0.12%	0.013%
10	6.910	665	667	671	rVB4	1573	1863	0.17%	0.019%
11	6.945	671	673	675	rBV2	1412	1685	0.16%	0.017%
12	6.987	675	680	702	rBV	150179	304383	28.16%	3.091%
13	7.122	702	703	706	rBV3	1888	1643	0.15%	0.017%
14	7.169	706	711	721	rBV	126516	213984	19.79%	2.173%
15	7.339	734	740	759	rVB	173147	311585	28.82%	3.164%
16	7.457	759	760	763	rBV3	1733	1133	0.10%	0.012%
17	7.822	816	822	835	rBV	93016	177586	16.43%	1.803%
18	8.539	938	944	961	rBV	164461	327468	30.29%	3.326%
19	9.022	1019	1026	1042	rBV	157026	303318	28.06%	3.080%
20	9.239	1060	1063	1068	rVB4	1266	1854	0.17%	0.019%
21	9.675	1135	1137	1141	rVB4	948	1387	0.13%	0.014%
22	9.733	1141	1147	1161	rBV	138417	262753	24.31%	2.668%
23	10.257	1228	1236	1254	rBV	153666	331593	30.67%	3.367%
24	10.551	1284	1286	1291	rVB4	992	1239	0.11%	0.013%
25	10.633	1292	1300	1313	rBV	136335	237181	21.94%	2.409%
26	10.810	1324	1330	1353	rBV2	122644	316057	29.24%	3.210%
27	12.257	1572	1576	1578	rVB4	1260	1219	0.11%	0.012%
28	13.327	1753	1758	1762	rVB5	1806	2569	0.24%	0.026%
29	13.480	1782	1784	1788	rBV2	876	1368	0.13%	0.014%
30	13.774	1832	1834	1839	rVB3	862	1127	0.10%	0.011%
31	13.898	1849	1855	1867	rBV	372994	533754	49.37%	5.420%
32	14.174	1896	1902	1916	rBV	410536	593993	54.95%	6.032%
33	14.263	1916	1917	1921	rVV3	1503	1322	0.12%	0.013%
34	14.304	1921	1924	1927	rVB3	1030	1176	0.11%	0.012%
35	14.474	1947	1953	1969	rVB	211016	310028	28.68%	3.148%
36	14.739	1992	1998	2019	rBV3	38510	162259	15.01%	1.648%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042850.D
 Acq On : 17 Nov 2023 18:51
 Operator : MA/JU
 Sample : PB157227BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK227

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	14.986	2038	2040	2044	rVB4	1106	1346	0.12%	0.014%
38	15.045	2049	2050	2053	rVB2	1772	1230	0.11%	0.012%
39	15.468	2116	2122	2136	rBV	506624	746054	69.01%	7.576%
40	15.621	2143	2148	2161	rBV	122320	208752	19.31%	2.120%
41	16.298	2260	2263	2266	rBV3	925	1179	0.11%	0.012%
42	17.227	2416	2421	2432	rVV	246919	368352	34.07%	3.741%
43	17.327	2432	2438	2457	rVV	547979	818941	75.76%	8.317%
44	17.451	2457	2459	2460	rVV2	1959	1402	0.13%	0.014%
45	17.462	2460	2461	2465	rVB4	1309	1254	0.12%	0.013%
46	18.274	2597	2599	2601	rBV3	1461	1631	0.15%	0.017%
47	18.321	2605	2607	2610	rVV3	960	1168	0.11%	0.012%
48	18.386	2616	2618	2621	rBV3	994	1148	0.11%	0.012%
49	18.703	2669	2672	2673	rVV2	1386	1215	0.11%	0.012%
50	19.192	2752	2755	2758	rVV3	4275	5462	0.51%	0.055%
51	19.268	2763	2768	2773	rBV3	3556	6776	0.63%	0.069%
52	19.315	2774	2776	2779	rVB2	1677	1154	0.11%	0.012%
53	19.350	2779	2782	2787	rBV6	1488	2821	0.26%	0.029%
54	19.627	2823	2829	2844	rBV	753059	1038682	96.08%	10.548%
55	20.421	2962	2964	2967	rBV3	3477	4151	0.38%	0.042%
56	21.415	3128	3133	3143	rBV	273672	410316	37.96%	4.167%
57	23.621	3501	3508	3520	rBV	552217	1081029	100.00%	10.978%
58	23.774	3528	3534	3546	rVB	217345	466994	43.20%	4.742%




Sum of corrected areas: 9847074

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042850.D
Acq On : 17 Nov 2023 18:51
Operator : MA/JU
Sample : PB157227BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK227

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

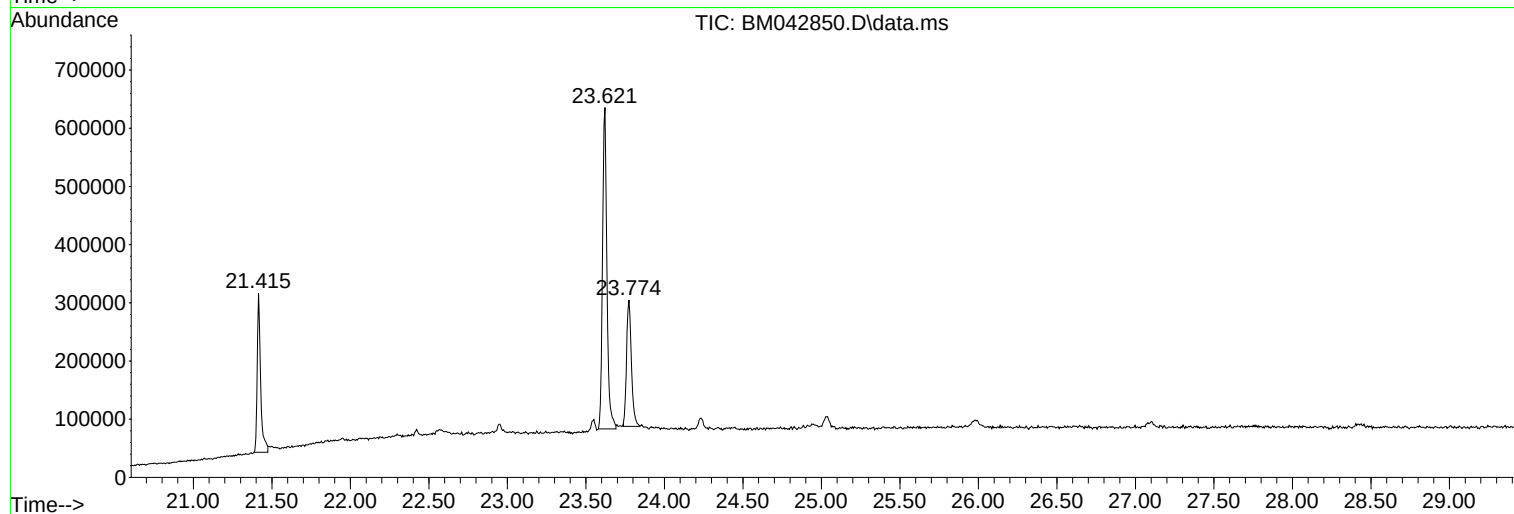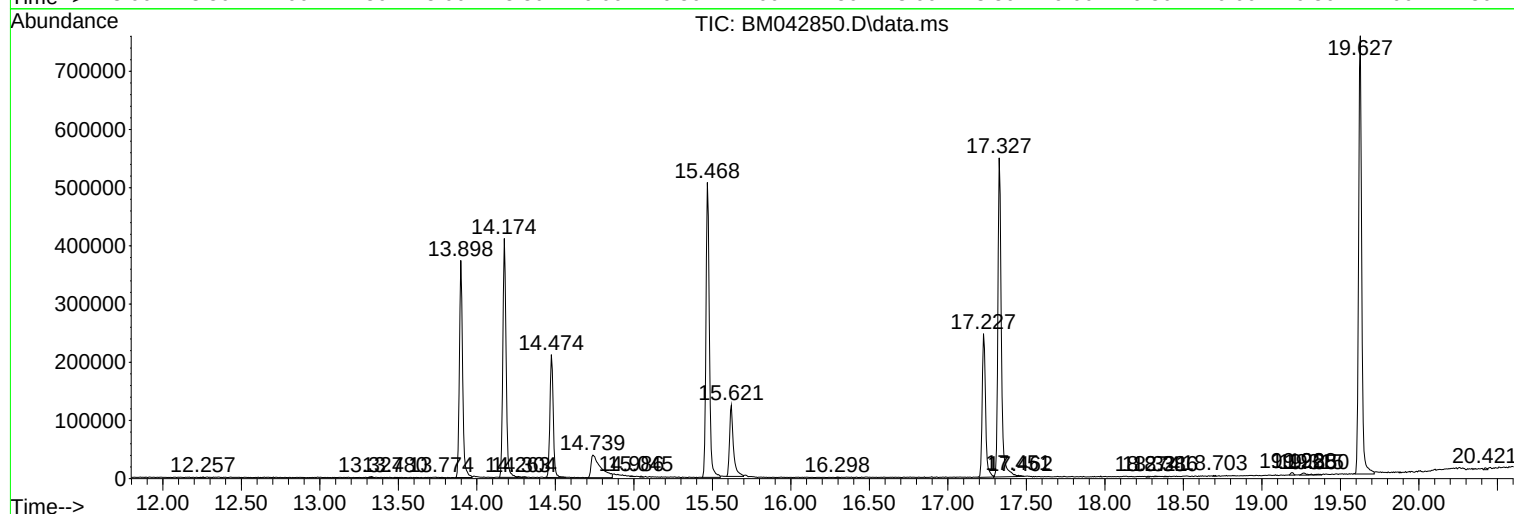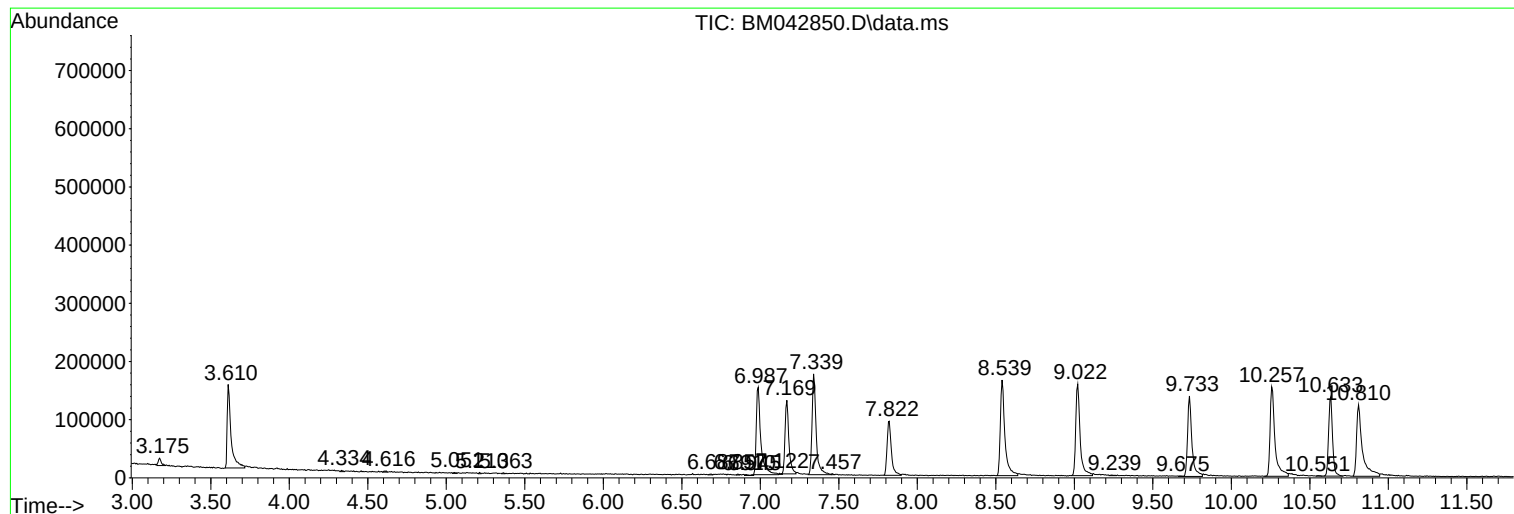

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042850.D
Acq On : 17 Nov 2023 18:51
Operator : MA/JU
Sample : PB157227BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK227

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042850.D
Acq On : 17 Nov 2023 18:51
Operator : MA/JU
Sample : PB157227BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK227

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------