

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042851.D
 Acq On : 17 Nov 2023 19:27
 Operator : MA/JU
 Sample : PB157005BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK005

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042851.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	29	31	37	rVB2	11446	15680	1.84%	0.188%
2	3.610	102	106	118	rBV	132796	217836	25.62%	2.617%
3	4.704	291	292	295	rBV2	1295	1229	0.14%	0.015%
4	4.781	303	305	306	rVB2	1702	1006	0.12%	0.012%
5	4.798	306	308	311	rBV3	1745	1567	0.18%	0.019%
6	4.987	339	340	345	rVB3	1665	1957	0.23%	0.024%
7	5.204	374	377	378	rBV2	1087	1201	0.14%	0.014%
8	5.363	402	404	408	rVB3	1497	2022	0.24%	0.024%
9	5.434	414	416	419	rBV3	1635	1143	0.13%	0.014%
10	5.581	439	441	445	rVB4	1325	1335	0.16%	0.016%
11	6.116	531	532	535	rBV3	1545	1194	0.14%	0.014%
12	6.187	542	544	548	rVB4	898	1080	0.13%	0.013%
13	6.357	571	573	577	rVB4	1014	916	0.11%	0.011%
14	6.475	590	593	595	rBV4	803	1131	0.13%	0.014%
15	6.492	595	596	599	rVV3	1244	1283	0.15%	0.015%
16	6.545	603	605	608	rVB3	824	891	0.10%	0.011%
17	6.987	674	680	699	rBV	131015	267895	31.51%	3.218%
18	7.169	705	711	722	rBV	112684	197665	23.25%	2.375%
19	7.339	734	740	754	rBV	156076	274835	32.33%	3.302%
20	7.581	779	781	785	rVB4	1000	880	0.10%	0.011%
21	7.822	813	822	836	rBV	104056	198558	23.36%	2.385%
22	8.539	938	944	963	rBV	143274	285389	33.57%	3.429%
23	9.022	1019	1026	1046	rBV	132931	267022	31.41%	3.208%
24	9.151	1046	1048	1052	rVB4	1481	1877	0.22%	0.023%
25	9.186	1052	1054	1055	rBV2	1596	1028	0.12%	0.012%
26	9.733	1141	1147	1161	rBV3	114167	218811	25.74%	2.629%
27	9.875	1168	1171	1173	rVB3	864	857	0.10%	0.010%
28	9.904	1174	1176	1179	rVB2	1243	1077	0.13%	0.013%
29	10.257	1229	1236	1248	rBV	125537	265860	31.27%	3.194%
30	10.633	1293	1300	1313	rBV	138015	245339	28.86%	2.947%
31	10.810	1324	1330	1348	rBV	103143	258849	30.45%	3.110%
32	11.057	1370	1372	1375	rVB2	1692	1431	0.17%	0.017%
33	11.674	1472	1477	1478	rVV4	1097	1833	0.22%	0.022%
34	11.704	1481	1482	1487	rVB3	660	938	0.11%	0.011%
35	12.263	1573	1577	1580	rBV2	1115	1646	0.19%	0.020%
36	12.639	1637	1641	1642	rBV2	724	854	0.10%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042851.D
 Acq On : 17 Nov 2023 19:27
 Operator : MA/JU
 Sample : PB157005BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK005

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	12.674	1645	1647	1650	rVB3	864	861	0.10%	0.010%
38	13.045	1706	1710	1712	rBV5	650	1017	0.12%	0.012%
39	13.321	1753	1757	1761	rBV3	1777	3189	0.38%	0.038%
40	13.398	1766	1770	1773	rBV3	828	999	0.12%	0.012%

41	13.698	1817	1821	1826	rBV	1208	2340	0.28%	0.028%
42	13.898	1849	1855	1871	rBV	294601	431566	50.77%	5.185%
43	13.998	1871	1872	1876	rVV2	1236	1457	0.17%	0.018%
44	14.174	1896	1902	1915	rBV	328799	484649	57.01%	5.822%
45	14.386	1933	1938	1943	rVB5	562	1059	0.12%	0.013%

46	14.474	1948	1953	1961	rBV	201476	304305	35.80%	3.656%
47	14.586	1971	1972	1979	rVB5	929	1621	0.19%	0.019%
48	14.657	1979	1984	1985	rBV2	763	931	0.11%	0.011%
49	14.751	1993	2000	2008	rBV4	23583	76869	9.04%	0.923%
50	15.298	2090	2093	2097	rVB2	935	1378	0.16%	0.017%

51	15.468	2116	2122	2133	rBV	401625	588796	69.26%	7.074%
52	15.621	2143	2148	2159	rBV2	85188	153802	18.09%	1.848%
53	15.715	2162	2164	2166	rVB2	1713	1343	0.16%	0.016%
54	15.851	2186	2187	2191	rVB3	805	942	0.11%	0.011%
55	16.045	2218	2220	2223	rBV3	981	1261	0.15%	0.015%

56	16.215	2245	2249	2251	rBV3	821	991	0.12%	0.012%
57	16.374	2273	2276	2279	rVV2	760	869	0.10%	0.010%
58	16.786	2341	2346	2349	rBV4	793	1418	0.17%	0.017%
59	17.033	2383	2388	2390	rBV3	855	1654	0.19%	0.020%
60	17.227	2415	2421	2432	rBV	240320	350493	41.23%	4.211%

61	17.327	2432	2438	2461	rVB	406633	628009	73.87%	7.545%
62	17.762	2509	2512	2515	rBV4	717	1020	0.12%	0.012%
63	17.921	2536	2539	2540	rBV2	1027	852	0.10%	0.010%
64	18.162	2579	2580	2583	rVV2	1188	1195	0.14%	0.014%
65	18.274	2597	2599	2602	rBV3	1261	1412	0.17%	0.017%

66	18.468	2629	2632	2633	rBV2	1025	875	0.10%	0.011%
67	18.521	2639	2641	2645	rVB4	1453	1352	0.16%	0.016%
68	18.674	2665	2667	2670	rBV3	951	1138	0.13%	0.014%
69	18.833	2692	2694	2695	rVB3	1350	860	0.10%	0.010%
70	18.845	2695	2696	2697	rBV	1381	882	0.10%	0.011%

71	18.880	2700	2702	2705	rVB3	1020	889	0.10%	0.011%
72	18.974	2712	2718	2719	rBV3	1273	1819	0.21%	0.022%
73	19.015	2723	2725	2729	rBV4	925	1187	0.14%	0.014%
74	19.092	2734	2738	2742	rBV4	1267	1931	0.23%	0.023%
75	19.127	2742	2744	2746	rBV3	825	945	0.11%	0.011%

76	19.192	2752	2755	2758	rBV5	3168	4555	0.54%	0.055%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042851.D
Acq On : 17 Nov 2023 19:27
Operator : MA/JU
Sample : PB157005BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK005

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Title : SVOA CALIBRATION

77	19.262	2765	2767	2770	rVB2	2203	2335	0.27%	0.028%
78	19.321	2773	2777	2779	rBV5	939	1179	0.14%	0.014%
79	19.580	2818	2821	2822	rBV	1398	1175	0.14%	0.014%
80	19.627	2823	2829	2843	rVV	575660	784079	92.23%	9.420%
81	20.133	2913	2915	2917	rBV3	1549	1219	0.14%	0.015%
82	20.203	2925	2927	2931	rBV5	1861	2075	0.24%	0.025%
83	21.415	3128	3133	3144	rBV	269365	398022	46.82%	4.782%
84	23.615	3501	3507	3519	rBV2	425989	850124	100.00%	10.213%
85	23.774	3527	3534	3546	rBV	218142	476877	56.09%	5.729%




Sum of corrected areas: 8323931

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042851.D
Acq On : 17 Nov 2023 19:27
Operator : MA/JU
Sample : PB157005BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK005

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

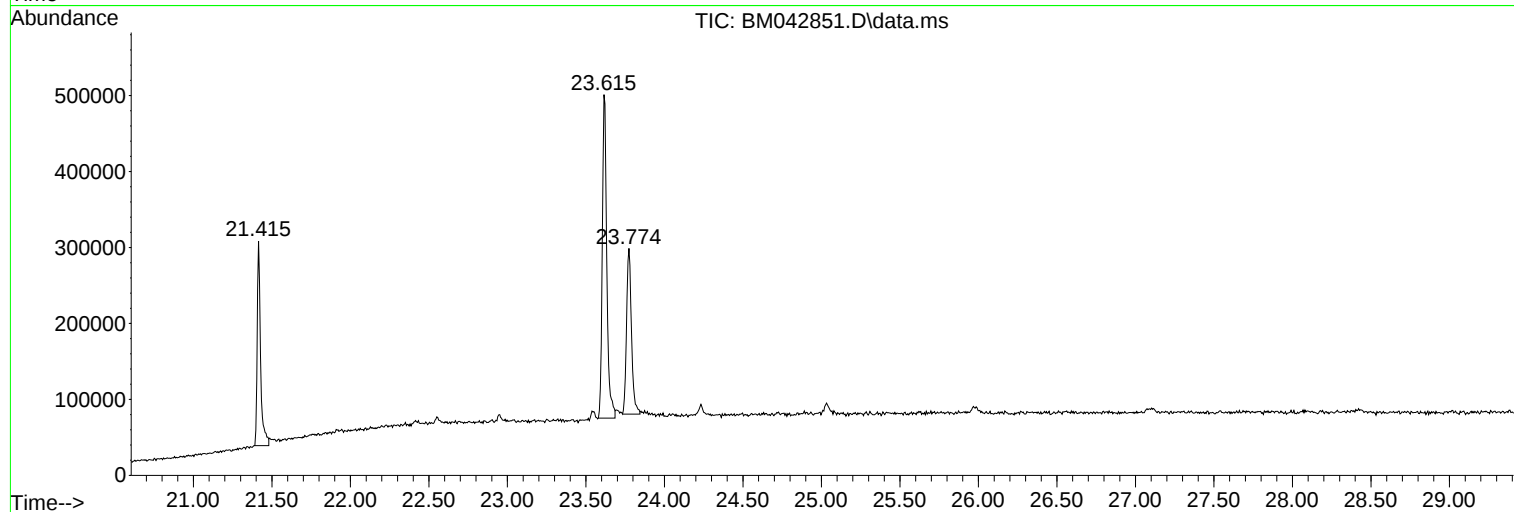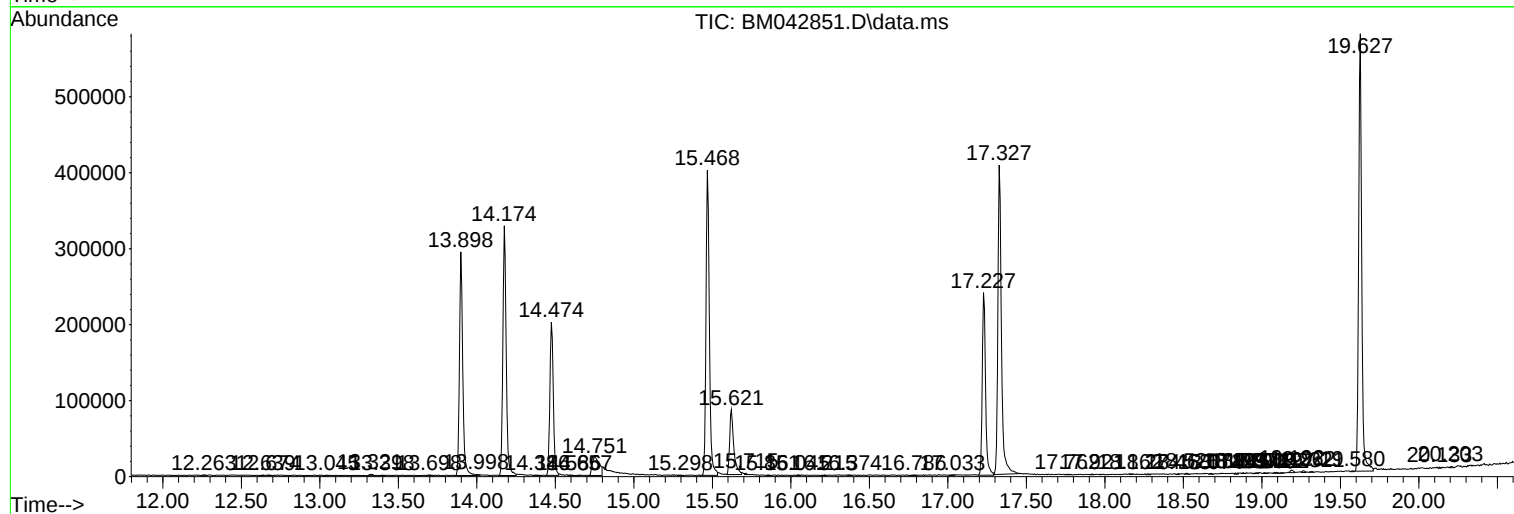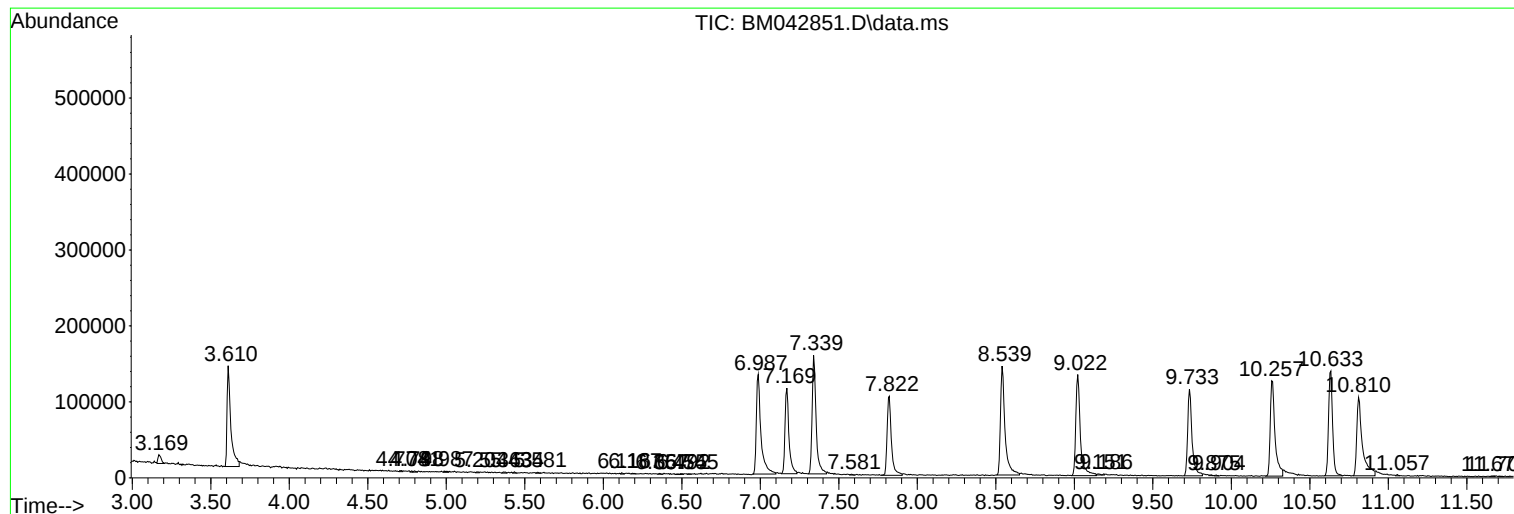

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042851.D
Acq On : 17 Nov 2023 19:27
Operator : MA/JU
Sample : PB157005BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK005

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042851.D
Acq On : 17 Nov 2023 19:27
Operator : MA/JU
Sample : PB157005BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK005

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc