

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042852.D
 Acq On : 17 Nov 2023 20:04
 Operator : MA/JU
 Sample : 05259-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCG93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042852.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	29	31	37	rVB5	5279	7482	0.79%	0.095%
2	3.622	105	108	118	rBV	34533	68513	7.26%	0.866%
3	5.281	388	390	395	rBV4	1400	2434	0.26%	0.031%
4	6.010	510	514	516	rBV4	1191	1740	0.18%	0.022%
5	6.057	520	522	525	rBV4	1156	1219	0.13%	0.015%
6	6.146	535	537	539	rBV2	1479	1342	0.14%	0.017%
7	6.446	586	588	591	rVB4	1565	1286	0.14%	0.016%
8	6.693	625	630	632	rBV5	842	1457	0.15%	0.018%
9	6.993	677	681	694	rVV2	17640	44457	4.71%	0.562%
10	7.169	705	711	725	rBV	97929	180315	19.11%	2.278%
11	7.340	735	740	756	rVV	94888	186588	19.77%	2.358%
12	7.475	762	763	765	rBV2	1336	945	0.10%	0.012%
13	7.557	776	777	783	rVB4	850	1212	0.13%	0.015%
14	7.675	794	797	801	rBV3	1432	1893	0.20%	0.024%
15	7.816	815	821	835	rBV	107413	204479	21.67%	2.584%
16	7.922	837	839	841	rVB3	1429	1021	0.11%	0.013%
17	8.545	940	945	959	rBV2	54030	119955	12.71%	1.516%
18	8.693	969	970	976	rVB4	1006	1119	0.12%	0.014%
19	9.022	1020	1026	1040	rBV	121759	240809	25.52%	3.043%
20	9.204	1053	1057	1061	rVB2	3912	5024	0.53%	0.063%
21	9.734	1141	1147	1158	rBV2	100555	192951	20.45%	2.438%
22	9.892	1171	1174	1175	rVV2	988	972	0.10%	0.012%
23	10.122	1209	1213	1215	rBV5	984	1605	0.17%	0.020%
24	10.263	1230	1237	1257	rBV2	102602	239205	25.35%	3.023%
25	10.392	1257	1259	1261	rVB3	1589	1463	0.16%	0.018%
26	10.504	1275	1278	1279	rVB3	1248	1156	0.12%	0.015%
27	10.528	1279	1282	1284	rBV3	1338	1035	0.11%	0.013%
28	10.634	1293	1300	1311	rBV	152327	261499	27.71%	3.304%
29	10.734	1314	1317	1320	rVB4	955	1072	0.11%	0.014%
30	10.810	1324	1330	1350	rBV	82357	214831	22.77%	2.715%
31	10.963	1355	1356	1364	rVV6	2515	3674	0.39%	0.046%
32	11.451	1438	1439	1444	rVB4	1364	1213	0.13%	0.015%
33	11.692	1475	1480	1483	rBV3	2546	3589	0.38%	0.045%
34	11.786	1493	1496	1499	rVB3	1000	1065	0.11%	0.013%
35	12.263	1574	1577	1580	rVB3	1031	1156	0.12%	0.015%
36	12.298	1580	1583	1585	rBV2	1127	1166	0.12%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042852.D
 Acq On : 17 Nov 2023 20:04
 Operator : MA/JU
 Sample : 05259-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCG93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	13.322	1750	1757	1764	rVB6	2764	4670	0.49%	0.059%
38	13.704	1819	1822	1827	rVB4	1683	2406	0.25%	0.030%
39	13.898	1849	1855	1866	rBV	289314	428513	45.41%	5.415%
40	13.986	1869	1870	1874	rVV3	2171	2132	0.23%	0.027%
41	14.175	1896	1902	1916	rBV	313324	470626	49.87%	5.947%
42	14.474	1947	1953	1965	rBV	228404	330595	35.03%	4.177%
43	14.798	2002	2008	2009	rBV2	1762	2051	0.22%	0.026%
44	14.816	2009	2011	2013	rVV	1740	1603	0.17%	0.020%
45	15.092	2053	2058	2059	rBV4	782	944	0.10%	0.012%
46	15.110	2059	2061	2065	rVB3	972	972	0.10%	0.012%
47	15.386	2104	2108	2111	rVB2	851	1186	0.13%	0.015%
48	15.416	2111	2113	2116	rBV2	1042	1142	0.12%	0.014%
49	15.469	2116	2122	2139	rVV	411260	611856	64.84%	7.731%
50	15.621	2141	2148	2162	rVV	88212	170989	18.12%	2.161%
51	15.716	2162	2164	2169	rVV4	3856	5658	0.60%	0.071%
52	15.763	2169	2172	2174	rVV3	1133	1523	0.16%	0.019%
53	17.227	2415	2421	2432	rBV	266793	379864	40.26%	4.800%
54	17.327	2432	2438	2465	rVV	473331	709329	75.17%	8.963%
55	17.498	2465	2467	2473	rVV3	1160	1916	0.20%	0.024%
56	17.868	2529	2530	2533	rBV2	1450	1259	0.13%	0.016%
57	18.051	2559	2561	2564	rBV3	808	1133	0.12%	0.014%
58	18.098	2564	2569	2570	rBV3	2973	4094	0.43%	0.052%
59	18.168	2580	2581	2583	rBV2	991	964	0.10%	0.012%
60	18.186	2583	2584	2587	rVV3	1509	1094	0.12%	0.014%
61	18.474	2631	2633	2635	rBV3	1147	972	0.10%	0.012%
62	18.909	2705	2707	2710	rVB3	1463	1288	0.14%	0.016%
63	18.998	2718	2722	2725	rBV3	1308	1440	0.15%	0.018%
64	19.192	2751	2755	2758	rVB4	2663	3392	0.36%	0.043%
65	19.268	2764	2768	2771	rBV4	3489	5311	0.56%	0.067%
66	19.315	2775	2776	2780	rBV4	1527	1353	0.14%	0.017%
67	19.374	2780	2786	2792	rBV7	3220	8037	0.85%	0.102%
68	19.421	2792	2794	2797	rVB3	1109	1119	0.12%	0.014%
69	19.498	2804	2807	2810	rBV5	2123	2681	0.28%	0.034%
70	19.557	2816	2817	2819	rBV2	1707	1215	0.13%	0.015%
71	19.627	2823	2829	2840	rBV	639529	867857	91.97%	10.966%
72	20.009	2892	2894	2897	rVB3	1811	2063	0.22%	0.026%
73	20.227	2929	2931	2932	rVB2	2031	961	0.10%	0.012%
74	20.362	2951	2954	2955	rBV3	2559	2706	0.29%	0.034%
75	21.415	3128	3133	3144	rBV	272712	425999	45.15%	5.383%
76	23.615	3501	3507	3523	rBV	472681	943614	100.00%	11.923%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042852.D
Acq On : 17 Nov 2023 20:04
Operator : MA/JU
Sample : 05259-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG93

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Title : SVOA CALIBRATION

77	23.774	3527	3534	3545	rBV	245802	506499	53.68%	6.400%
----	--------	------	------	------	-----	--------	--------	--------	--------




Sum of corrected areas: 7913968

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042852.D
Acq On : 17 Nov 2023 20:04
Operator : MA/JU
Sample : 05259-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG93

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

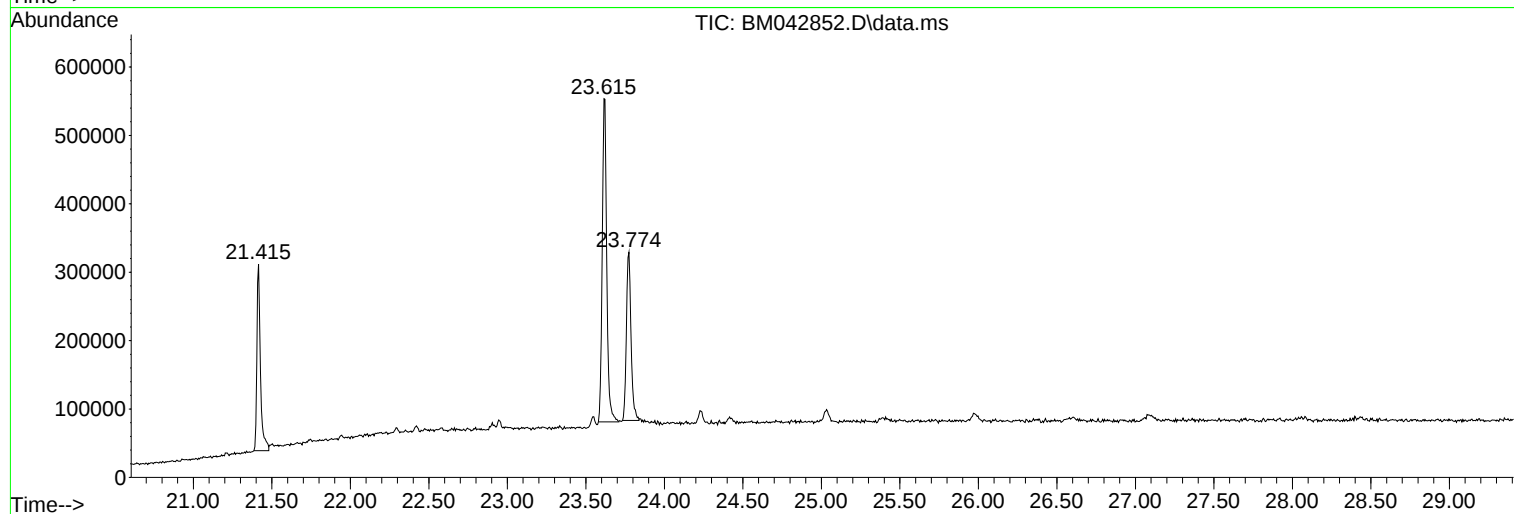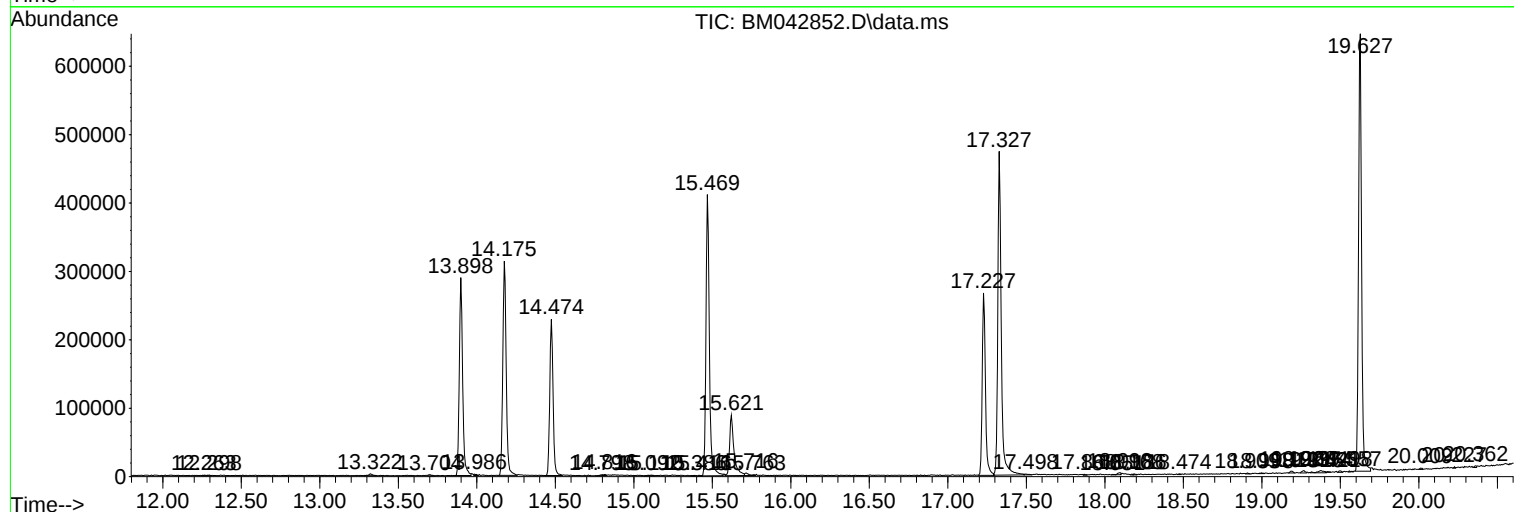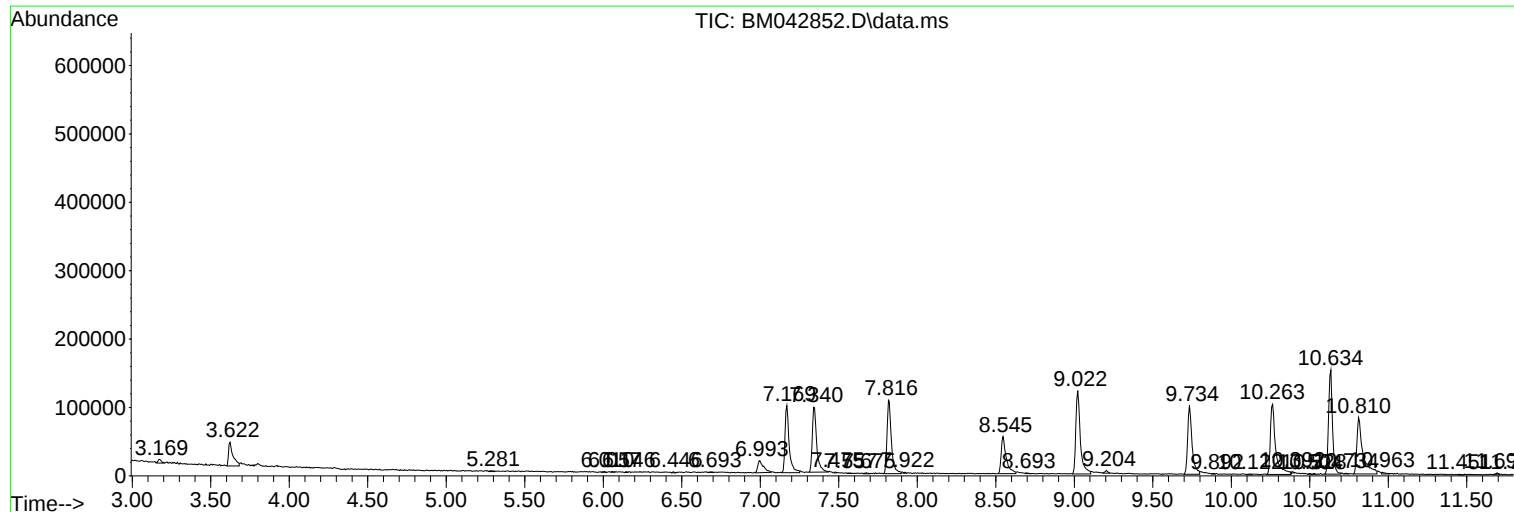

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042852.D
Acq On : 17 Nov 2023 20:04
Operator : MA/JU
Sample : 05259-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG93

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042852.D
Acq On : 17 Nov 2023 20:04
Operator : MA/JU
Sample : 05259-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG93

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc