

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042854.D
 Acq On : 17 Nov 2023 21:16
 Operator : MA/JU
 Sample : 05268-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042854.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.622	104	108	122	rBV	40706	82012	5.96%	0.782%
2	4.940	330	332	336	rVB5	1492	2029	0.15%	0.019%
3	6.116	529	532	534	rBV3	1457	1943	0.14%	0.019%
4	6.322	565	567	572	rBV6	1173	1752	0.13%	0.017%
5	6.993	674	681	692	rBV2	27478	71143	5.17%	0.678%
6	7.169	705	711	723	rBV	144591	258277	18.75%	2.462%
7	7.340	735	740	753	rBV	144675	266113	19.32%	2.537%
8	7.722	803	805	808	rBV4	1197	1382	0.10%	0.013%
9	7.822	816	822	834	rBV	107882	200031	14.53%	1.907%
10	8.539	939	944	957	rBV	77485	167438	12.16%	1.596%
11	8.681	965	968	971	rBV5	1654	2216	0.16%	0.021%
12	9.022	1019	1026	1046	rBV	183346	355677	25.83%	3.391%
13	9.734	1140	1147	1163	rBV	145150	291912	21.20%	2.783%
14	9.839	1163	1165	1174	rVB7	2691	4551	0.33%	0.043%
15	10.257	1229	1236	1259	rBV2	165045	356377	25.88%	3.397%
16	10.628	1292	1299	1307	rBV	147176	259431	18.84%	2.473%
17	10.810	1323	1330	1343	rBV	122146	285785	20.75%	2.724%
18	11.645	1468	1472	1474	rBV3	1213	1687	0.12%	0.016%
19	11.692	1475	1480	1484	rVB3	1408	2772	0.20%	0.026%
20	13.322	1753	1757	1762	rVB4	1660	2965	0.22%	0.028%
21	13.898	1849	1855	1872	rBV	447991	631892	45.88%	6.024%
22	14.174	1896	1902	1916	rBV	483167	686071	49.82%	6.540%
23	14.263	1916	1917	1922	rVV3	2239	2502	0.18%	0.024%
24	14.316	1922	1926	1928	rVB3	1292	1498	0.11%	0.014%
25	14.474	1947	1953	1961	rBV2	216462	318269	23.11%	3.034%
26	14.533	1961	1963	1967	rVB3	1378	1880	0.14%	0.018%
27	14.780	1999	2005	2009	rBV7	3946	8804	0.64%	0.084%
28	14.892	2021	2024	2028	rVB4	1788	1954	0.14%	0.019%
29	15.251	2084	2085	2090	rVB3	1393	1419	0.10%	0.014%
30	15.468	2116	2122	2136	rBV	635126	907207	65.88%	8.649%
31	15.616	2142	2147	2161	rBV	169360	277515	20.15%	2.646%
32	17.227	2415	2421	2432	rBV	261286	380015	27.59%	3.623%
33	17.327	2432	2438	2457	rVV	750831	1039472	75.48%	9.909%
34	17.480	2462	2464	2466	rVV3	2143	1691	0.12%	0.016%
35	17.680	2496	2498	2503	rBV5	1115	1626	0.12%	0.016%
36	17.857	2525	2528	2533	rVB3	3745	4607	0.33%	0.044%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042854.D
 Acq On : 17 Nov 2023 21:16
 Operator : MA/JU
 Sample : 05268-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	18.098	2562	2569	2572	rBV4	2876	5959	0.43%	0.057%
38	18.827	2690	2693	2695	rBV4	1291	1628	0.12%	0.016%
39	18.974	2715	2718	2721	rBV4	1607	1765	0.13%	0.017%
40	19.115	2741	2742	2745	rBV3	1334	1516	0.11%	0.014%
41	19.186	2750	2754	2759	rVB3	6639	9413	0.68%	0.090%
42	19.262	2764	2767	2772	rVB4	5107	6473	0.47%	0.062%
43	19.374	2783	2786	2788	rBV3	1794	2565	0.19%	0.024%
44	19.498	2805	2807	2810	rBV4	1282	1611	0.12%	0.015%
45	19.627	2823	2829	2839	rBV	982365	1305733	94.82%	12.448%
46	21.415	3128	3133	3143	rBV2	278887	421658	30.62%	4.020%
47	23.621	3501	3508	3521	rBV	710683	1377136	100.00%	13.128%
48	23.774	3527	3534	3544	rBV	223172	472355	34.30%	4.503%




Sum of corrected areas: 10489727

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042854.D
Acq On : 17 Nov 2023 21:16
Operator : MA/JU
Sample : 05268-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

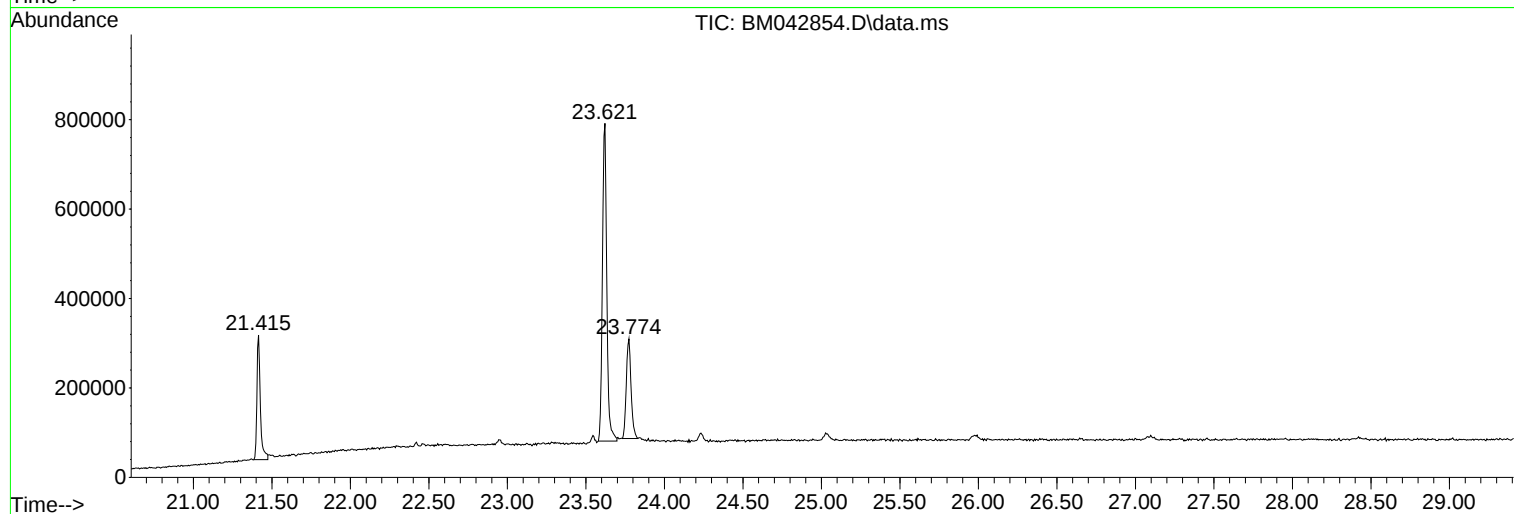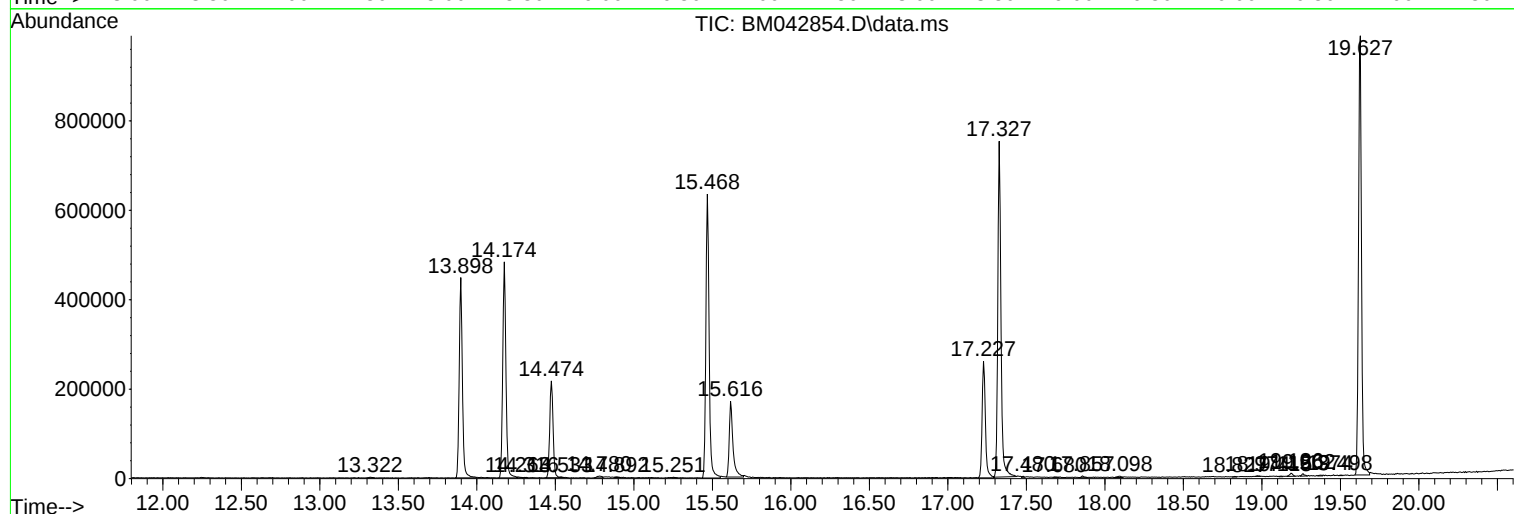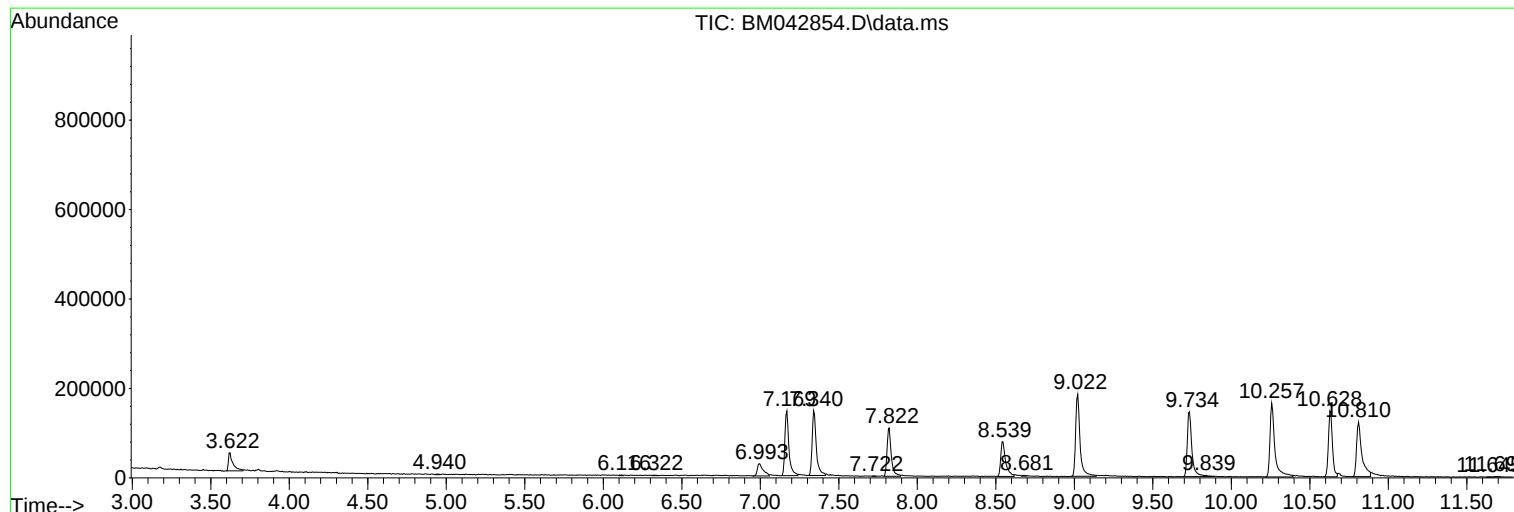

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042854.D
Acq On : 17 Nov 2023 21:16
Operator : MA/JU
Sample : 05268-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042854.D
Acq On : 17 Nov 2023 21:16
Operator : MA/JU
Sample : 05268-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc