

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042855.D
 Acq On : 17 Nov 2023 21:53
 Operator : MA/JU
 Sample : 05268-13
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042855.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	29	31	36	rBV4	4295	5693	0.50%	0.066%
2	3.628	105	109	119	rBV2	18453	40334	3.56%	0.467%
3	4.352	231	232	234	rBV2	1771	1847	0.16%	0.021%
4	4.634	277	280	281	rBV3	1409	1286	0.11%	0.015%
5	4.693	288	290	294	rVB4	2691	2075	0.18%	0.024%
6	4.722	294	295	298	rBV3	1662	1738	0.15%	0.020%
7	5.075	353	355	358	rVB3	1384	1295	0.11%	0.015%
8	5.469	418	422	423	rBV4	1017	1169	0.10%	0.014%
9	5.540	432	434	438	rBV4	908	1363	0.12%	0.016%
10	5.687	458	459	464	rBV5	1373	2248	0.20%	0.026%
11	6.546	603	605	607	rBV3	1610	1260	0.11%	0.015%
12	6.887	661	663	666	rBV3	1455	1450	0.13%	0.017%
13	6.998	676	682	694	rBV2	18141	48034	4.24%	0.556%
14	7.169	705	711	723	rBV	117509	211319	18.63%	2.446%
15	7.340	734	740	756	rBV	106306	204450	18.03%	2.367%
16	7.822	814	822	840	rBV	99310	191165	16.86%	2.213%
17	8.004	851	853	858	rVB5	1173	1194	0.11%	0.014%
18	8.545	939	945	963	rBV2	52754	121624	10.72%	1.408%
19	9.022	1019	1026	1039	rBV	145418	279386	24.64%	3.234%
20	9.687	1136	1139	1141	rBV3	866	1195	0.11%	0.014%
21	9.734	1141	1147	1161	rVV	109981	219477	19.35%	2.541%
22	9.839	1163	1165	1168	rVB3	1484	1776	0.16%	0.021%
23	10.263	1231	1237	1259	rBV	116275	259769	22.91%	3.007%
24	10.404	1259	1261	1262	rVV2	2414	1869	0.16%	0.022%
25	10.422	1262	1264	1266	rVV3	1632	1353	0.12%	0.016%
26	10.492	1272	1276	1278	rVB3	1282	1998	0.18%	0.023%
27	10.516	1278	1280	1282	rBV2	1810	1588	0.14%	0.018%
28	10.634	1292	1300	1311	rBV	136643	244816	21.59%	2.834%
29	10.810	1323	1330	1349	rBV	89123	237851	20.97%	2.754%
30	10.986	1358	1360	1363	rVB4	1843	1358	0.12%	0.016%
31	11.192	1394	1395	1399	rBV4	940	1152	0.10%	0.013%
32	11.622	1466	1468	1471	rBV3	976	1190	0.10%	0.014%
33	11.698	1474	1481	1486	rVV4	1778	3551	0.31%	0.041%
34	12.522	1617	1621	1626	rVB4	889	1644	0.14%	0.019%
35	13.310	1752	1755	1756	rBV	1452	1263	0.11%	0.015%
36	13.327	1756	1758	1762	rVB4	1595	1727	0.15%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042855.D
 Acq On : 17 Nov 2023 21:53
 Operator : MA/JU
 Sample : 05268-13
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	13.898	1849	1855	1866	rBV	351547	493180	43.49%	5.709%
38	13.986	1869	1870	1873	rVB3	1332	1229	0.11%	0.014%
39	14.174	1895	1902	1912	rBV	362924	542240	47.81%	6.277%
40	14.474	1947	1953	1962	rBV	200060	298588	26.33%	3.457%
41	15.469	2116	2122	2137	rBV	472485	701368	61.85%	8.119%
42	15.621	2143	2148	2163	rBV	110497	201547	17.77%	2.333%
43	15.745	2168	2169	2175	rVB3	1335	1697	0.15%	0.020%
44	17.227	2415	2421	2432	rBV	239210	342300	30.18%	3.963%
45	17.327	2432	2438	2454	rVV	530522	812520	71.65%	9.406%
46	17.580	2478	2481	2486	rVV5	1073	1725	0.15%	0.020%
47	17.827	2519	2523	2525	rVB3	775	1137	0.10%	0.013%
48	17.862	2525	2529	2531	rBV4	1499	1661	0.15%	0.019%
49	18.015	2554	2555	2559	rBV3	869	1202	0.11%	0.014%
50	18.080	2562	2566	2574	rBV3	16388	27470	2.42%	0.318%
51	18.180	2580	2583	2586	rBV3	1495	1641	0.14%	0.019%
52	19.186	2751	2754	2759	rVB4	4096	5046	0.44%	0.058%
53	19.262	2763	2767	2773	rBV3	3508	5038	0.44%	0.058%
54	19.368	2779	2785	2793	rBV3	14407	27252	2.40%	0.315%
55	19.498	2805	2807	2810	rBV4	1816	2283	0.20%	0.026%
56	19.621	2823	2828	2839	rBV	777112	1060388	93.50%	12.276%
57	19.951	2882	2884	2886	rBV3	1813	1840	0.16%	0.021%
58	20.086	2905	2907	2908	rBV	2469	1532	0.14%	0.018%
59	20.103	2908	2910	2911	rBV2	2571	2146	0.19%	0.025%
60	21.415	3128	3133	3144	rBV	261840	390835	34.46%	4.525%
61	23.621	3501	3508	3522	rBV	568016	1134055	100.00%	13.129%
62	23.774	3527	3534	3549	rVB	220657	475659	41.94%	5.507%




Sum of corrected areas: 8638086

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042855.D
Acq On : 17 Nov 2023 21:53
Operator : MA/JU
Sample : 05268-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

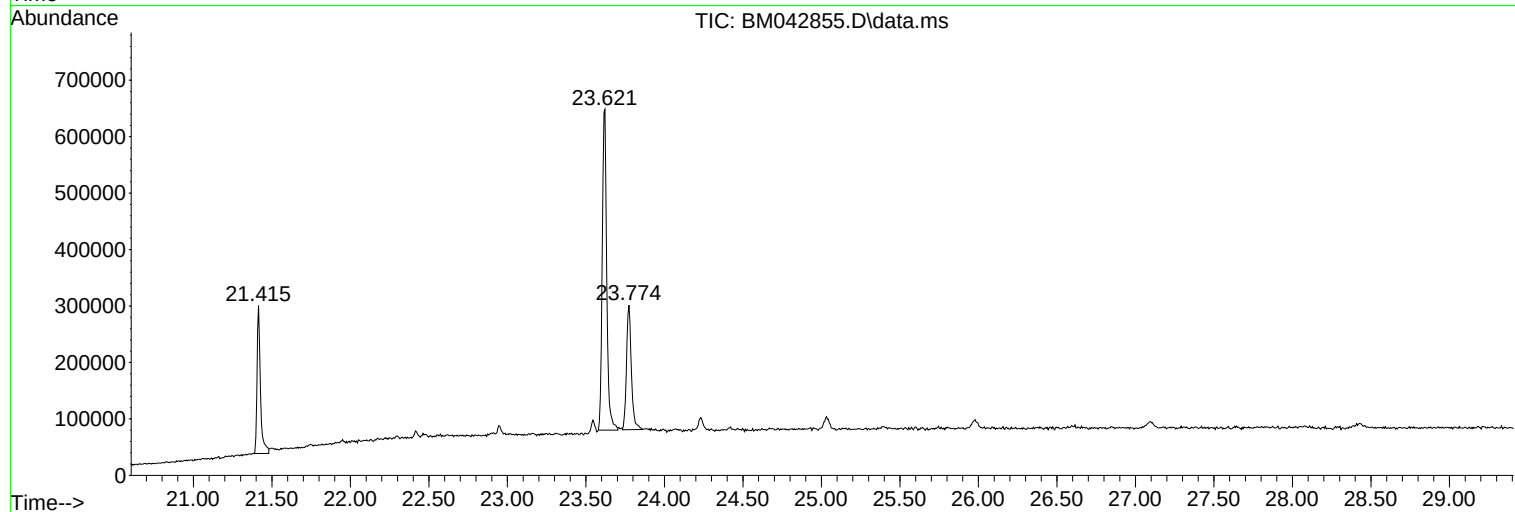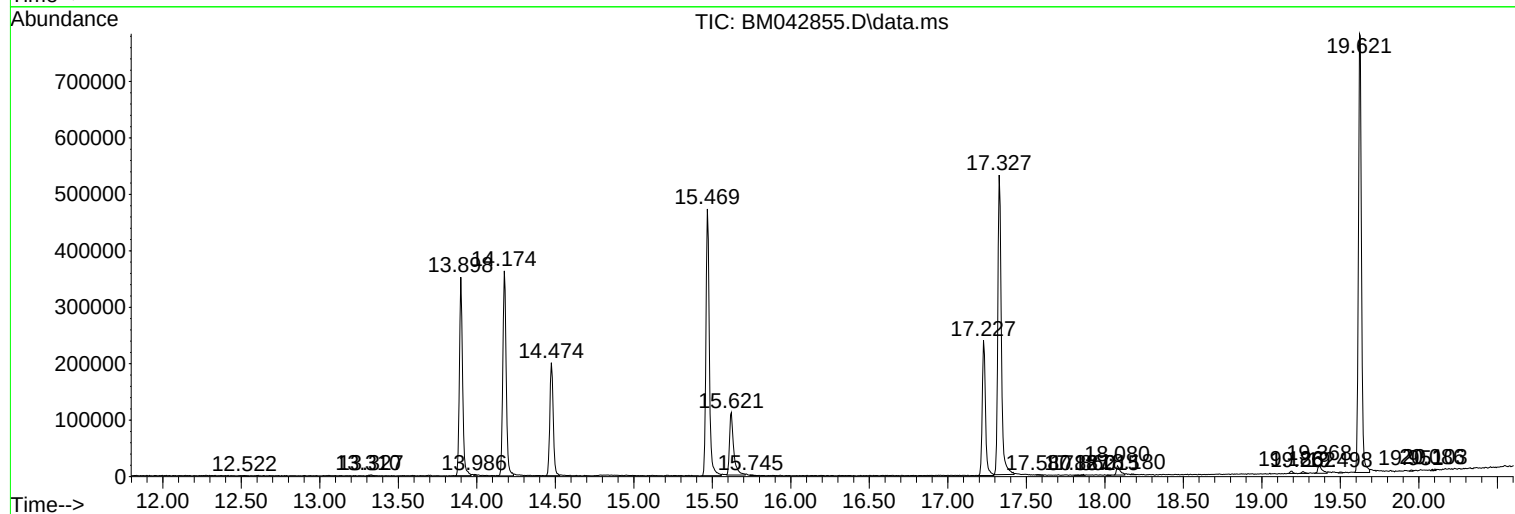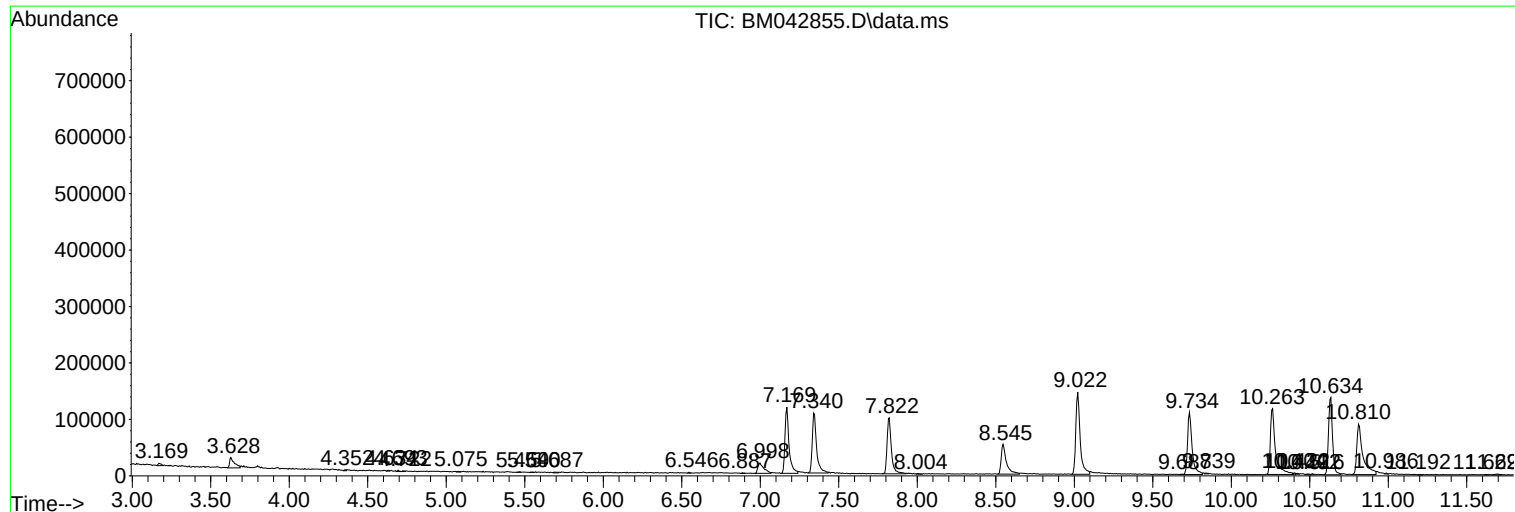

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042855.D
Acq On : 17 Nov 2023 21:53
Operator : MA/JU
Sample : 05268-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042855.D
Acq On : 17 Nov 2023 21:53
Operator : MA/JU
Sample : 05268-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc