

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042856.D
 Acq On : 17 Nov 2023 22:29
 Operator : MA/JU
 Sample : 05268-14
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042856.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	30	32	38	rVB4	7615	9428	0.92%	0.114%
2	3.622	105	108	124	rBV	29866	65921	6.41%	0.797%
3	4.493	254	256	259	rVB3	1694	1665	0.16%	0.020%
4	4.734	296	297	300	rVB3	1687	1196	0.12%	0.014%
5	5.540	431	434	436	rBV3	1481	1865	0.18%	0.023%
6	5.581	440	441	444	rVB2	1603	1077	0.10%	0.013%
7	5.934	499	501	503	rBV3	994	1092	0.11%	0.013%
8	6.187	542	544	546	rBV3	1155	1098	0.11%	0.013%
9	6.463	587	591	594	rBV5	934	1221	0.12%	0.015%
10	6.998	676	682	694	rVV	21456	58635	5.70%	0.709%
11	7.169	705	711	726	rBV	107517	196363	19.10%	2.373%
12	7.339	735	740	757	rBV	110391	211021	20.53%	2.550%
13	7.822	815	822	833	rBV2	98765	189993	18.48%	2.296%
14	7.910	835	837	841	rVV3	1700	2209	0.21%	0.027%
15	7.957	841	845	847	rVB4	988	1274	0.12%	0.015%
16	8.545	939	945	958	rBV	62677	133603	13.00%	1.615%
17	8.939	1009	1012	1015	rBV5	920	1271	0.12%	0.015%
18	9.022	1020	1026	1042	rBV	131894	262400	25.52%	3.171%
19	9.692	1135	1140	1141	rBV4	955	1428	0.14%	0.017%
20	9.733	1141	1147	1161	rVV2	104953	204017	19.84%	2.466%
21	10.175	1219	1222	1226	rBV4	836	1603	0.16%	0.019%
22	10.263	1231	1237	1255	rBV	115084	255085	24.81%	3.083%
23	10.633	1292	1300	1306	rBV	139040	244885	23.82%	2.960%
24	10.680	1306	1308	1317	rVB2	10854	18197	1.77%	0.220%
25	10.810	1323	1330	1354	rBV2	110243	289006	28.11%	3.493%
26	11.192	1390	1395	1397	rVV4	892	1234	0.12%	0.015%
27	11.345	1417	1421	1424	rBV2	1095	1610	0.16%	0.019%
28	11.692	1476	1480	1484	rVB4	2766	3965	0.39%	0.048%
29	12.527	1618	1622	1627	rBV3	1383	2016	0.20%	0.024%
30	13.321	1754	1757	1760	rBV3	2034	2634	0.26%	0.032%
31	13.698	1818	1821	1824	rBV2	988	1259	0.12%	0.015%
32	13.898	1849	1855	1869	rBV	335150	462622	45.00%	5.591%
33	14.174	1896	1902	1917	rBV	338277	501293	48.76%	6.059%
34	14.474	1947	1953	1961	rBV	206117	302083	29.38%	3.651%
35	14.539	1961	1964	1970	rVB2	4137	6411	0.62%	0.077%
36	14.792	2002	2007	2011	rBV5	2582	5678	0.55%	0.069%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042856.D
 Acq On : 17 Nov 2023 22:29
 Operator : MA/JU
 Sample : 05268-14
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	14.904	2021	2026	2030	rBV5	1380	2485	0.24%	0.030%
38	15.468	2116	2122	2137	rBV	454707	654032	63.62%	7.905%
39	15.562	2137	2138	2141	rVV3	2015	2004	0.19%	0.024%
40	15.621	2143	2148	2164	rVV	95316	175617	17.08%	2.122%
41	16.504	2296	2298	2303	rVB3	1045	1560	0.15%	0.019%
42	17.227	2416	2421	2432	rBV	238147	350587	34.10%	4.237%
43	17.327	2432	2438	2453	rVV	473145	727343	70.75%	8.791%
44	17.492	2464	2466	2470	rVB4	991	1106	0.11%	0.013%
45	17.792	2514	2517	2519	rBV4	866	1069	0.10%	0.013%
46	18.092	2564	2568	2571	rBV4	3981	6880	0.67%	0.083%
47	18.398	2618	2620	2625	rVV3	1159	1306	0.13%	0.016%
48	18.527	2639	2642	2643	rBV2	1240	1142	0.11%	0.014%
49	18.568	2648	2649	2652	rVB3	1318	1276	0.12%	0.015%
50	18.651	2659	2663	2664	rBV3	1044	1213	0.12%	0.015%
51	19.109	2739	2741	2743	rVB3	1470	1346	0.13%	0.016%
52	19.145	2743	2747	2748	rBV3	1390	1256	0.12%	0.015%
53	19.192	2751	2755	2759	rVB6	4246	6475	0.63%	0.078%
54	19.262	2765	2767	2769	rBV3	3686	3375	0.33%	0.041%
55	19.374	2782	2786	2790	rBV6	2614	4093	0.40%	0.049%
56	19.462	2799	2801	2804	rBV4	1466	1486	0.14%	0.018%
57	19.498	2804	2807	2810	rBV4	2145	3029	0.29%	0.037%
58	19.550	2814	2816	2817	rBV2	1237	1062	0.10%	0.013%
59	19.627	2823	2829	2843	rBV	694544	944264	91.85%	11.412%
60	19.850	2865	2867	2868	rVB2	1732	1117	0.11%	0.013%
61	19.868	2868	2870	2873	rBV4	1569	1774	0.17%	0.021%
62	19.956	2884	2885	2888	rBV3	2004	1670	0.16%	0.020%
63	20.009	2891	2894	2897	rBV4	2618	3442	0.33%	0.042%
64	21.415	3128	3133	3145	rBV	258070	397908	38.70%	4.809%
65	23.544	3491	3495	3500	rVB3	27433	41517	4.04%	0.502%
66	23.615	3500	3507	3522	rBV2	501001	1028097	100.00%	12.425%
67	23.774	3527	3534	3548	rVB	209315	458238	44.57%	5.538%




Sum of corrected areas: 8274127

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042856.D
Acq On : 17 Nov 2023 22:29
Operator : MA/JU
Sample : 05268-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

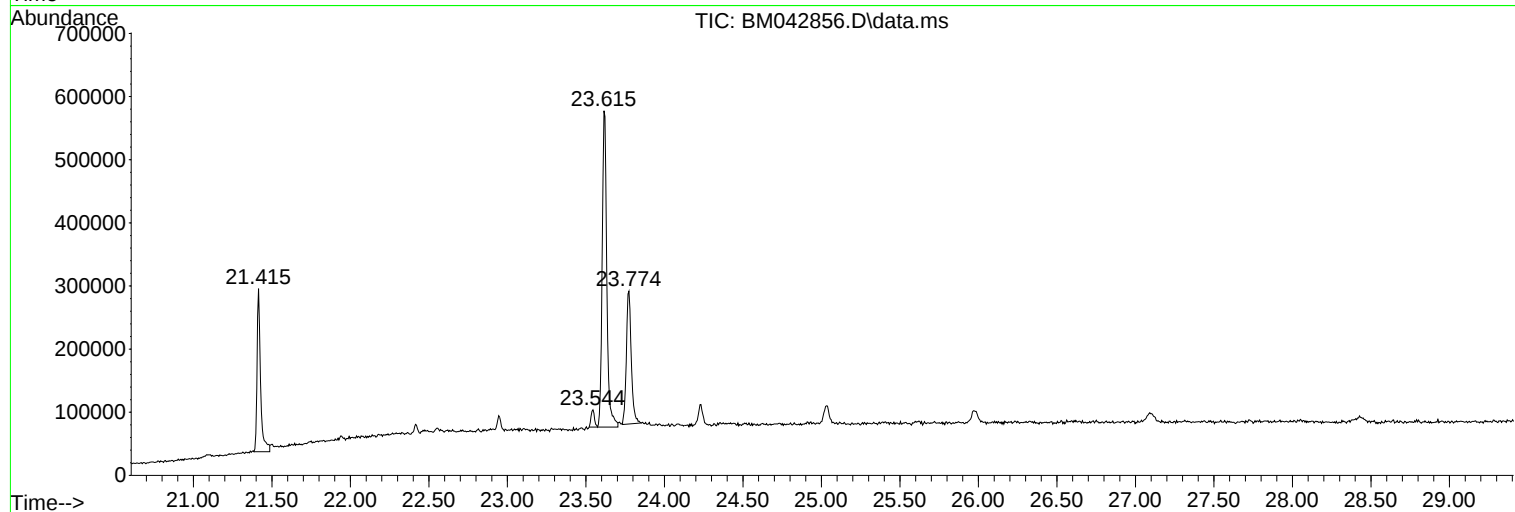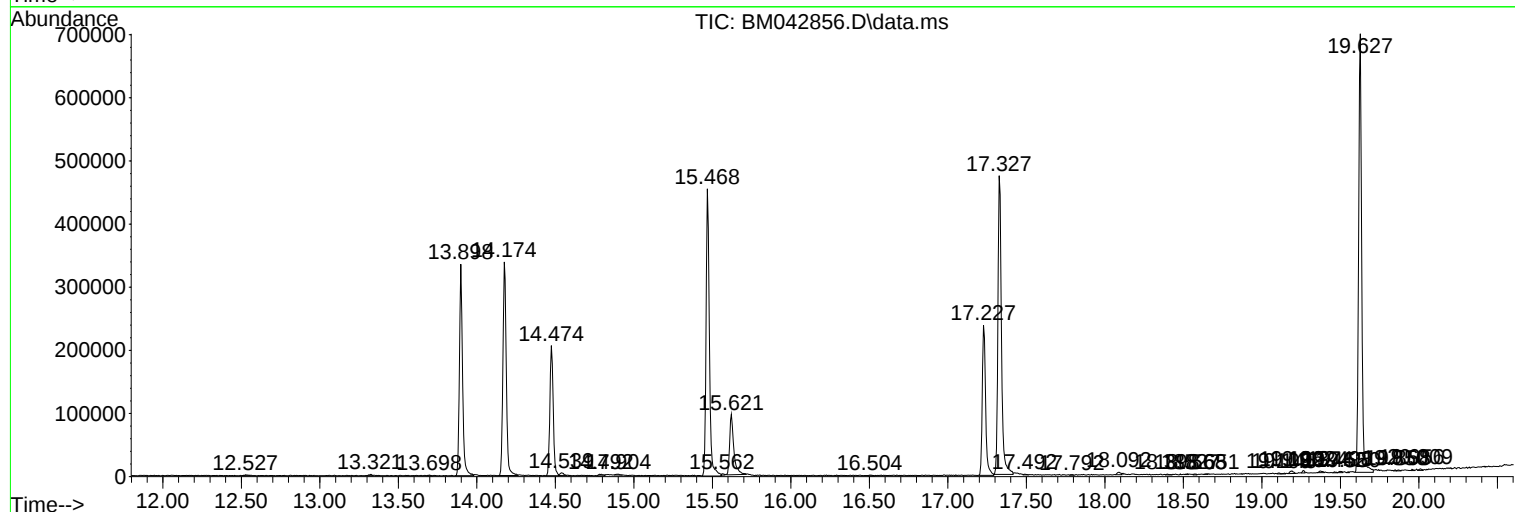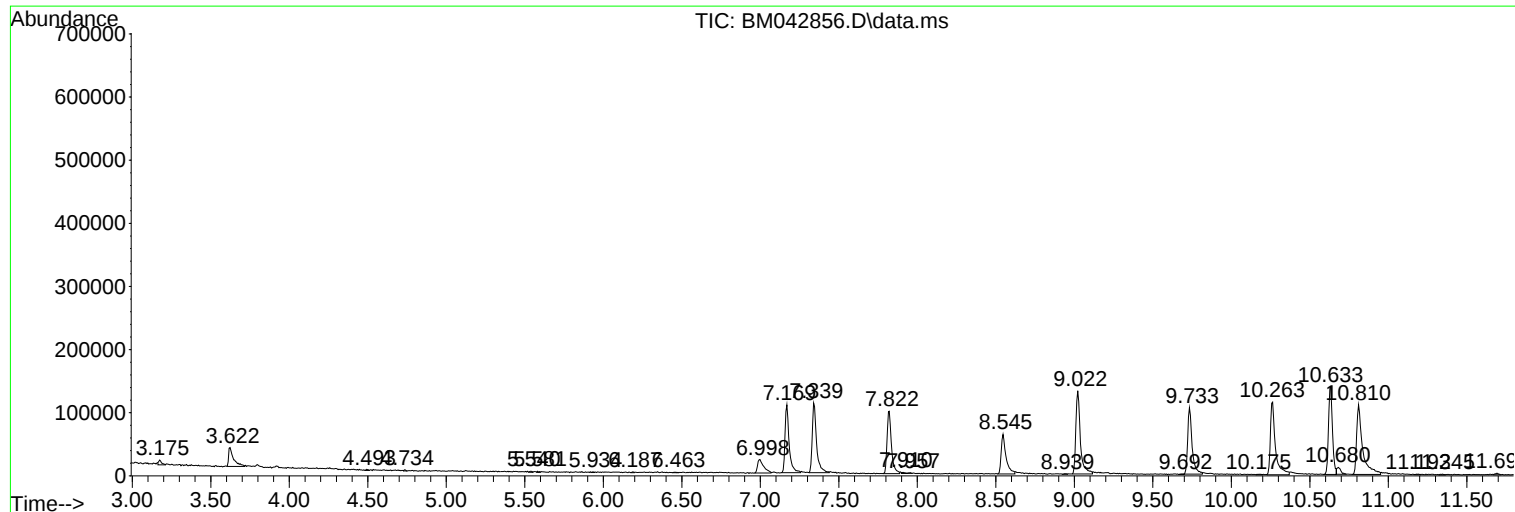

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042856.D
Acq On : 17 Nov 2023 22:29
Operator : MA/JU
Sample : 05268-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042856.D
Acq On : 17 Nov 2023 22:29
Operator : MA/JU
Sample : 05268-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc