

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042857.D
 Acq On : 17 Nov 2023 23:06
 Operator : MA/JU
 Sample : 05268-18
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKE6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042857.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	37	rVB2	6642	8156	0.74%	0.088%
2	3.622	105	108	116	rBV	22438	43364	3.95%	0.469%
3	6.140	533	536	537	rBV3	1381	1271	0.12%	0.014%
4	6.546	603	605	608	rBV3	1230	1224	0.11%	0.013%
5	6.593	611	613	616	rVB4	1312	1548	0.14%	0.017%
6	6.840	652	655	657	rBV3	1843	1567	0.14%	0.017%
7	6.993	673	681	693	rBV3	22951	63396	5.77%	0.685%
8	7.169	705	711	726	rBV	128251	236306	21.51%	2.555%
9	7.340	734	740	749	rBV	127235	228566	20.80%	2.471%
10	7.816	816	821	836	rBV	116167	214777	19.55%	2.322%
11	8.222	886	890	893	rBV4	860	1317	0.12%	0.014%
12	8.546	939	945	958	rBV2	62109	135259	12.31%	1.463%
13	8.793	986	987	991	rBV3	1195	1495	0.14%	0.016%
14	9.022	1018	1026	1045	rBV	166674	324509	29.53%	3.509%
15	9.734	1140	1147	1162	rBV	132816	257532	23.44%	2.785%
16	10.257	1230	1236	1255	rBV	140704	301379	27.43%	3.259%
17	10.569	1287	1289	1292	rVB2	1148	1277	0.12%	0.014%
18	10.628	1292	1299	1309	rBV	161191	288094	26.22%	3.115%
19	10.810	1324	1330	1350	rBV	82907	223693	20.36%	2.419%
20	10.957	1354	1355	1357	rVB2	2325	1446	0.13%	0.016%
21	11.034	1366	1368	1373	rVB4	1157	1135	0.10%	0.012%
22	11.157	1385	1389	1392	rVB5	1230	1289	0.12%	0.014%
23	11.375	1423	1426	1431	rVB4	1049	2048	0.19%	0.022%
24	13.322	1753	1757	1762	rVB5	1756	3025	0.28%	0.033%
25	13.439	1773	1777	1780	rBV3	849	1230	0.11%	0.013%
26	13.898	1849	1855	1869	rBV	385017	542962	49.41%	5.871%
27	13.992	1869	1871	1873	rVV3	2013	2020	0.18%	0.022%
28	14.039	1877	1879	1884	rVB3	851	1126	0.10%	0.012%
29	14.175	1896	1902	1914	rBV2	419802	596481	54.28%	6.450%
30	14.475	1947	1953	1963	rBV	240138	345138	31.41%	3.732%
31	14.710	1990	1993	1997	rVB3	682	1108	0.10%	0.012%
32	14.798	2003	2008	2011	rBV4	2274	4878	0.44%	0.053%
33	14.839	2014	2015	2019	rVV2	1426	1883	0.17%	0.020%
34	14.892	2021	2024	2027	rVB4	1082	1684	0.15%	0.018%
35	15.104	2058	2060	2064	rBV3	970	1289	0.12%	0.014%
36	15.469	2116	2122	2137	rBV	518432	765405	69.66%	8.276%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042857.D
 Acq On : 17 Nov 2023 23:06
 Operator : MA/JU
 Sample : 05268-18
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKE6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	15.622	2143	2148	2163	rBV	123419	220878	20.10%	2.388%
38	15.716	2163	2164	2169	rVB4	3294	2240	0.20%	0.024%
39	16.833	2351	2354	2356	rBV3	904	1106	0.10%	0.012%
40	17.227	2416	2421	2433	rBV	278359	397795	36.20%	4.301%
41	17.327	2433	2438	2451	rBV	574838	834005	75.90%	9.018%
42	17.474	2461	2463	2468	rVB4	1584	1757	0.16%	0.019%
43	18.086	2563	2567	2569	rBV3	2927	3801	0.35%	0.041%
44	18.851	2694	2697	2698	rBV3	1280	1352	0.12%	0.015%
45	19.021	2722	2726	2728	rBV3	1408	1827	0.17%	0.020%
46	19.186	2750	2754	2759	rBV5	4518	6736	0.61%	0.073%
47	19.268	2764	2768	2771	rVB	3597	4684	0.43%	0.051%
48	19.374	2783	2786	2788	rBV4	1929	2143	0.20%	0.023%
49	19.510	2804	2809	2810	rBV4	2594	3105	0.28%	0.034%
50	19.627	2823	2829	2841	rBV	791018	1071170	97.48%	11.582%
51	21.415	3128	3133	3146	rBV	293204	442843	40.30%	4.788%
52	22.951	3390	3394	3397	rBV4	16732	23525	2.14%	0.254%
53	23.615	3501	3507	3524	rBV	565394	1098808	100.00%	11.881%
54	23.774	3527	3534	3547	rVB	242752	521749	47.48%	5.642%




Sum of corrected areas: 9248401

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042857.D
Acq On : 17 Nov 2023 23:06
Operator : MA/JU
Sample : 05268-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKE6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

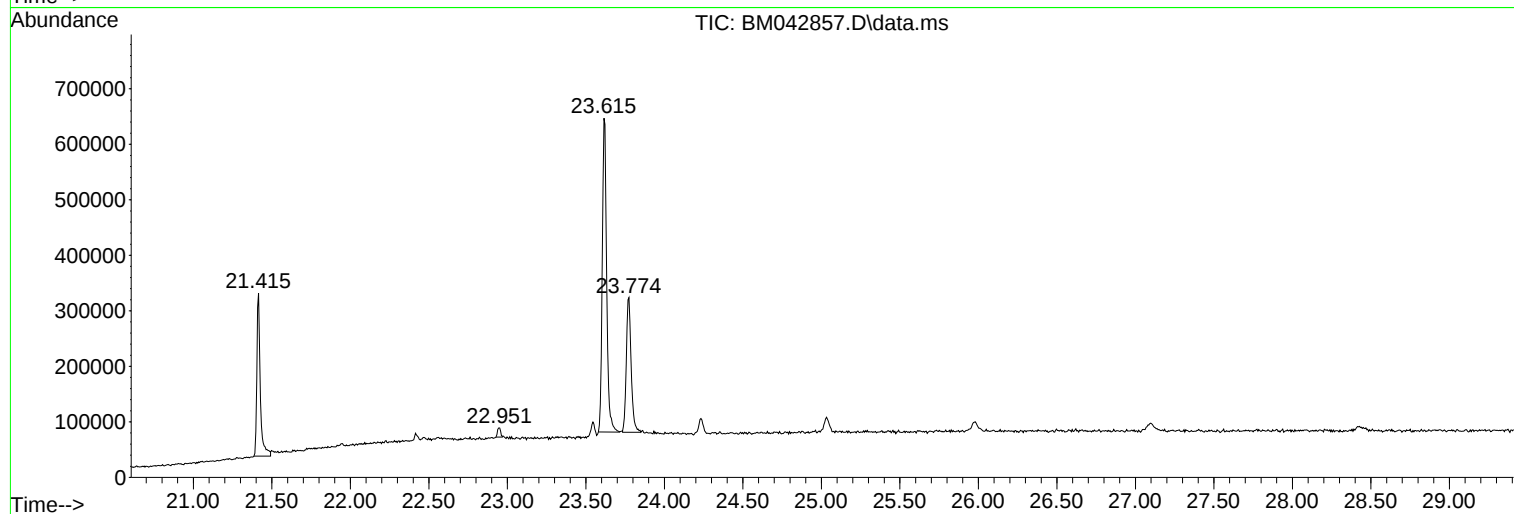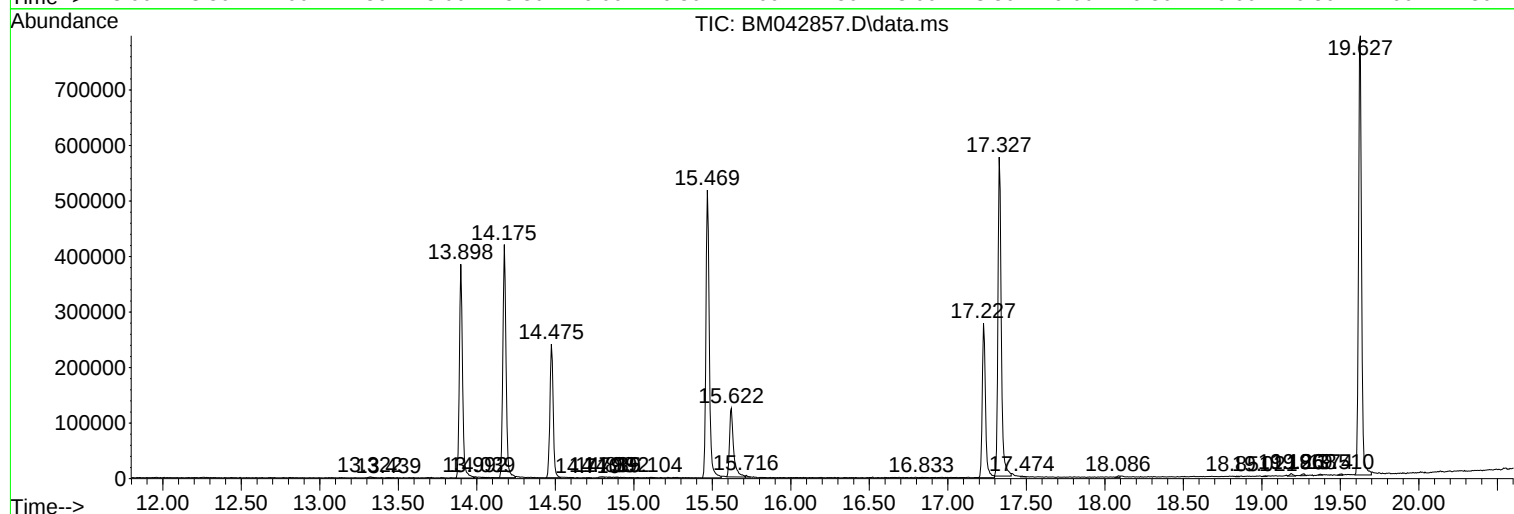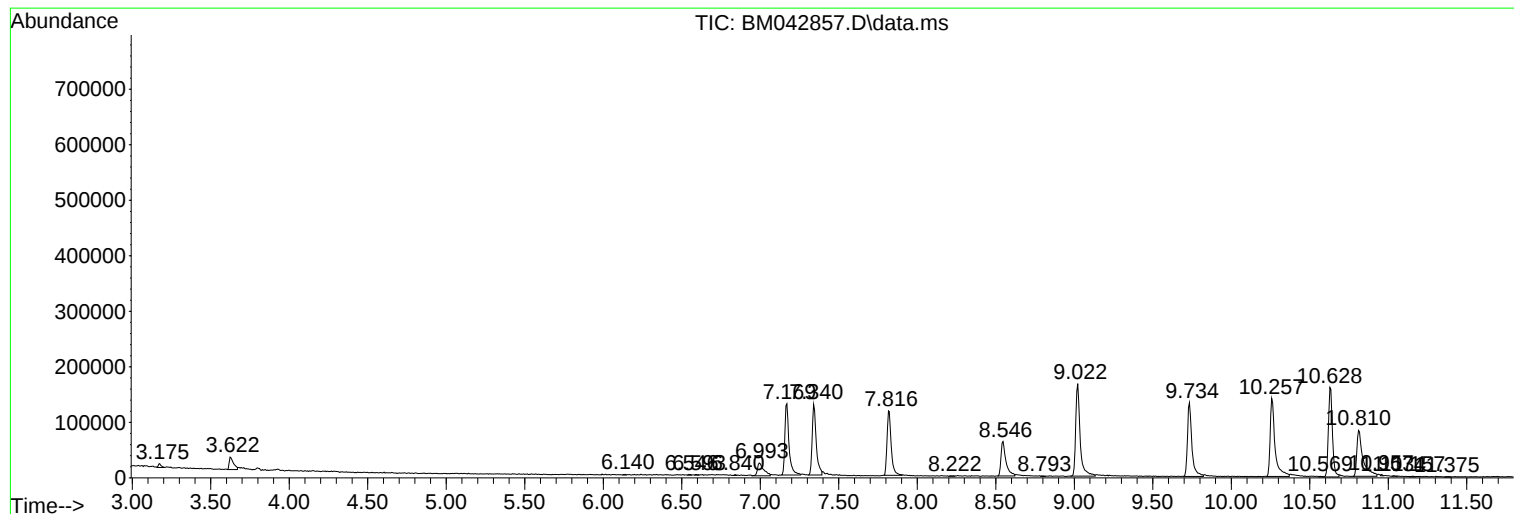

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042857.D
Acq On : 17 Nov 2023 23:06
Operator : MA/JU
Sample : 05268-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKE6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042857.D
Acq On : 17 Nov 2023 23:06
Operator : MA/JU
Sample : 05268-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKE6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc