

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042859.D
 Acq On : 18 Nov 2023 00:19
 Operator : MA/JU
 Sample : 05226-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCG85

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042859.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	29	31	36	rVB4	7148	9117	0.95%	0.124%
2	3.622	105	108	115	rBV	26957	45726	4.79%	0.622%
3	3.922	157	159	161	rVB3	3237	2484	0.26%	0.034%
4	5.604	441	445	448	rVB6	1624	2259	0.24%	0.031%
5	5.934	499	501	505	rVB5	1568	1622	0.17%	0.022%
6	5.969	505	507	509	rBV4	904	973	0.10%	0.013%
7	6.510	597	599	601	rVB3	1259	1013	0.11%	0.014%
8	6.546	601	605	607	rBV5	1135	1749	0.18%	0.024%
9	6.728	634	636	639	rVB3	1403	1222	0.13%	0.017%
10	6.763	640	642	646	rVV5	1079	1153	0.12%	0.016%
11	6.810	648	650	652	rBV2	864	998	0.10%	0.014%
12	6.893	662	664	669	rVB4	1288	1869	0.20%	0.025%
13	6.998	676	682	694	rBV3	10687	33407	3.50%	0.454%
14	7.169	706	711	729	rBV	91729	172466	18.05%	2.346%
15	7.345	735	741	755	rBV	86207	168057	17.59%	2.286%
16	7.440	755	757	760	rVB3	2471	2036	0.21%	0.028%
17	7.822	816	822	839	rBV	84001	163078	17.07%	2.218%
18	8.251	891	895	898	rBV4	761	1140	0.12%	0.016%
19	8.545	939	945	956	rBV	40794	92508	9.68%	1.258%
20	8.887	1002	1003	1009	rBV5	658	1090	0.11%	0.015%
21	9.022	1019	1026	1047	rBV	115909	239534	25.07%	3.258%
22	9.198	1053	1056	1062	rVB6	1643	2661	0.28%	0.036%
23	9.245	1062	1064	1068	rVB5	1046	1526	0.16%	0.021%
24	9.734	1141	1147	1162	rBV3	89575	180076	18.85%	2.449%
25	9.869	1168	1170	1172	rVB3	1330	1196	0.13%	0.016%
26	10.022	1191	1196	1199	rVB4	937	1770	0.19%	0.024%
27	10.057	1199	1202	1204	rBV3	919	1063	0.11%	0.014%
28	10.181	1220	1223	1227	rBV4	816	1115	0.12%	0.015%
29	10.263	1230	1237	1252	rBV	93912	213650	22.36%	2.906%
30	10.634	1293	1300	1313	rBV	117046	206663	21.63%	2.811%
31	10.757	1319	1321	1325	rVB2	1393	1741	0.18%	0.024%
32	10.816	1325	1331	1348	rBV2	73114	204908	21.45%	2.787%
33	10.951	1352	1354	1358	rVB3	2152	2820	0.30%	0.038%
34	11.157	1386	1389	1396	rVB5	935	1457	0.15%	0.020%
35	11.339	1416	1420	1423	rVB2	969	1317	0.14%	0.018%
36	12.133	1552	1555	1557	rBV2	703	964	0.10%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042859.D
 Acq On : 18 Nov 2023 00:19
 Operator : MA/JU
 Sample : 05226-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCG85

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	13.322	1752	1757	1762	rBV3	2230	3633	0.38%	0.049%
38	13.898	1849	1855	1870	rBV	288910	427787	44.78%	5.818%
39	14.174	1896	1902	1918	rBV	309534	459738	48.12%	6.253%
40	14.474	1947	1953	1963	rBV	173868	258517	27.06%	3.516%
41	15.468	2116	2122	2133	rBV	404060	605027	63.33%	8.229%
42	15.563	2136	2138	2143	rVB4	1681	1751	0.18%	0.024%
43	15.621	2143	2148	2159	rBV2	94120	170052	17.80%	2.313%
44	16.868	2356	2360	2361	rBV2	826	1010	0.11%	0.014%
45	17.227	2415	2421	2433	rBV	202724	296828	31.07%	4.037%
46	17.327	2433	2438	2454	rVV	477602	716408	74.99%	9.743%
47	17.574	2479	2480	2485	rVB4	1019	1211	0.13%	0.016%
48	17.715	2502	2504	2507	rBV3	1017	1161	0.12%	0.016%
49	17.892	2530	2534	2535	rBV3	838	975	0.10%	0.013%
50	18.009	2552	2554	2556	rBV3	911	1062	0.11%	0.014%
51	18.033	2556	2558	2561	rVB3	1089	1078	0.11%	0.015%
52	18.092	2563	2568	2575	rBV5	5482	13706	1.43%	0.186%
53	18.527	2640	2642	2645	rVB3	1256	1215	0.13%	0.017%
54	18.562	2645	2648	2651	rBV2	1351	1323	0.14%	0.018%
55	18.709	2669	2673	2677	rBV3	1434	2567	0.27%	0.035%
56	19.109	2739	2741	2742	rBV2	1575	1097	0.11%	0.015%
57	19.192	2750	2755	2759	rBV6	3949	6188	0.65%	0.084%
58	19.262	2763	2767	2771	rBV3	3539	4170	0.44%	0.057%
59	19.374	2781	2786	2794	rBV9	4529	12351	1.29%	0.168%
60	19.474	2801	2803	2806	rVB4	1553	1047	0.11%	0.014%
61	19.504	2806	2808	2811	rBV4	1683	1576	0.16%	0.021%
62	19.545	2811	2815	2816	rBV2	1349	1434	0.15%	0.020%
63	19.627	2823	2829	2839	rBV	680359	909997	95.26%	12.376%
64	19.880	2871	2872	2875	rVB3	1982	1467	0.15%	0.020%
65	19.939	2880	2882	2884	rVB3	1828	1035	0.11%	0.014%
66	20.221	2928	2930	2931	rBV2	2550	1567	0.16%	0.021%
67	20.251	2931	2935	2937	rVV5	2420	3229	0.34%	0.044%
68	20.286	2939	2941	2943	rBV2	1961	1502	0.16%	0.020%
69	21.415	3128	3133	3144	rBV	214232	330843	34.63%	4.500%
70	23.615	3501	3507	3523	rBV2	472082	955316	100.00%	12.993%
71	23.774	3528	3534	3547	rVB	181499	388438	40.66%	5.283%




Sum of corrected areas: 7352734

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042859.D
Acq On : 18 Nov 2023 00:19
Operator : MA/JU
Sample : 05226-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG85

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

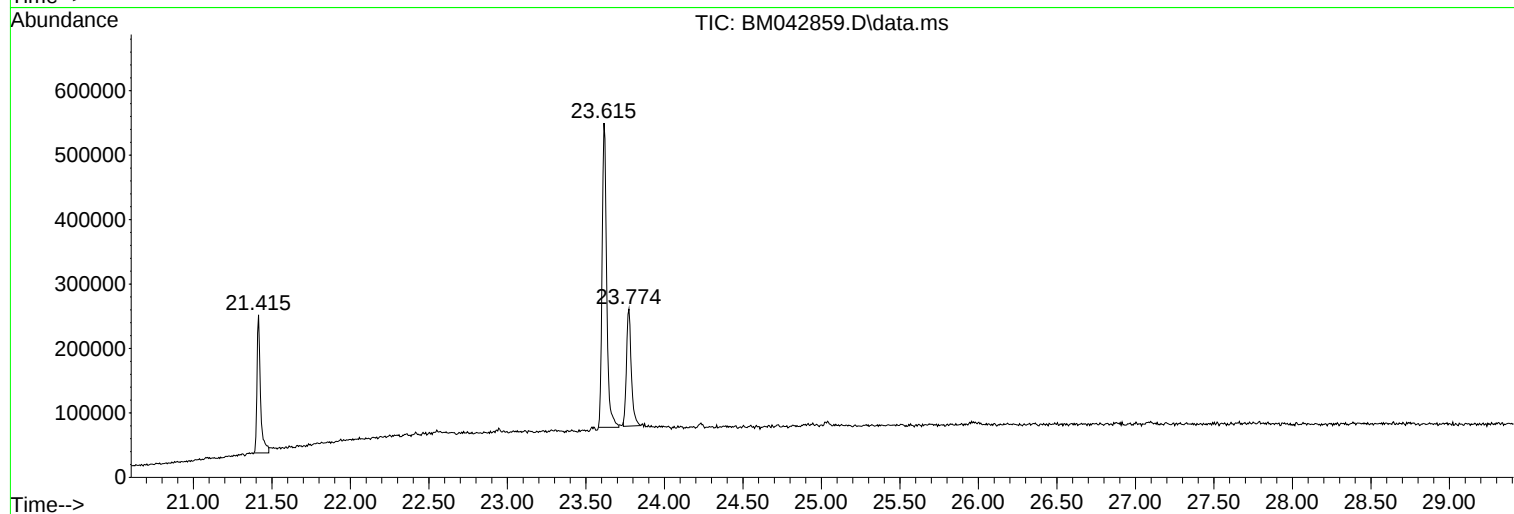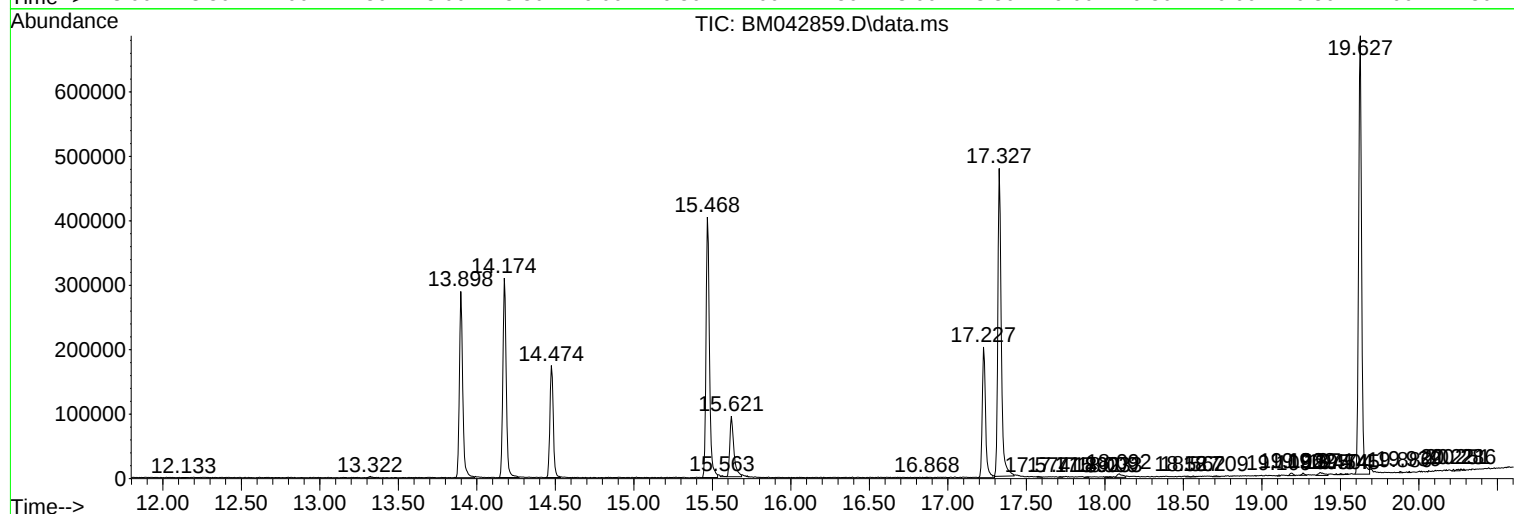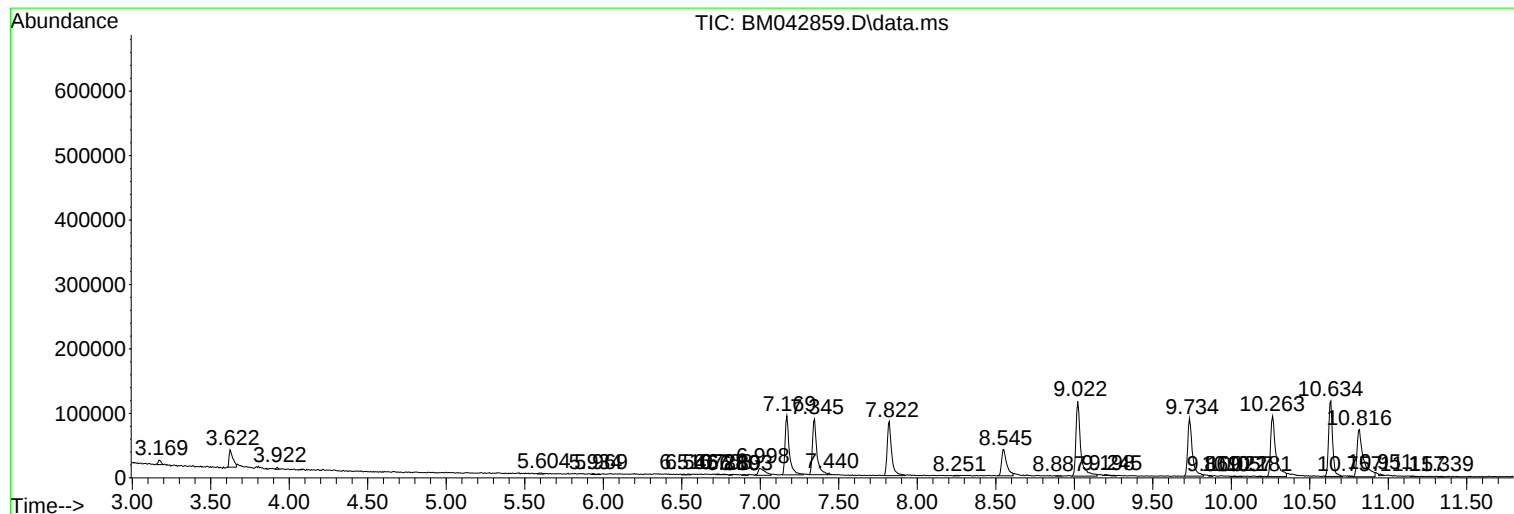

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042859.D
Acq On : 18 Nov 2023 00:19
Operator : MA/JU
Sample : 05226-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG85

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042859.D
Acq On : 18 Nov 2023 00:19
Operator : MA/JU
Sample : 05226-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG85

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc